

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092217\
 Data File : BF098697.D
 Acq On : 22 Sep 2017 13:57
 Operator : SJ/JU
 Sample : I5293-10 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-B-R-SIDE-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.139	516	519	526	rBV	95857	93008	7.70%	0.746%
2	5.534	582	586	589	rBV	669175	597345	49.44%	4.789%
3	6.533	752	756	760	rBV	784929	612304	50.67%	4.908%
4	6.686	778	782	786	rBV	753676	629149	52.07%	5.043%
5	6.928	819	823	826	rBV	1146339	909369	75.26%	7.290%
6	7.080	845	849	853	rVB	600701	467857	38.72%	3.751%
7	7.480	913	917	920	rBV	447838	335984	27.81%	2.693%
8	8.210	1037	1041	1044	rBV	1449969	1208328	100.00%	9.686%
9	9.280	1219	1223	1226	rBV	875590	670967	55.53%	5.379%
10	9.357	1233	1236	1239	rBV3	15012	14143	1.17%	0.113%
11	9.669	1287	1289	1293	rBV	69172	55965	4.63%	0.449%
12	9.821	1311	1315	1319	rBV	12809	14235	1.18%	0.114%
13	9.886	1322	1326	1329	rVB3	13848	15702	1.30%	0.126%
14	9.963	1335	1339	1343	rBV	1441405	1191119	98.58%	9.548%
15	9.992	1343	1344	1347	rVB	27994	20858	1.73%	0.167%
16	10.163	1368	1373	1377	rVB	16568	16201	1.34%	0.130%
17	10.386	1409	1411	1415	rVB	18642	14182	1.17%	0.114%
18	10.510	1428	1432	1435	rBV2	16092	15539	1.29%	0.125%
19	10.745	1468	1472	1477	rBV	352810	273382	22.62%	2.192%
20	10.857	1488	1491	1492	rBV	21254	16597	1.37%	0.133%
21	11.021	1515	1519	1521	rBV	37435	30667	2.54%	0.246%
22	11.221	1548	1553	1555	rBV2	22503	25510	2.11%	0.204%
23	11.339	1569	1573	1576	rVB2	15422	17980	1.49%	0.144%
24	11.398	1579	1583	1585	rBV2	18695	19811	1.64%	0.159%
25	11.451	1588	1592	1594	rVV	1170773	1006909	83.33%	8.072%
26	11.468	1594	1595	1598	rVV	147254	106042	8.78%	0.850%
27	11.521	1602	1604	1607	rVB	36042	26177	2.17%	0.210%
28	11.733	1637	1640	1645	rVB3	14043	15909	1.32%	0.128%
29	11.945	1674	1676	1679	rBV2	18145	22588	1.87%	0.181%
30	11.974	1679	1681	1685	rVB	30676	25995	2.15%	0.208%
31	12.063	1692	1696	1698	rBV2	34130	41140	3.40%	0.330%
32	12.080	1698	1699	1702	rVB	20551	14607	1.21%	0.117%
33	12.139	1706	1709	1714	rVB3	13595	15109	1.25%	0.121%
34	12.245	1724	1727	1728	rBV2	21521	17391	1.44%	0.139%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092217\
Data File : BF098697.D
Acq On : 22 Sep 2017 13:57
Operator : SJ/JU
Sample : I5293-10 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-B-R-SIDE-COMP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092117.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.268	1728	1731	1737	rVB6	11333	17526	1.45%	0.140%
36	12.498	1767	1770	1772	rBV	20953	21539	1.78%	0.173%
37	12.527	1772	1775	1778	rVV4	19956	22083	1.83%	0.177%
38	12.580	1781	1784	1790	rVB3	17944	16573	1.37%	0.133%
39	12.657	1794	1797	1801	rBV	289514	264333	21.88%	2.119%
40	12.698	1802	1804	1807	rBV2	21652	20445	1.69%	0.164%
41	12.886	1830	1836	1841	rBV	270823	305654	25.30%	2.450%
42	13.027	1857	1860	1868	rVB	593672	482873	39.96%	3.871%
43	13.110	1869	1874	1877	rBV5	22378	37803	3.13%	0.303%
44	13.198	1885	1889	1890	rBV4	16009	21894	1.81%	0.176%
45	13.215	1890	1892	1896	rVB	33801	31892	2.64%	0.256%
46	13.280	1901	1903	1905	rVV2	22783	17429	1.44%	0.140%
47	13.321	1907	1910	1912	rVV2	27447	26436	2.19%	0.212%
48	13.721	1975	1978	1982	rVB	25940	29754	2.46%	0.239%
49	13.862	2000	2002	2004	rBV	24254	18779	1.55%	0.151%
50	13.886	2004	2006	2009	rBV2	18771	22716	1.88%	0.182%
51	14.086	2033	2040	2043	rBV	1090923	1114575	92.24%	8.935%
52	14.109	2043	2044	2050	rVB	136787	96058	7.95%	0.770%
53	15.133	2215	2218	2222	rBV	108117	174475	14.44%	1.399%
54	15.445	2269	2271	2278	rVB	55486	69437	5.75%	0.557%
55	15.509	2279	2282	2286	rVV	85499	103997	8.61%	0.834%
56	15.580	2289	2294	2305	rVB	731595	1000158	82.77%	8.018%


Sum of corrected areas: 12474498

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092217\
Data File : BF098697.D
Acq On : 22 Sep 2017 13:57
Operator : SJ/JU
Sample : I5293-10 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-B-R-SIDE-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

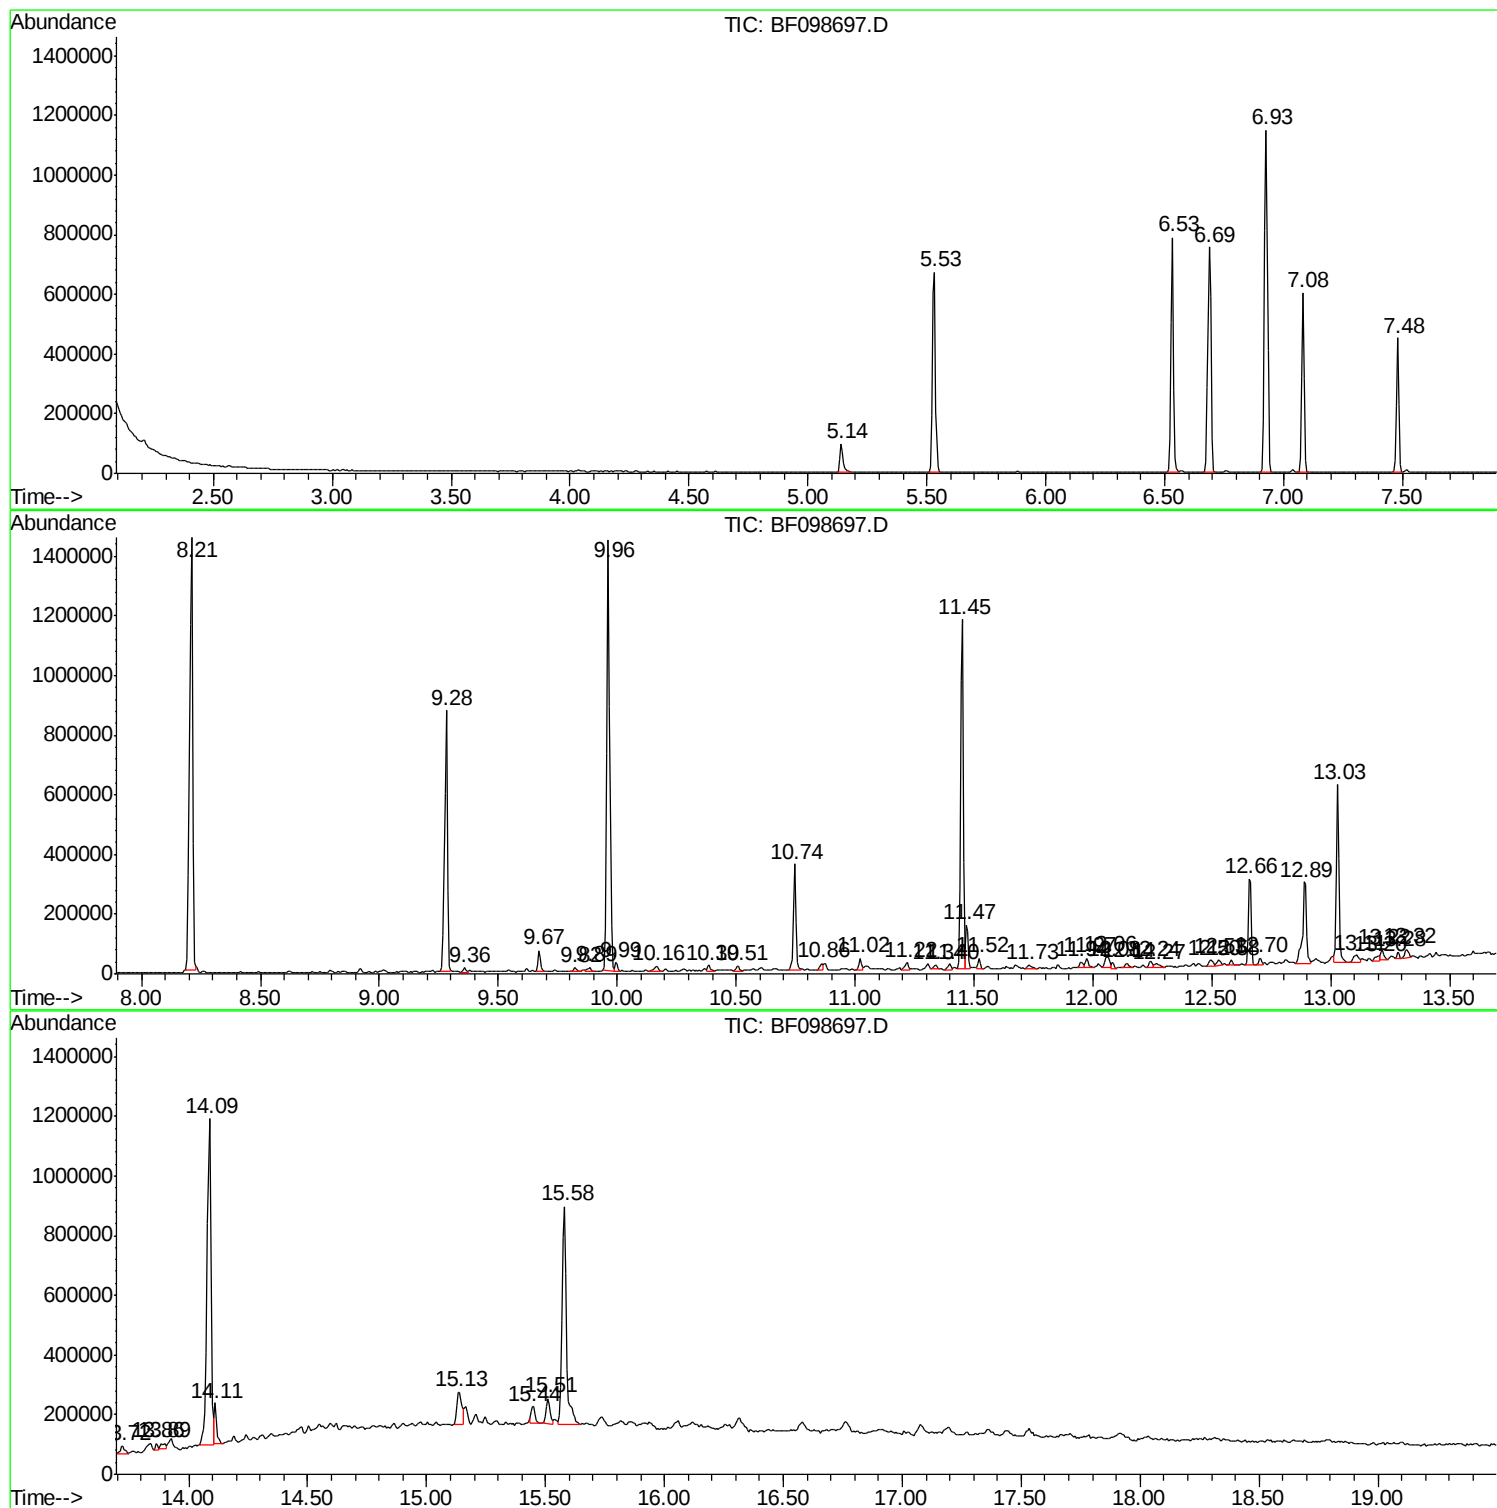

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092217\
Data File : BF098697.D
Acq On : 22 Sep 2017 13:57
Operator : SJ/JU
Sample : I5293-10 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-B-R-SIDE-COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.14	2.05 ng	93008	1,4-Dichlorobenzene-d4	6.93

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	38
3			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	28
4			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	22
5			4-Penten-2-one, 4-methyl-	98	C6H10O	003744-02-3	10

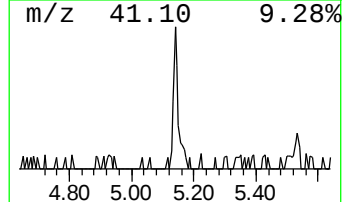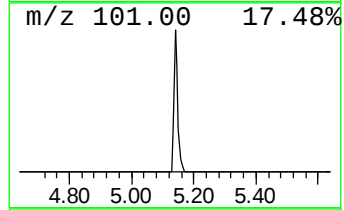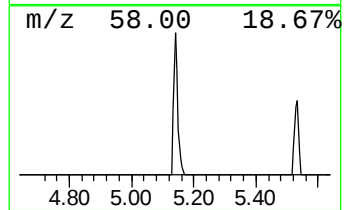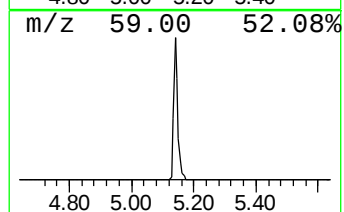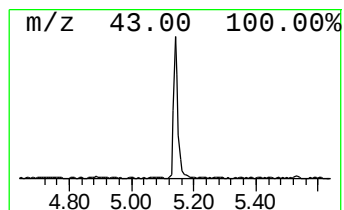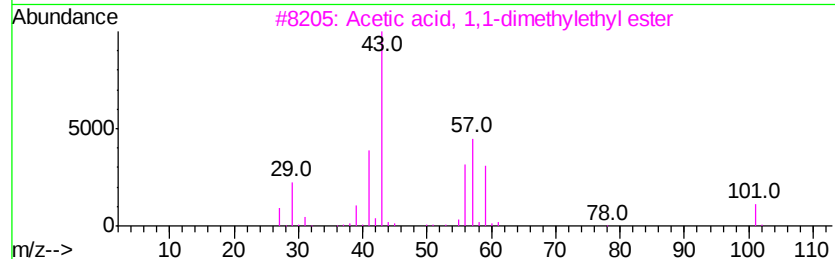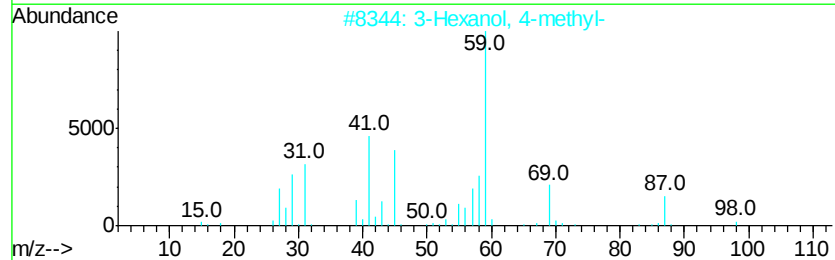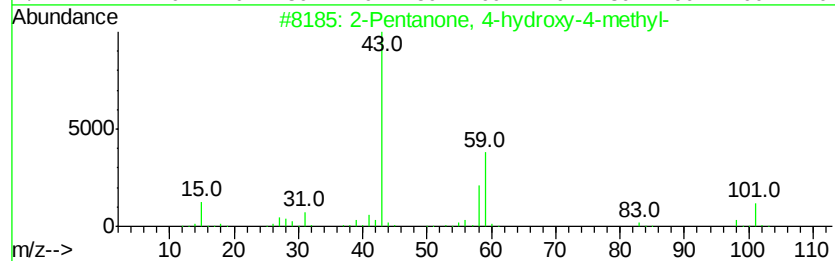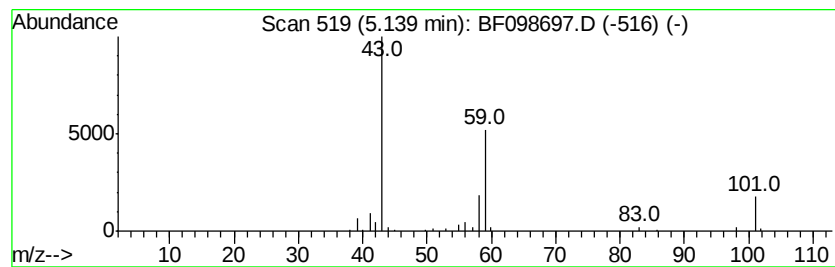

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092217\
Data File : BF098697.D
Acq On : 22 Sep 2017 13:57
Operator : SJ/JU
Sample : I5293-10 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-B-R-SIDE-COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.69 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.69	13.84 ng	629149	1,4-Dichlorobenzene-d4	6.93

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	10
2		Benzeneethanamine, .alpha.-methy...	223	C16H17N	002980-02-1	10
3		N-(-phenylisopropyl)benzalimine	223	C16H17N	1000379-01-3	10
4		Amphetaminil	250	C17H18N2	017590-01-1	10
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

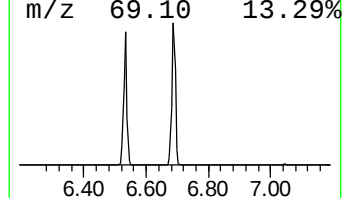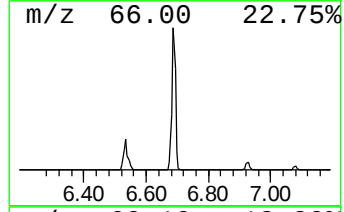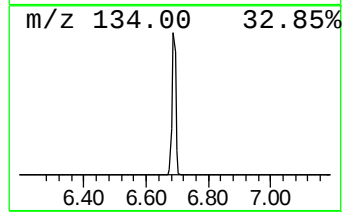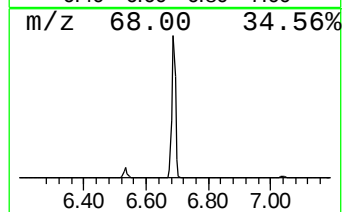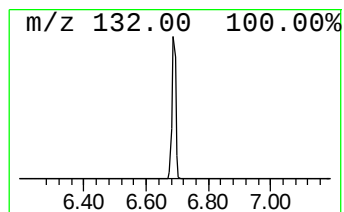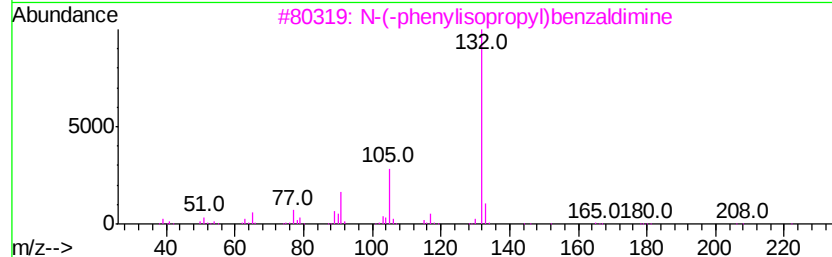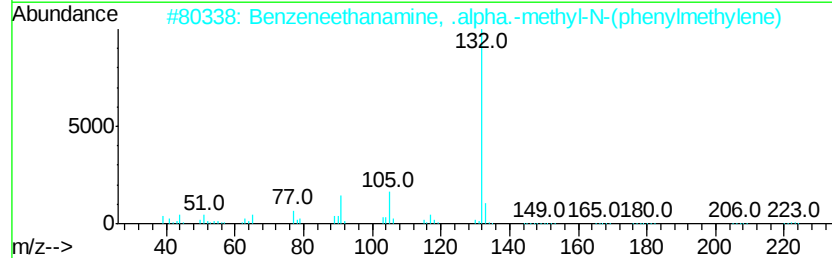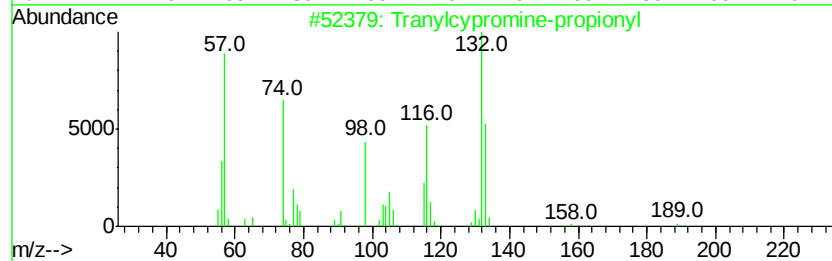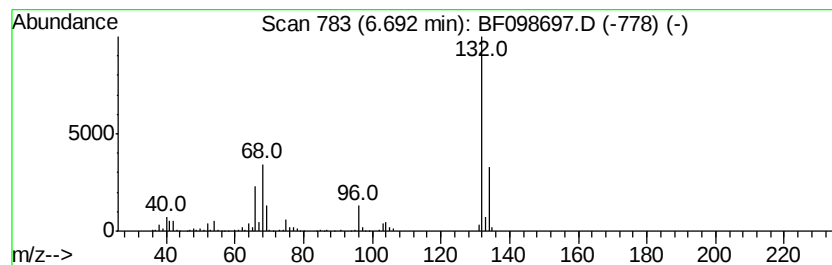

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092217\
Data File : BF098697.D
Acq On : 22 Sep 2017 13:57
Operator : SJ/JU
Sample : I5293-10 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-B-R-SIDE-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.14	2.0	ng	93008	1	6.93	909369	20.0
unknown6.69	6.69	13.8	ng	629149	1	6.93	909369	20.0