


Data Path : Z:\HPCHEM1\BNA F\Data\BF092217\
 Data File : BF098702.D
 Acq On : 22 Sep 2017 17:59
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 22 10:38:37 2017

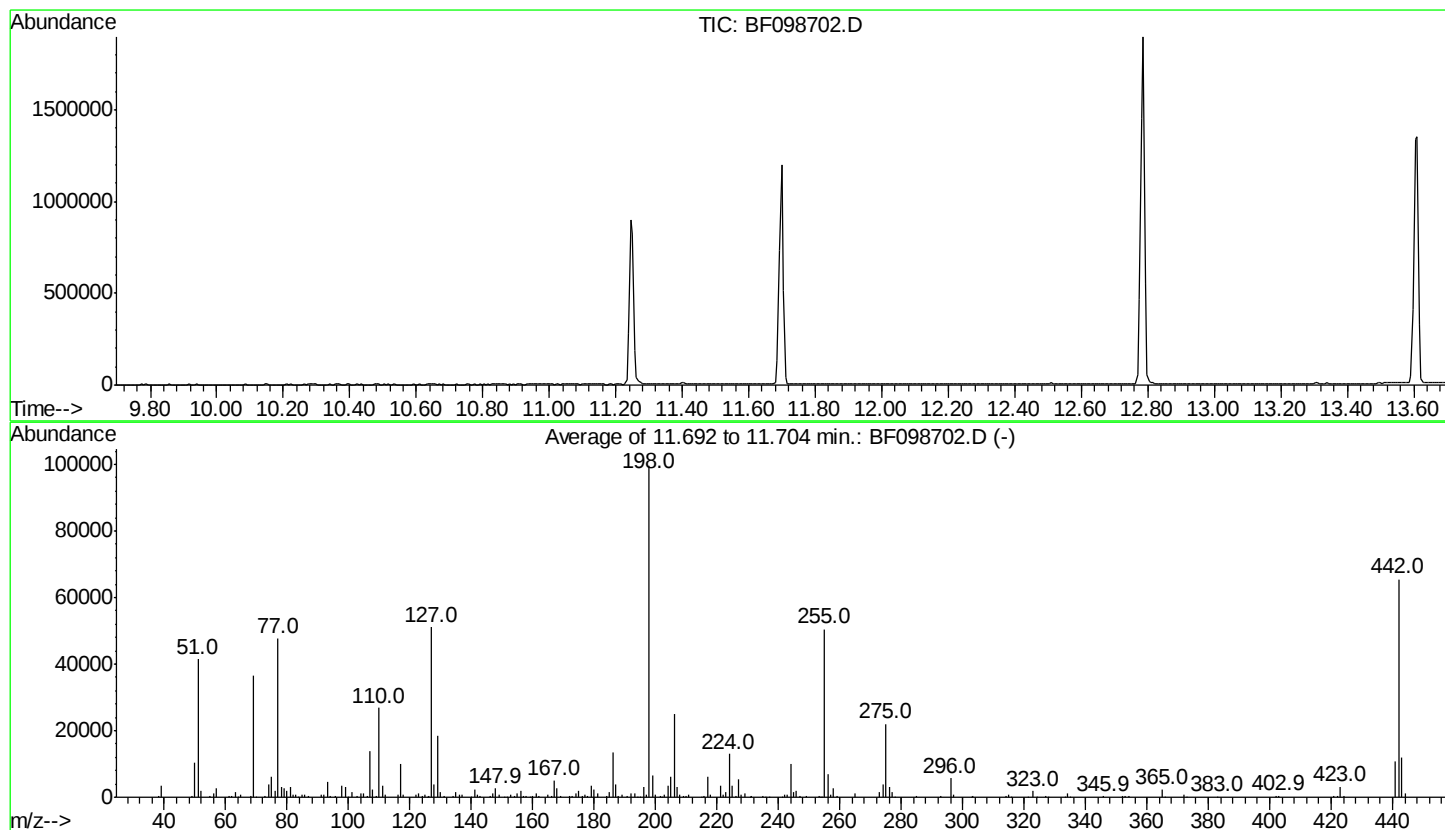

AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	41505	PASS
68	69	0.00	2	1.5	553	PASS
69	198	0.00	100	36.6	36483	PASS
70	69	0.00	2	0.3	105	PASS
127	198	10	80	51.2	50968	PASS
197	198	0.00	2	0.7	731	PASS
198	198	100	100	100.0	99605	PASS
199	198	5	9	6.5	6487	PASS
275	198	10	60	22.1	22040	PASS
365	198	1	100	2.2	2211	PASS
441	442	0.01	24	16.3	10711	PASS
442	198	50	100	65.8	65562	PASS
443	442	15	24	18.5	12098	PASS