

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092222\
 Data File : BF130384.D
 Acq On : 22 Sep 2022 19:52
 Operator : CG\JU
 Sample : N4753-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EO-01-092122

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.546	242	248	253	rBV2	6729	9895	1.30%	0.187%
2	5.251	534	538	548	rBV	174359	172172	22.68%	3.249%
3	6.293	712	715	733	rBV	156063	174275	22.96%	3.289%
4	6.651	773	776	780	rBV	696737	638728	84.13%	12.055%
5	7.216	869	872	877	rBV	122874	102408	13.49%	1.933%
6	7.940	990	995	998	rBV	861430	759171	100.00%	14.328%
7	8.363	1063	1067	1069	rBV2	10340	10363	1.37%	0.196%
8	8.534	1093	1096	1099	rBV	21656	16475	2.17%	0.311%
9	8.745	1128	1132	1137	rBV6	7216	11424	1.50%	0.216%
10	8.963	1166	1169	1172	rVB2	11596	9977	1.31%	0.188%
11	9.010	1174	1177	1184	rVV	244319	207067	27.28%	3.908%
12	9.098	1188	1192	1196	rVV	29913	29816	3.93%	0.563%
13	9.163	1199	1203	1208	rVB8	5510	11441	1.51%	0.216%
14	9.269	1218	1221	1225	rVB5	8006	11301	1.49%	0.213%
15	9.345	1232	1234	1237	rBV2	13323	12733	1.68%	0.240%
16	9.416	1243	1246	1248	rVB2	11105	9758	1.29%	0.184%
17	9.628	1279	1282	1286	rVB	32649	25471	3.36%	0.481%
18	9.687	1288	1292	1296	rVV	915374	701062	92.35%	13.231%
19	9.886	1323	1326	1329	rVB4	7168	8969	1.18%	0.169%
20	10.128	1363	1367	1369	rVB2	20605	18680	2.46%	0.353%
21	10.345	1401	1404	1409	rVB	12668	12516	1.65%	0.236%
22	10.475	1421	1426	1430	rBV	90758	89983	11.85%	1.698%
23	10.598	1444	1447	1452	rBV2	28644	34906	4.60%	0.659%
24	11.045	1520	1523	1525	rBV	23212	19889	2.62%	0.375%
25	11.069	1525	1527	1532	rVB5	10972	15857	2.09%	0.299%
26	11.169	1540	1544	1547	rBV	802992	626869	82.57%	11.831%
27	11.469	1593	1595	1598	rBV2	17053	15541	2.05%	0.293%
28	11.575	1609	1613	1618	rBV6	7921	17464	2.30%	0.330%
29	11.698	1632	1634	1639	rVB5	10226	10929	1.44%	0.206%
30	11.875	1662	1664	1667	rBV	14885	13350	1.76%	0.252%
31	12.092	1699	1701	1704	rBV4	11262	14081	1.85%	0.266%
32	12.216	1720	1722	1725	rBV2	12772	11622	1.53%	0.219%
33	12.375	1747	1749	1752	rVB	19134	15396	2.03%	0.291%
34	12.604	1785	1788	1791	rBV	28880	29702	3.91%	0.561%
35	12.751	1810	1813	1821	rVB	228813	194316	25.60%	3.667%
36	13.798	1988	1991	1995	rBV	630714	594906	78.36%	11.228%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092222\
Data File : BF130384.D
Acq On : 22 Sep 2022 19:52
Operator : CG\JU
Sample : N4753-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-01-092122

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	13.904	2005	2009	2014	rVB	212118	216040	28.46%	4.077%
38	15.198	2225	2229	2234	rVB	380488	423946	55.84%	8.001%




Sum of corrected areas: 5298499

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092222\
Data File : BF130384.D
Acq On : 22 Sep 2022 19:52
Operator : CG\JU
Sample : N4753-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-01-092122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

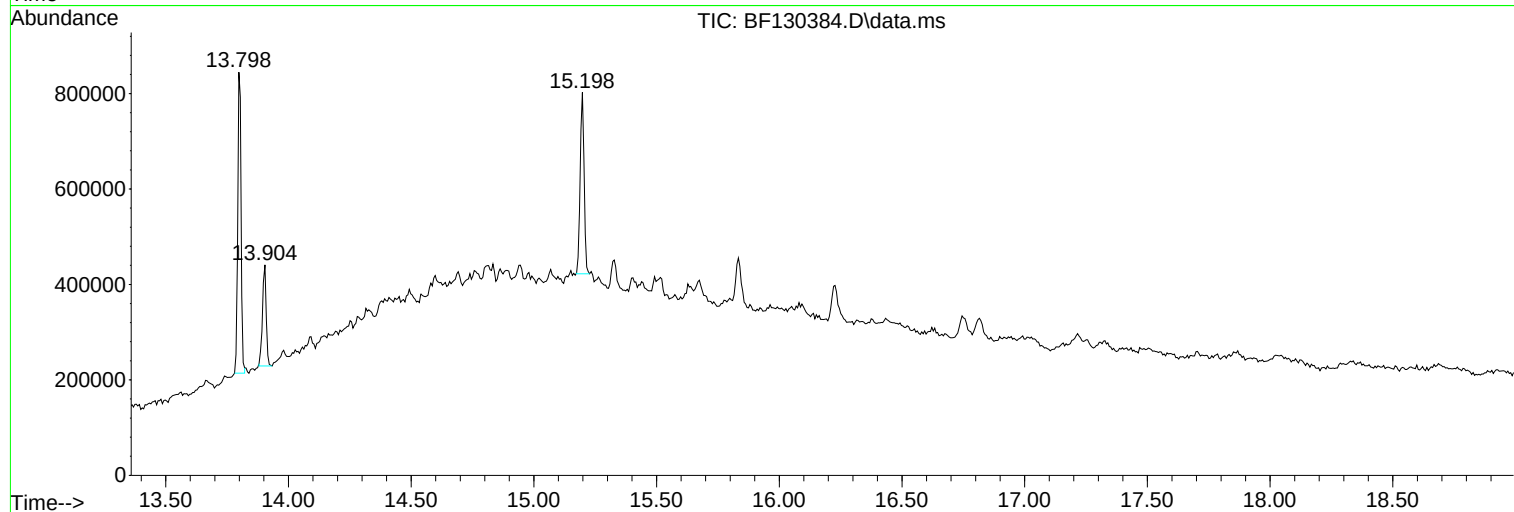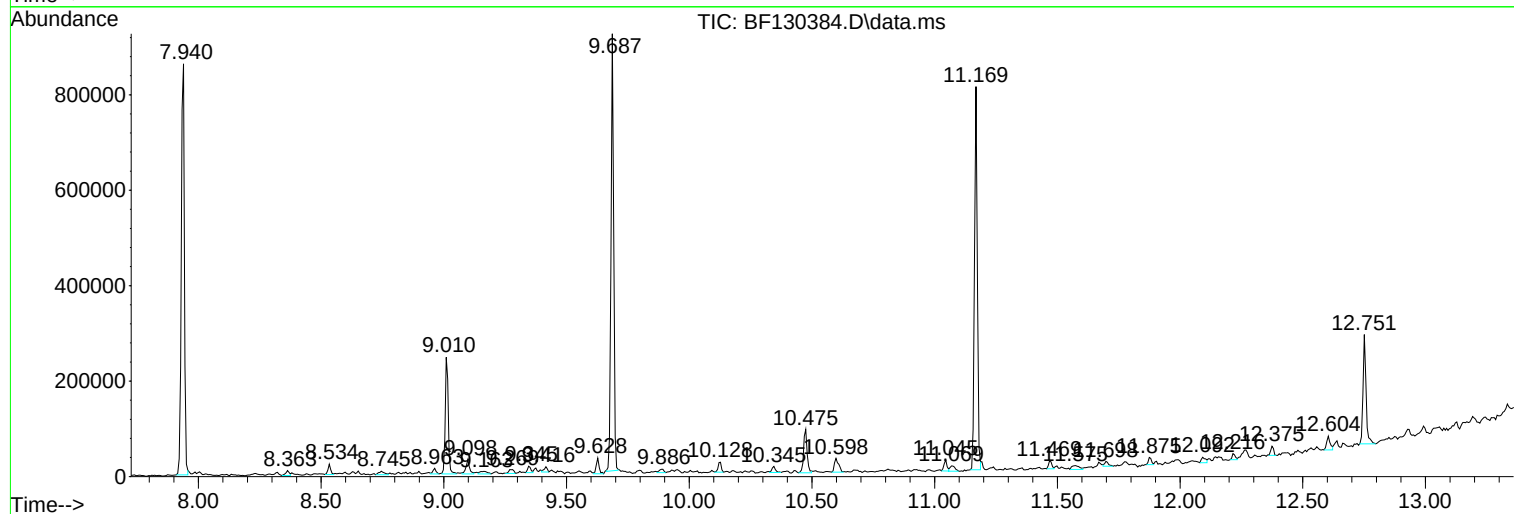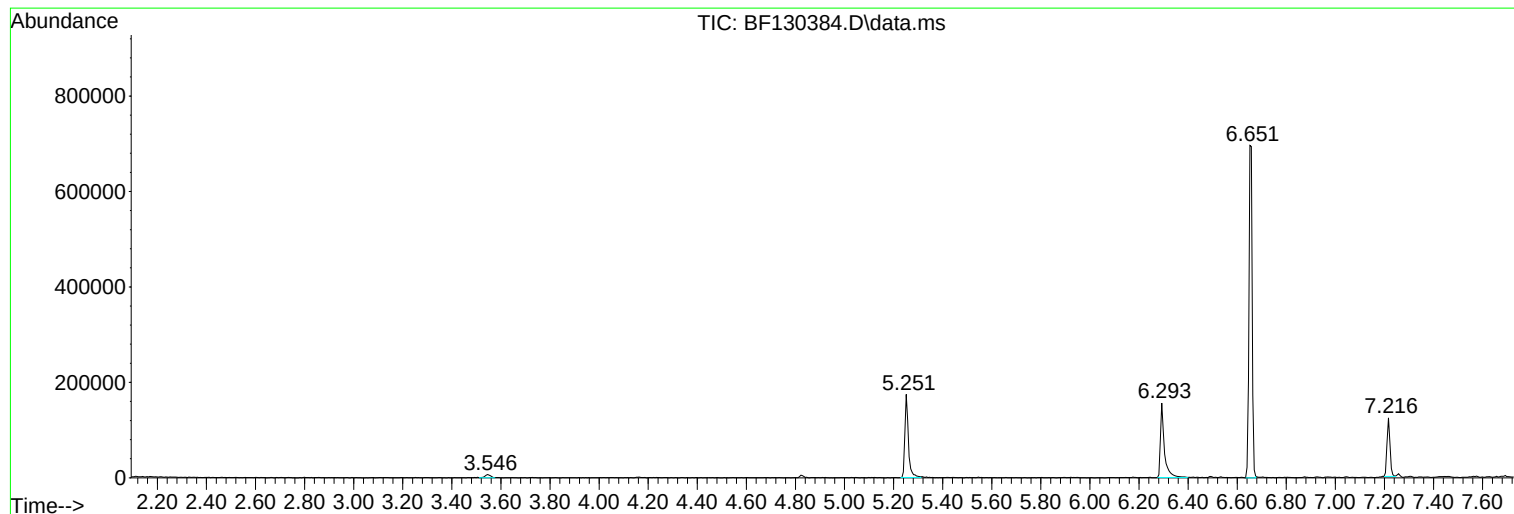

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092222\
Data File : BF130384.D
Acq On : 22 Sep 2022 19:52
Operator : CG\JU
Sample : N4753-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-01-092122










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.904	7.26 ng	216040	Chrysene-d12	13.798

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	58
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	45
4			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	42
5			2-Phenyl-6-(trifluoromethyl)-1H-...	277	C15H10F3NO	1000387-59-3	38

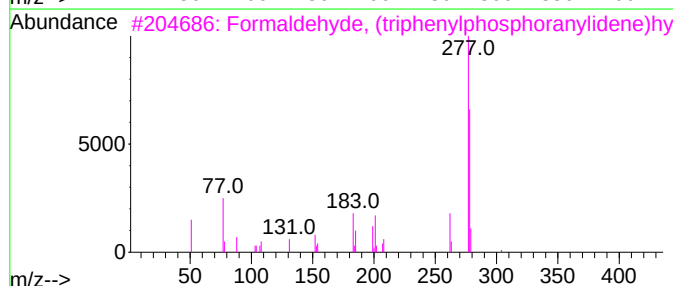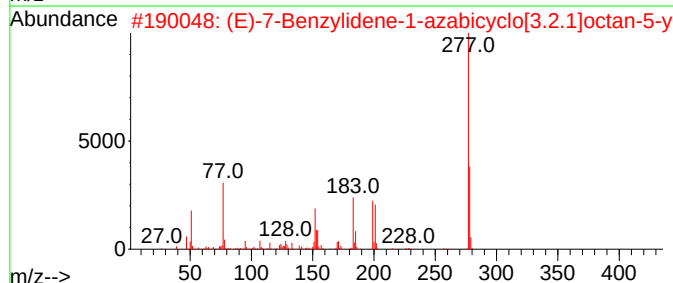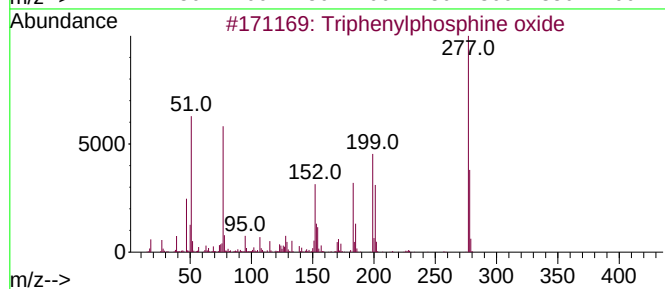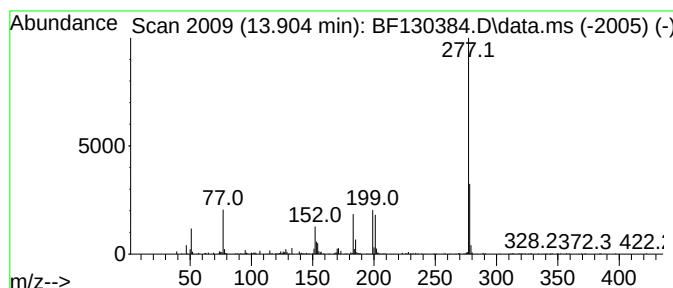

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092222\
Data File : BF130384.D
Acq On : 22 Sep 2022 19:52
Operator : CG\JU
Sample : N4753-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-01-092122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	13.904	7.3	ng	216040	5	13.798	594906	20.0