


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092222\
 Data File : BF130372.D
 Acq On : 22 Sep 2022 11:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 19 15:06:14 2022

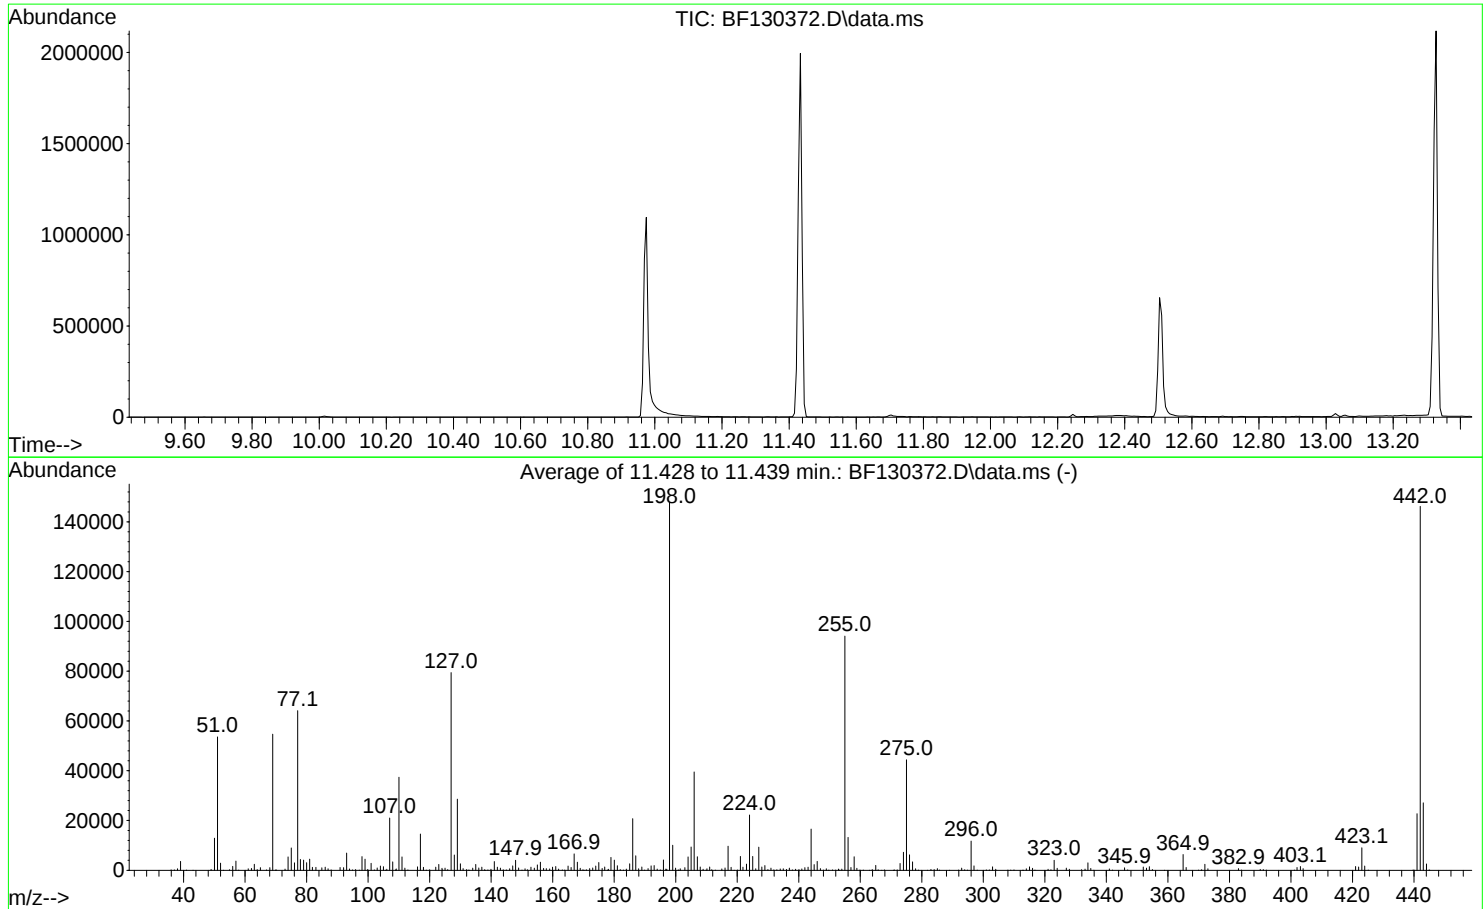




AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	53613	PASS
68	69	0.00	2	2.0	1086	PASS
69	198	0.00	100	37.0	54685	PASS
70	69	0.00	2	0.3	148	PASS
127	198	10	80	53.7	79408	PASS
197	198	0.00	2	0.3	464	PASS
198	198	100	100	100.0	147808	PASS
199	198	5	9	6.8	10093	PASS
275	198	10	60	30.0	44384	PASS
365	198	1	100	4.3	6316	PASS
441	198	0.01	100	15.4	22719	PASS
442	442	50	100	100.0	146251	PASS
443	442	15	24	18.6	27131	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092222\
Data File : BF130372.D
Acq On : 22 Sep 2022 11:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 22 16:58:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 15:06:14 2022
Response via : Initial Calibration

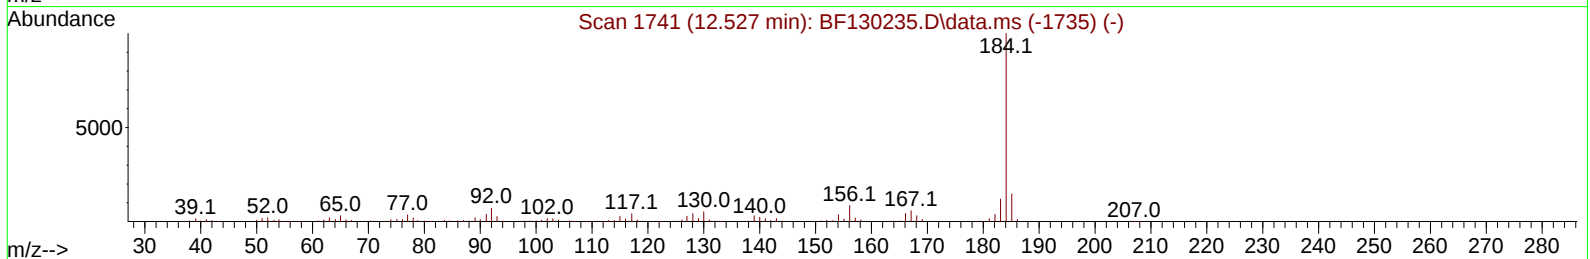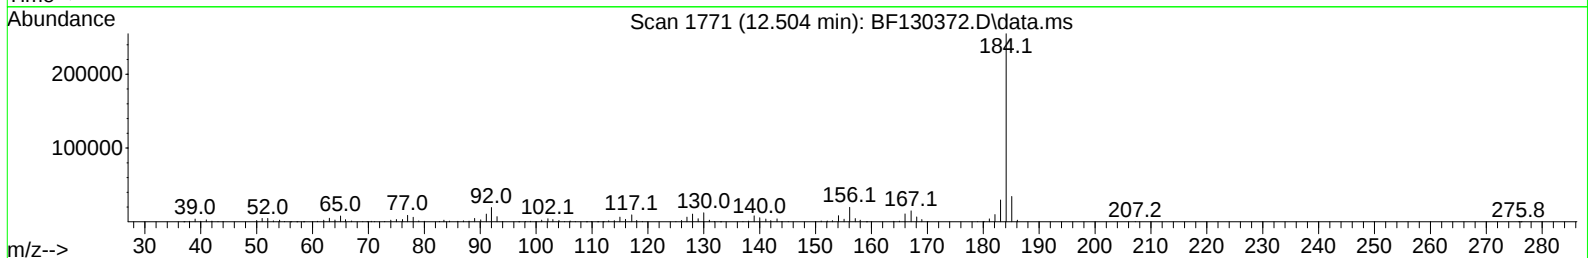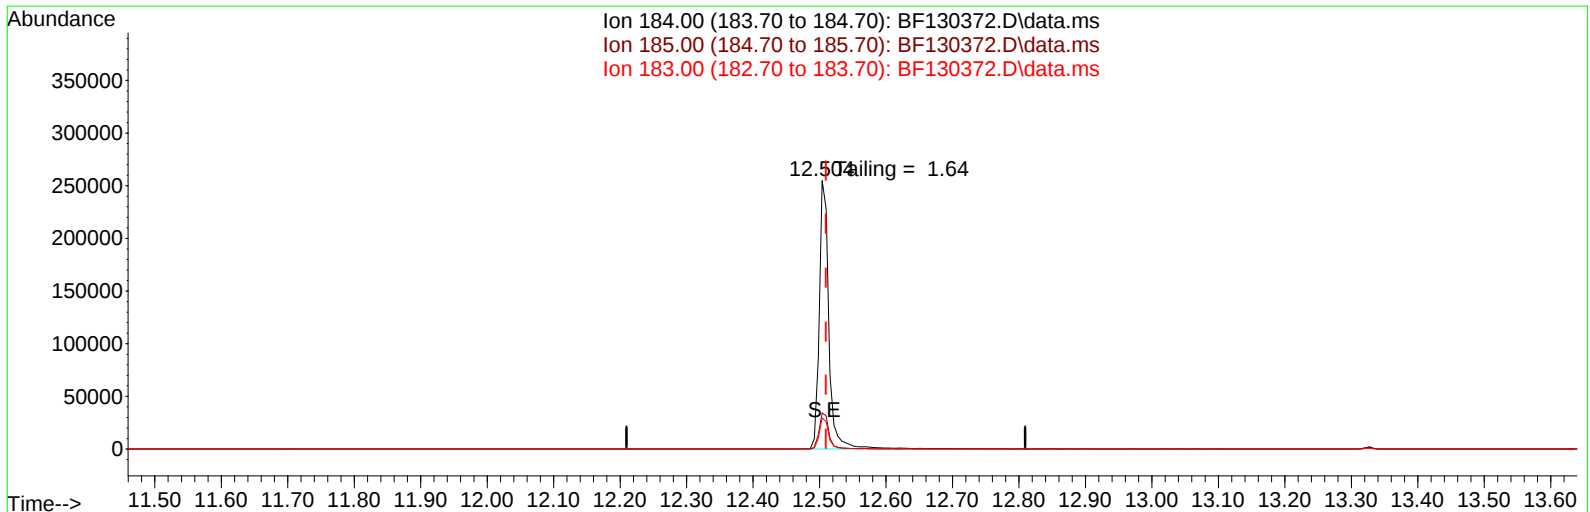

TIC: BF130372.D\data.ms

(77) Benzidine

12.504min (-0.006) 40216.60 ng




response 255672

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.47
183.00	11.40	11.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092222\
 Data File : BF130372.D
 Acq On : 22 Sep 2022 11:27
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 22 16:58:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 19 15:06:14 2022
 Response via : Initial Calibration

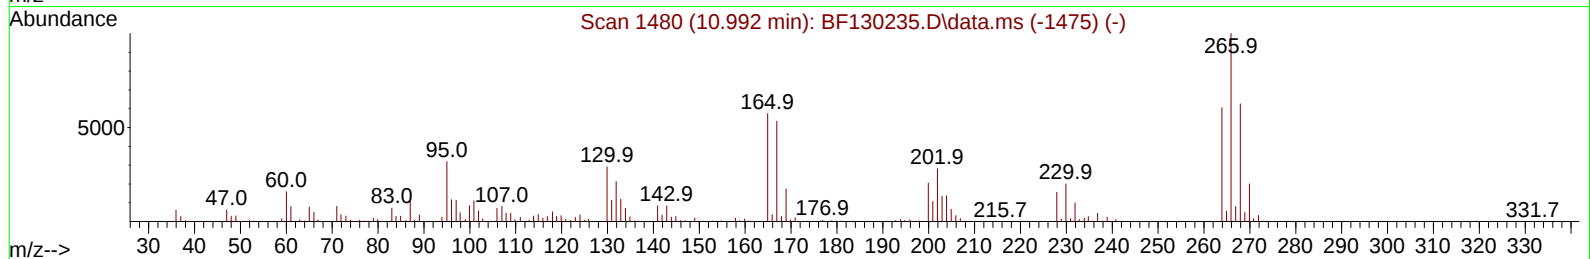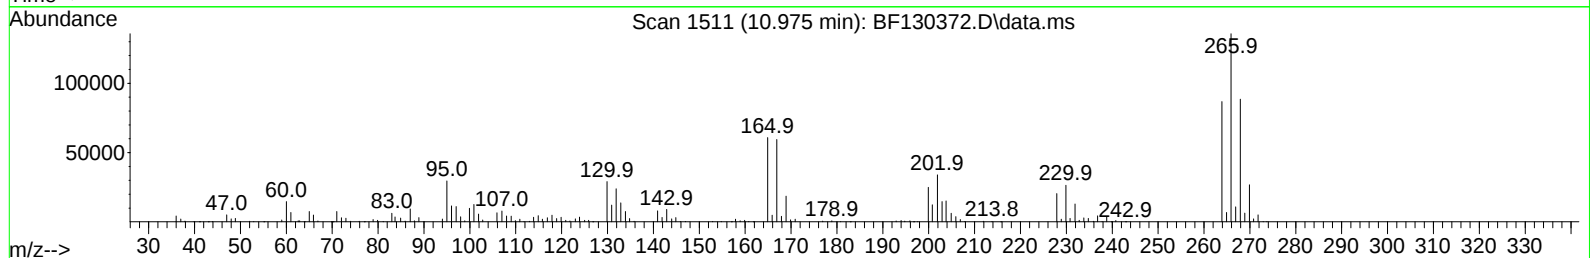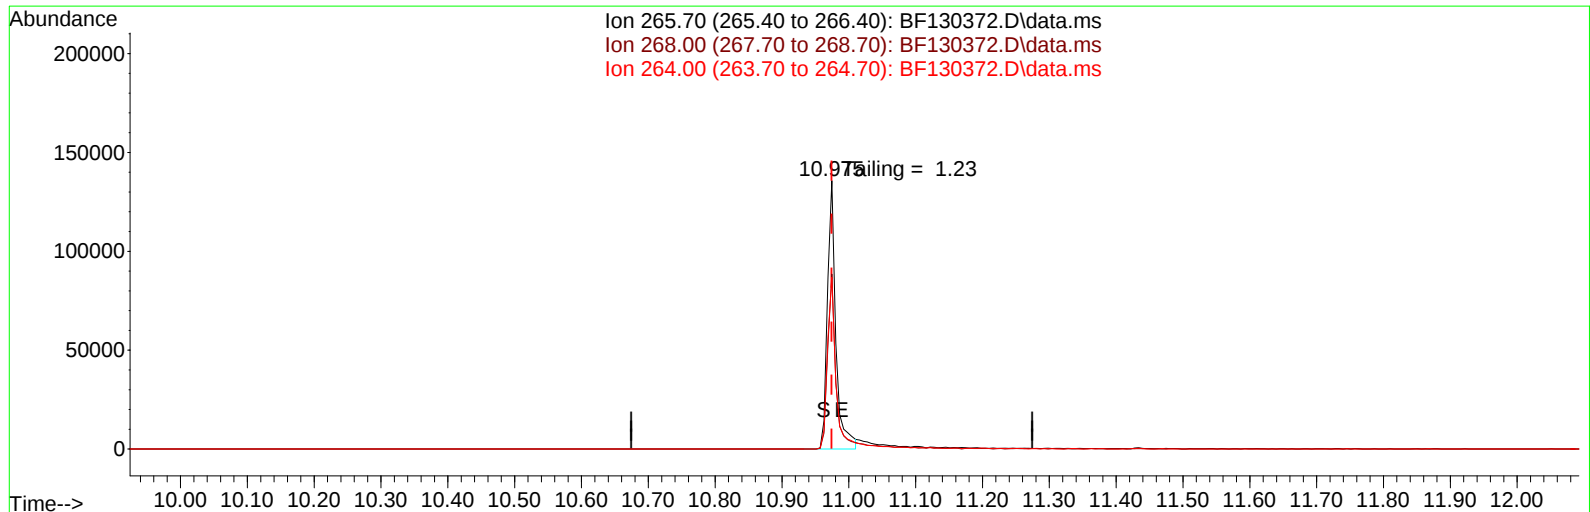

TIC: BF130372.D\data.ms

(70) Pentachlorophenol (C)

10.975min (+ 0.000) 353423.85 ng

response 130457

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.20
264.00	63.10	63.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/22/2022	BNA_F	<u>BF130372.D</u>
Compound Name	Response	Retention Time
DDT	326218	13.32
DDD	3136	13.02
DDE	654	12.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3790	330008	1.15

Instrument :
BNA_F
ClientSampleId :
DFTPP