
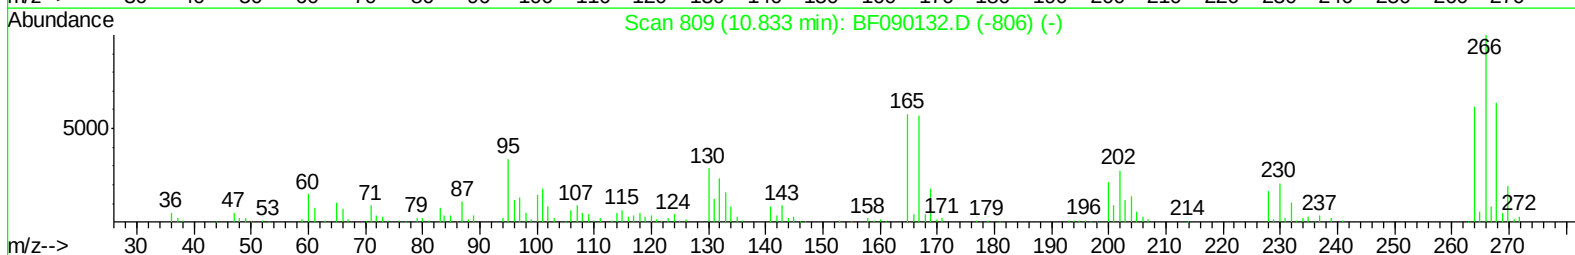
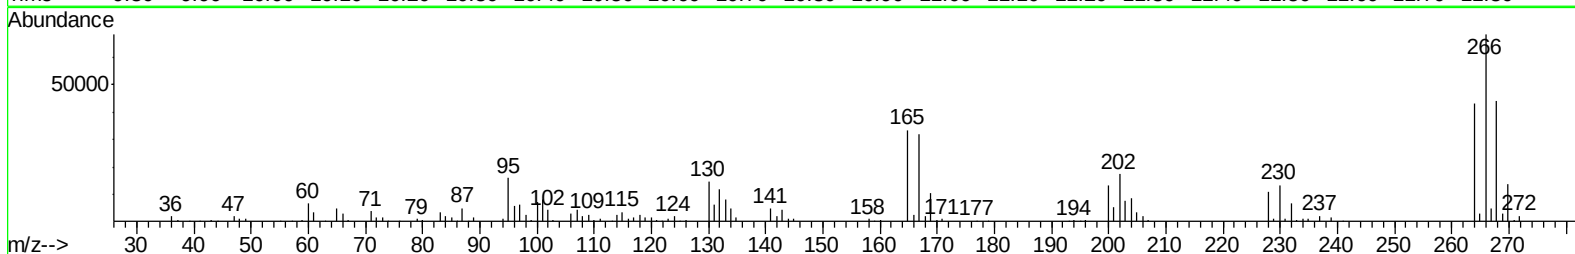


Data Path : Z:\HPCHEM1\BNA_F\Data\BF092316\
Data File : BF090194.D
Acq On : 23 Sep 2016 12:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 04:43:00 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 17:58:29 2016
Response via : Initial Calibration

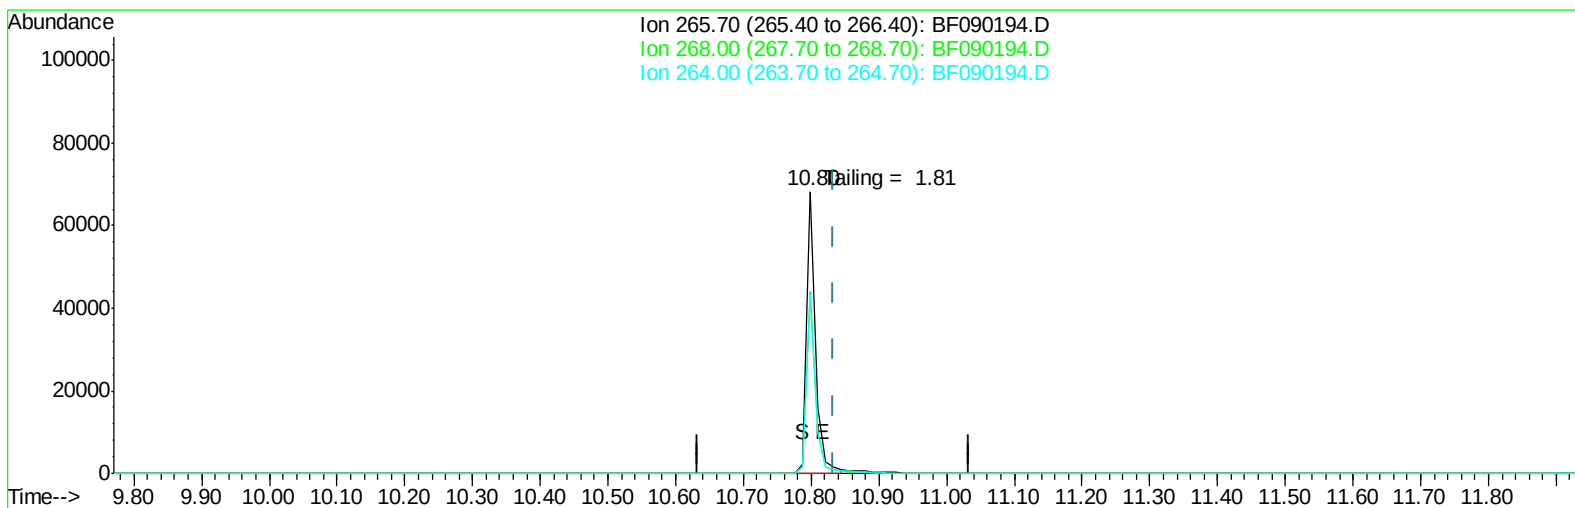

TIC: BF090194.D

(69) Pentachlorophenol (C)




10.799min (-0.034) 14431.84ng

response 65104

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	64.73
264.00	62.90	63.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF092316\
Data File : BF090194.D
Acq On : 23 Sep 2016 12:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 04:43:00 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 17:58:29 2016
Response via : Initial Calibration

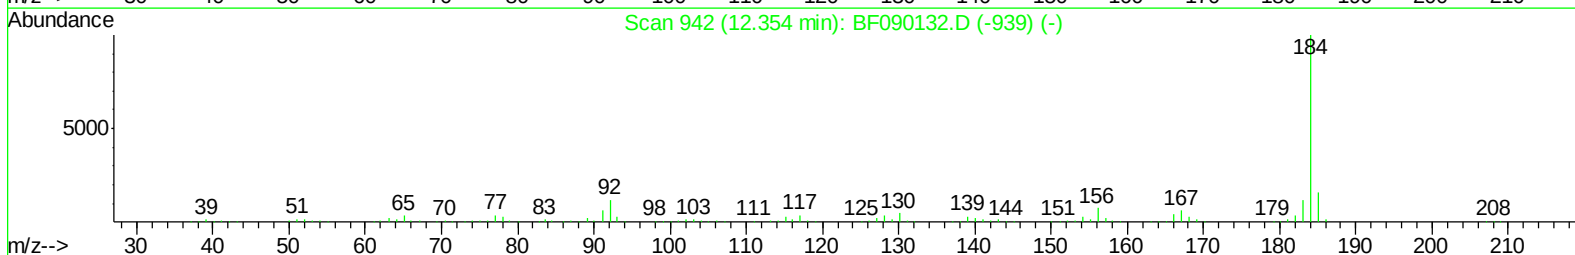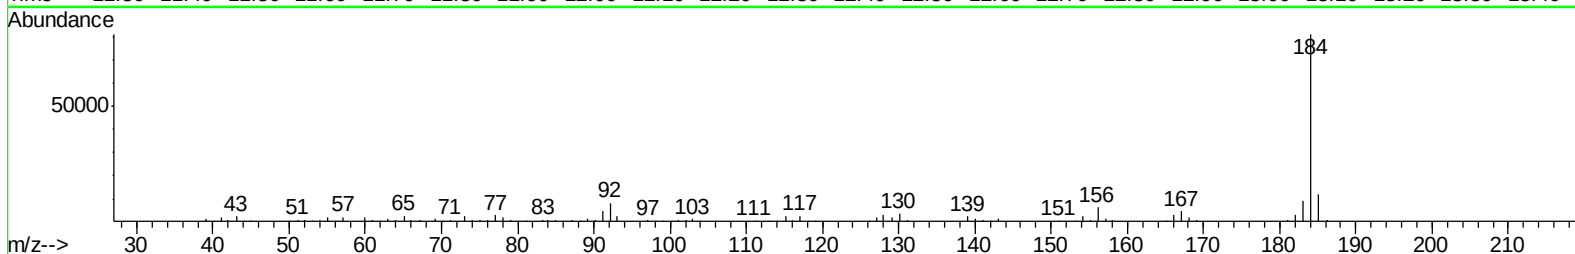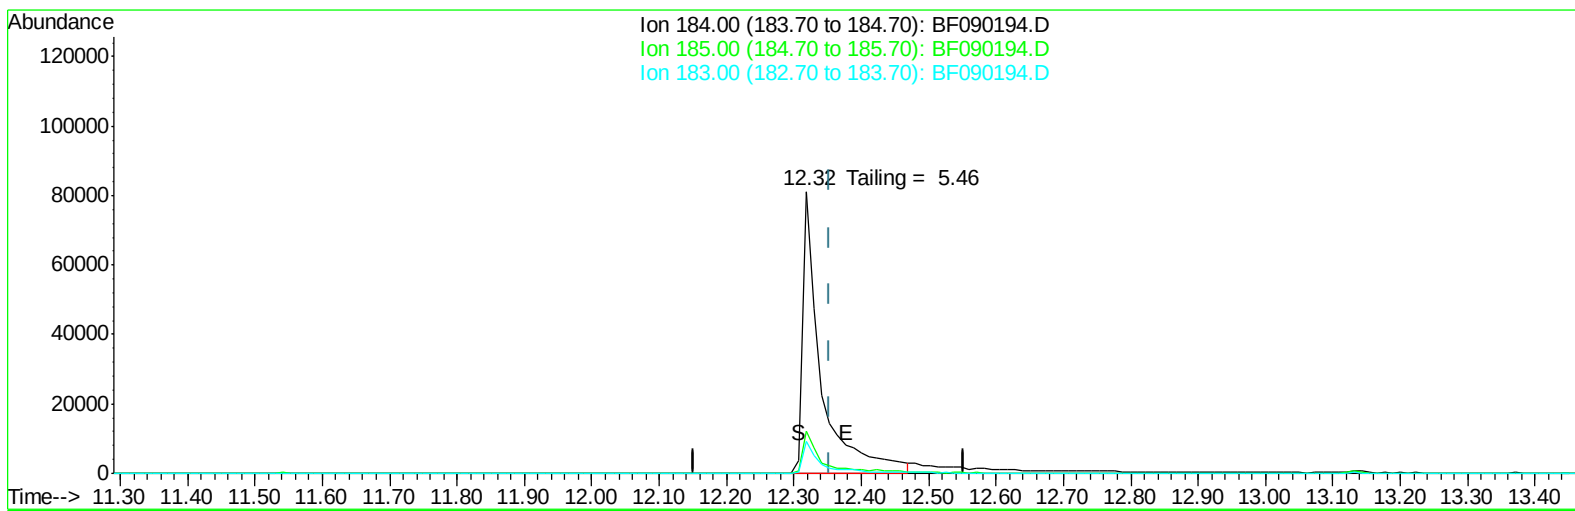

TIC: BF090194.D

(76) Benzidine

12.319min (-0.034) 6023.41ng

response 154232

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	14.92
183.00	11.50	11.18
0.00	0.00	0.00