
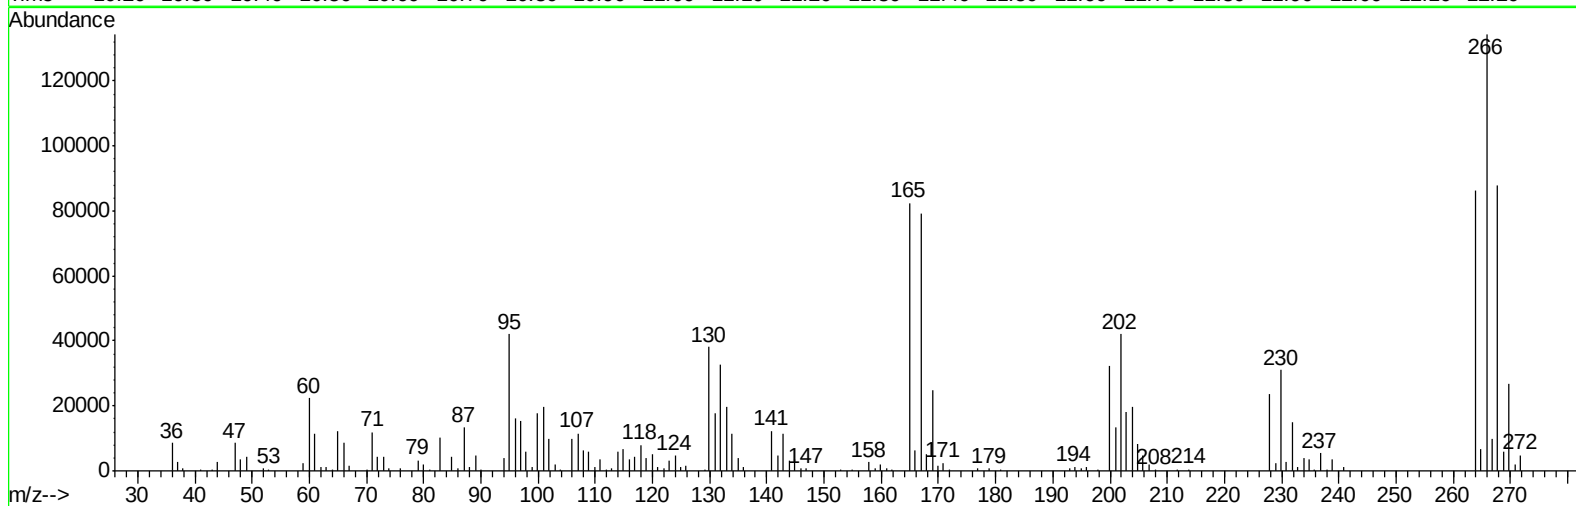


Data Path : Z:\HPCHEM1\BNA F\Data\BF092317\
Data File : BF098728.D
Acq On : 23 Sep 2017 10:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 00:52:01 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

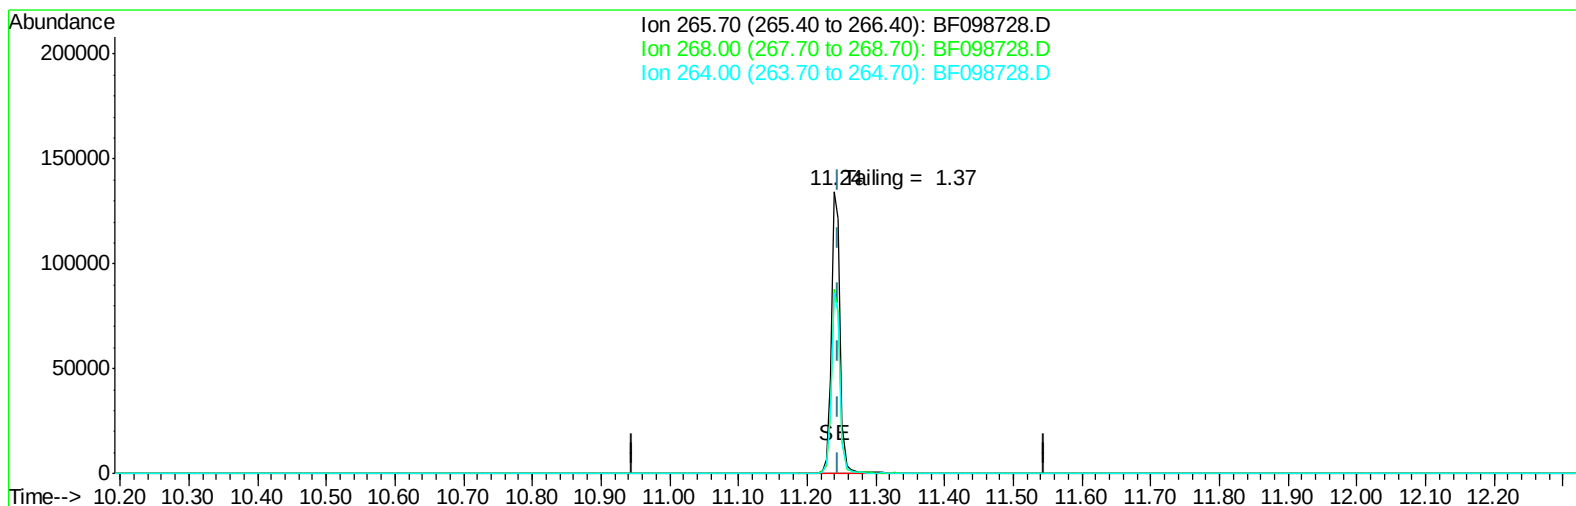

TIC: BF098728.D

(69) Pentachlorophenol (C)



11.239min (-0.006) 28368.61ng

response 120898

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.47
264.00	61.90	64.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF092317\
Data File : BF098728.D
Acq On : 23 Sep 2017 10:03
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 09:11:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

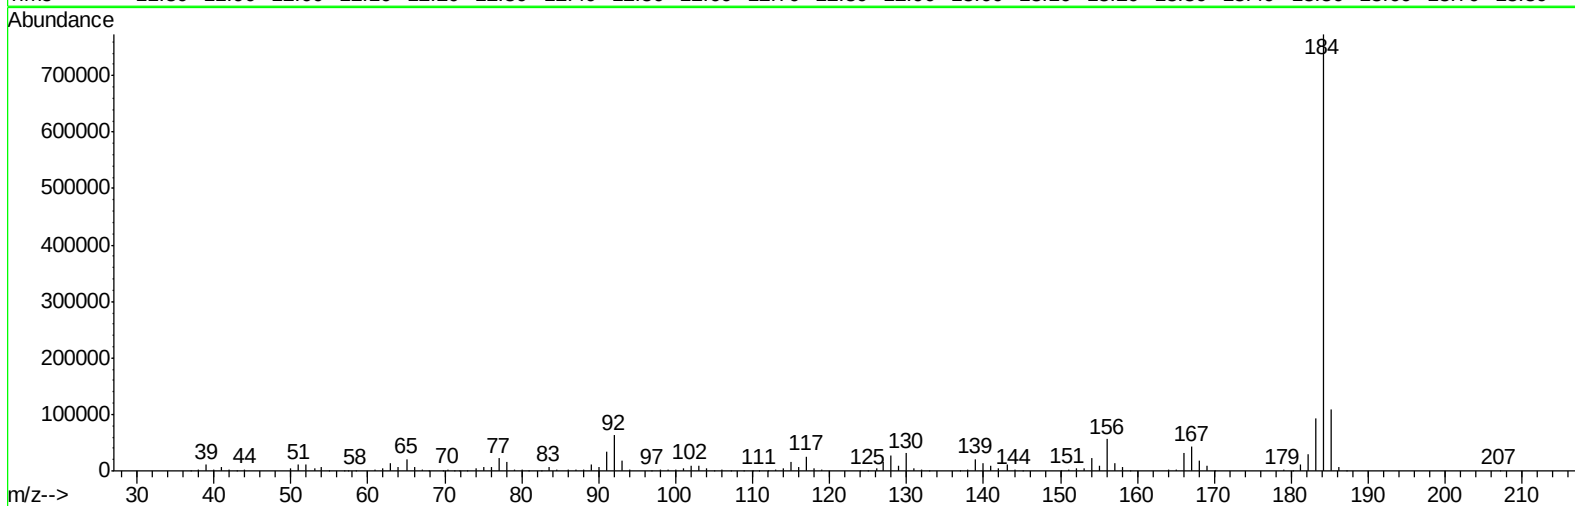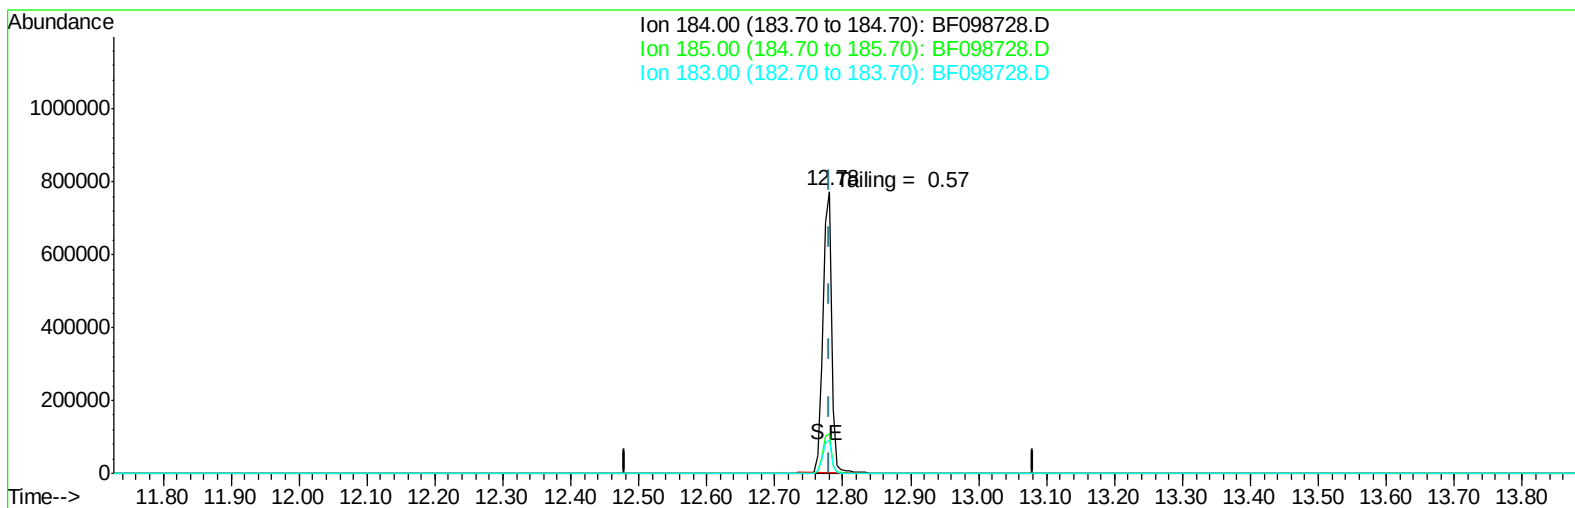

TIC: BF098728.D

(76) Benzidine

12.780min (+0.000) 0.00ng

response 725624

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.22
183.00	11.60	11.98
0.00	0.00	0.00