

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092317\
 Data File : BF098765.D
 Acq On : 24 Sep 2017 4:33
 Operator : SJ/JU
 Sample : I5291-01DL 50X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OILY-STONEDL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	582	585	589	rBV	91635	81208	4.48%	0.448%
2	6.528	752	755	759	rVB	92516	81501	4.49%	0.450%
3	6.686	779	782	785	rVB	101405	84352	4.65%	0.465%
4	6.922	818	822	826	rVB	968783	777311	42.83%	4.287%
5	7.075	842	848	851	rBV	88271	75065	4.14%	0.414%
6	7.475	914	916	919	rBV	50548	38623	2.13%	0.213%
7	7.728	957	959	964	rVB3	27216	26288	1.45%	0.145%
8	8.204	1036	1040	1042	rBV	1063719	951744	52.45%	5.249%
9	8.228	1042	1044	1047	rVB	1207395	858750	47.32%	4.736%
10	8.257	1047	1049	1052	rVB2	42485	33620	1.85%	0.185%
11	8.286	1052	1054	1057	rBV	46857	39761	2.19%	0.219%
12	8.463	1076	1084	1085	rBV2	67291	87117	4.80%	0.480%
13	8.586	1101	1105	1108	rBV	242870	200187	11.03%	1.104%
14	8.669	1116	1119	1123	rVB	161759	131711	7.26%	0.726%
15	8.704	1123	1125	1128	rBV2	102746	103489	5.70%	0.571%
16	8.763	1132	1135	1137	rVV	285753	217906	12.01%	1.202%
17	8.792	1137	1140	1142	rVV	124708	105134	5.79%	0.580%
18	8.916	1157	1161	1165	rVB	2025617	1814682	100.00%	10.009%
19	8.980	1169	1172	1174	rBV2	27356	28677	1.58%	0.158%
20	9.016	1174	1178	1182	rBV	1137245	949775	52.34%	5.238%
21	9.110	1192	1194	1197	rVB3	25254	28151	1.55%	0.155%
22	9.151	1197	1201	1206	rBV5	48947	82242	4.53%	0.454%
23	9.198	1206	1209	1211	rBV3	40592	38770	2.14%	0.214%
24	9.216	1211	1212	1217	rVB3	41243	31480	1.73%	0.174%
25	9.275	1218	1222	1224	rBV2	128984	112465	6.20%	0.620%
26	9.322	1227	1230	1232	rBV3	24274	30142	1.66%	0.166%
27	9.357	1232	1236	1238	rBV2	91139	117884	6.50%	0.650%
28	9.427	1246	1248	1251	rVB2	62698	53866	2.97%	0.297%
29	9.475	1251	1256	1259	rBV	123962	143864	7.93%	0.793%
30	9.539	1263	1267	1272	rVB	178564	247955	13.66%	1.368%
31	9.616	1273	1280	1283	rBV2	331413	449378	24.76%	2.478%
32	9.645	1283	1285	1287	rVV	128596	110183	6.07%	0.608%
33	9.669	1287	1289	1292	rVV2	156044	160838	8.86%	0.887%
34	9.698	1292	1294	1297	rVB2	52031	43659	2.41%	0.241%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092317\
 Data File : BF098765.D
 Acq On : 24 Sep 2017 4:33
 Operator : SJ/JU
 Sample : I5291-01DL 50X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OILY-STONEDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	9.733	1297	1300	1302	rBV2	200249	181129	9.98%	0.999%
36	9.822	1312	1315	1318	rBV2	149055	188403	10.38%	1.039%
37	9.869	1318	1323	1327	rVV4	184297	277527	15.29%	1.531%
38	9.957	1330	1338	1342	rVV	1000388	1311329	72.26%	7.232%
39	9.992	1342	1344	1346	rBV3	110353	93827	5.17%	0.517%
40	10.063	1353	1356	1360	rBV4	91868	121784	6.71%	0.672%
41	10.116	1362	1365	1367	rBV3	112439	132679	7.31%	0.732%
42	10.204	1378	1380	1384	rBV3	125123	133346	7.35%	0.735%
43	10.239	1384	1386	1389	rVB	112011	102223	5.63%	0.564%
44	10.274	1390	1392	1394	rBV3	128452	119798	6.60%	0.661%
45	10.298	1394	1396	1398	rBV3	95920	88143	4.86%	0.486%
46	10.369	1405	1408	1410	rBV2	264888	295100	16.26%	1.628%
47	10.416	1413	1416	1418	rBV	291336	289478	15.95%	1.597%
48	10.604	1443	1448	1451	rBV	604937	875820	48.26%	4.830%
49	10.657	1455	1457	1460	rVB	218994	182166	10.04%	1.005%
50	10.874	1490	1494	1500	rBV	1168835	1468950	80.95%	8.102%
51	11.051	1522	1524	1526	rBV	260870	234301	12.91%	1.292%
52	11.339	1570	1573	1576	rBV	1013396	822156	45.31%	4.534%
53	11.451	1589	1592	1595	rBV	895969	824555	45.44%	4.548%
54	11.686	1630	1632	1635	rBV	338354	302920	16.69%	1.671%
55	12.421	1755	1757	1760	rBV	266259	244878	13.49%	1.351%
56	14.086	2037	2040	2044	rVB	911688	801166	44.15%	4.419%
57	15.580	2289	2294	2301	rVB	511766	660673	36.41%	3.644%
58	16.045	2370	2373	2378	rVB2	28103	41005	2.26%	0.226%


Sum of corrected areas: 18131134

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092317\
Data File : BF098765.D
Acq On : 24 Sep 2017 4:33
Operator : SJ/JU
Sample : I5291-01DL 50X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OILY-STONEDL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

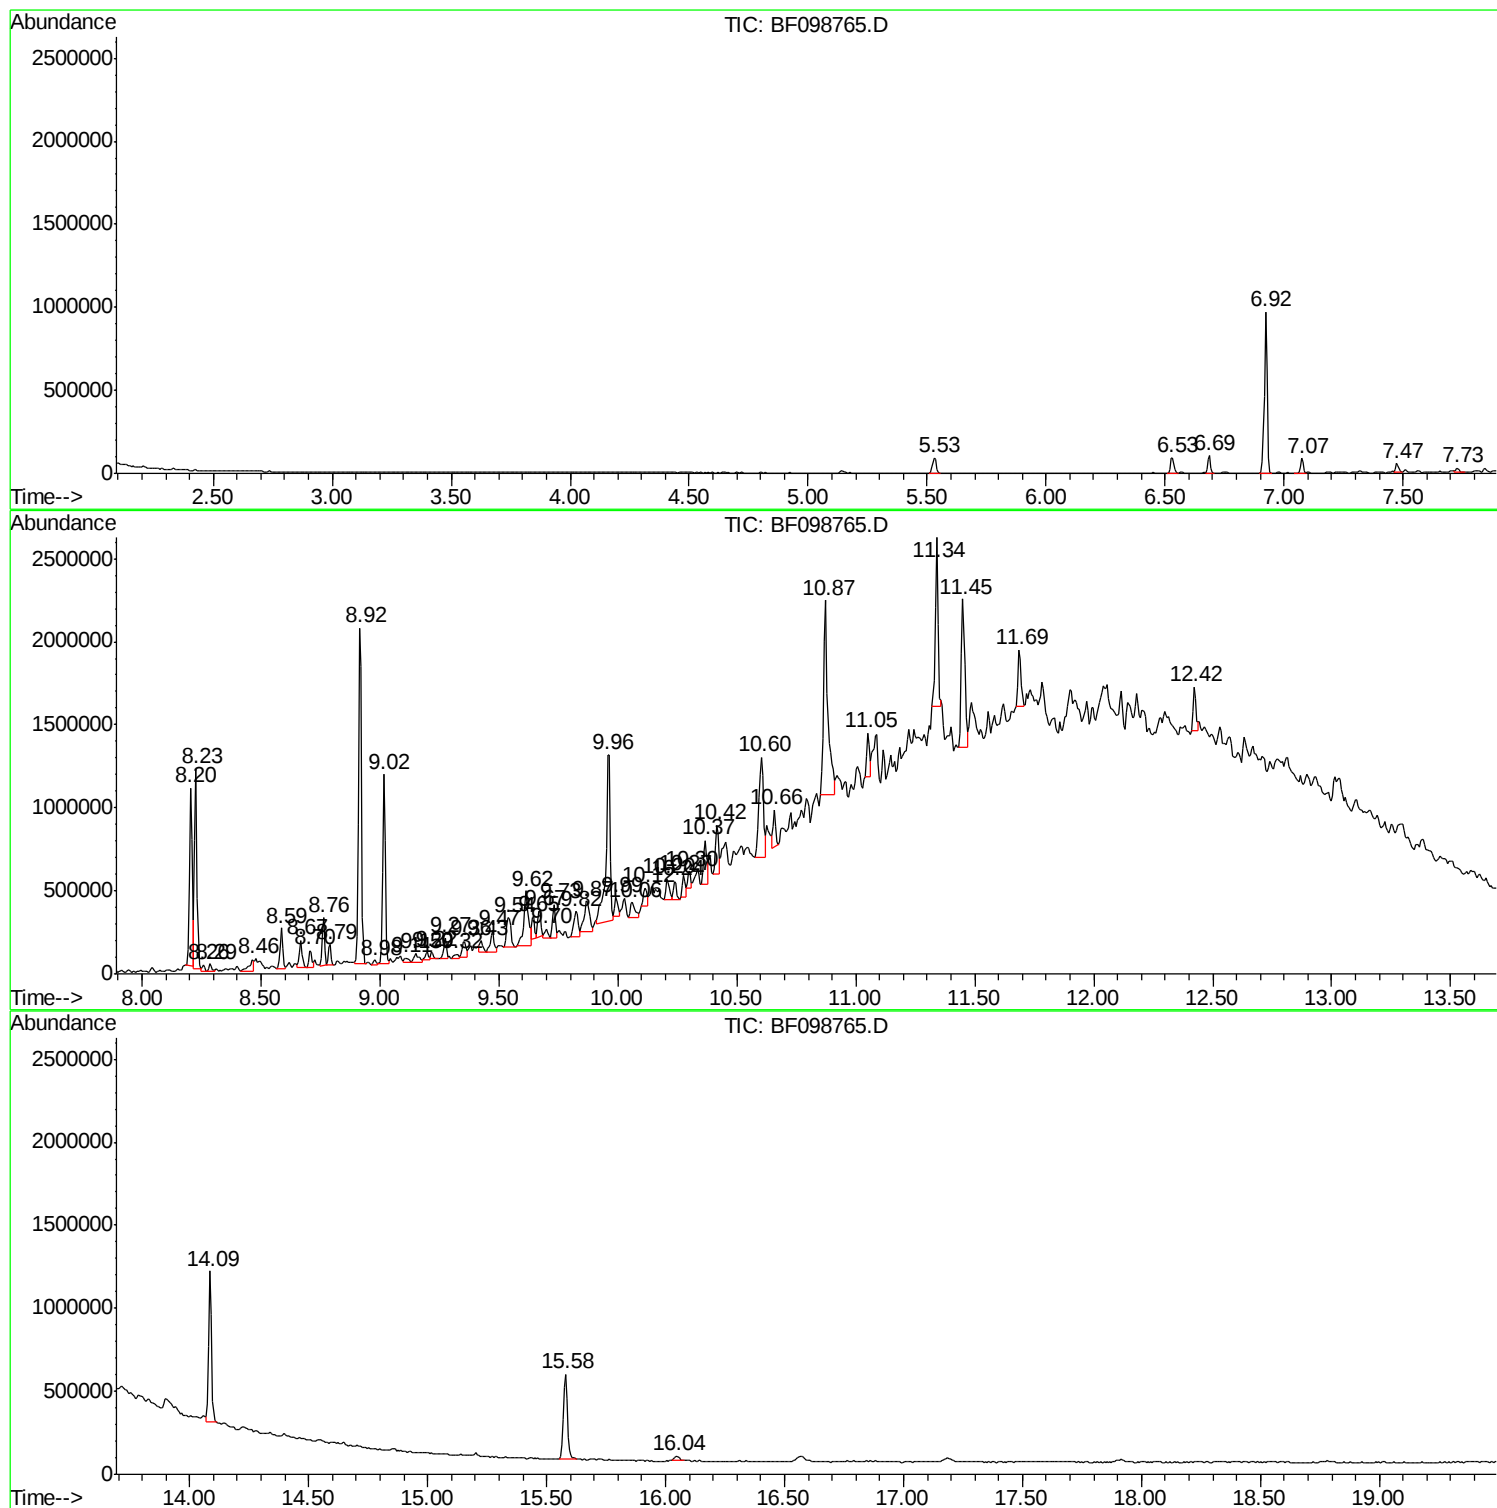

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF092317\
Data_File : BF098765.D
Acq_On : 24 Sep 2017 4:333
Operator : SJ/JUU
Sample : I5291-01DL_50XX
Misc :
ALS_Vial : 27 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
OILY-STONEDL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
