

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092317\
 Data File : BF098766.D
 Acq On : 24 Sep 2017 5:02
 Operator : SJ/JU
 Sample : I5288-01DL 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DRUM-A-OILYSTONESDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.140	515	519	525	rBV	63690	66239	2.59%	0.266%
2	5.528	581	585	589	rBV	509349	437175	17.12%	1.754%
3	6.534	752	756	760	rBV	483151	411057	16.10%	1.649%
4	6.687	778	782	785	rBV	533967	436048	17.08%	1.749%
5	6.922	818	822	826	rVB	709131	566067	22.17%	2.271%
6	7.075	845	848	852	rVB	400997	341303	13.37%	1.369%
7	7.475	913	916	920	rVB	270354	224638	8.80%	0.901%
8	8.204	1036	1040	1043	rVB	827356	651319	25.51%	2.613%
9	8.786	1136	1139	1143	rVB	38257	32461	1.27%	0.130%
10	9.216	1210	1212	1217	rVB	37897	34470	1.35%	0.138%
11	9.275	1218	1222	1225	rBV	526420	407802	15.97%	1.636%
12	9.351	1232	1235	1239	rBV2	54153	62586	2.45%	0.251%
13	9.622	1274	1281	1286	rBV	117366	143073	5.60%	0.574%
14	9.669	1286	1289	1292	rBV2	159394	158321	6.20%	0.635%
15	9.827	1312	1316	1318	rBV	39285	42720	1.67%	0.171%
16	9.875	1318	1324	1327	rVV2	61781	110803	4.34%	0.444%
17	9.957	1334	1338	1342	rVB2	630466	600848	23.53%	2.410%
18	10.116	1361	1365	1367	rBV2	56283	72887	2.85%	0.292%
19	10.204	1377	1380	1384	rBV2	55226	66878	2.62%	0.268%
20	10.239	1384	1386	1389	rVB	57584	42921	1.68%	0.172%
21	10.380	1405	1410	1413	rBV2	82835	116093	4.55%	0.466%
22	10.416	1413	1416	1418	rBV3	60074	67610	2.65%	0.271%
23	10.592	1443	1446	1450	rBV2	189747	293638	11.50%	1.178%
24	10.657	1454	1457	1459	rVB	76960	61897	2.42%	0.248%
25	10.686	1459	1462	1466	rBV	85543	88987	3.48%	0.357%
26	10.722	1466	1468	1470	rBV	120754	99742	3.91%	0.400%
27	10.745	1470	1472	1475	rVB	158324	124561	4.88%	0.500%
28	10.869	1488	1493	1500	rBV2	208571	498264	19.51%	1.999%
29	11.051	1520	1524	1528	rBV	299120	473374	18.54%	1.899%
30	11.116	1532	1535	1537	rBV	162101	141226	5.53%	0.567%
31	11.139	1537	1539	1543	rBV	148617	167214	6.55%	0.671%
32	11.180	1543	1546	1548	rBV	242823	191076	7.48%	0.766%
33	11.304	1565	1567	1568	rBV	170546	115089	4.51%	0.462%
34	11.333	1568	1572	1575	rVV	543612	613029	24.01%	2.459%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092317\
 Data File : BF098766.D
 Acq On : 24 Sep 2017 5:02
 Operator : SJ/JU
 Sample : I5288-01DL 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DRUM-A-OILYSTONESDL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.445	1589	1591	1595	rBV	616780	582088	22.79%	2.335%
36	11.480	1595	1597	1602	rVV	467372	673789	26.39%	2.703%
37	11.521	1602	1604	1606	rVB	220236	159801	6.26%	0.641%
38	11.551	1606	1609	1611	rBV	279346	248929	9.75%	0.999%
39	11.580	1611	1614	1617	rBV	181556	187190	7.33%	0.751%
40	11.616	1617	1620	1623	rBV	359195	366037	14.33%	1.468%
41	11.686	1630	1632	1635	rVB	170301	131972	5.17%	0.529%
42	11.745	1638	1642	1646	rBV2	285320	549505	21.52%	2.204%
43	11.898	1665	1668	1673	rBV	753513	1082308	42.38%	4.342%
44	11.969	1677	1680	1682	rBV	348303	323747	12.68%	1.299%
45	11.998	1682	1685	1688	rBV2	508359	602034	23.58%	2.415%
46	12.027	1688	1690	1693	rBV3	485523	560138	21.93%	2.247%
47	12.145	1707	1710	1713	rBV	596948	705683	27.63%	2.831%
48	12.180	1714	1716	1719	rVV	296241	292014	11.44%	1.171%
49	12.292	1732	1735	1738	rBV	789601	1082922	42.41%	4.344%
50	12.363	1745	1747	1749	rBV	304583	269218	10.54%	1.080%
51	12.427	1755	1758	1762	rBV	665639	761892	29.84%	3.056%
52	12.533	1773	1776	1778	rBV	691700	675161	26.44%	2.708%
53	12.674	1797	1800	1803	rBV	871245	1130189	44.26%	4.534%
54	12.745	1810	1812	1814	rBV	440854	356386	13.96%	1.430%
55	12.904	1837	1839	1841	rBV	478419	402124	15.75%	1.613%
56	13.033	1856	1861	1871	rBV2	1127079	2553655	100.00%	10.244%
57	13.257	1897	1899	1902	rBV	499337	447346	17.52%	1.794%
58	13.292	1902	1905	1909	rVB	492278	693287	27.15%	2.781%
59	13.386	1919	1921	1925	rVB2	658894	665960	26.08%	2.671%
60	14.063	2034	2036	2039	rVB	744645	615895	24.12%	2.471%
61	15.586	2292	2295	2303	rVB	386005	602581	23.60%	2.417%
62	16.686	2479	2482	2490	rVB	155249	245599	9.62%	0.985%


Sum of corrected areas: 24928866

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092317\
Data File : BF098766.D
Acq On : 24 Sep 2017 5:02
Operator : SJ/JU
Sample : I5288-01DL 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DRUM-A-OILYSTONESDL

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

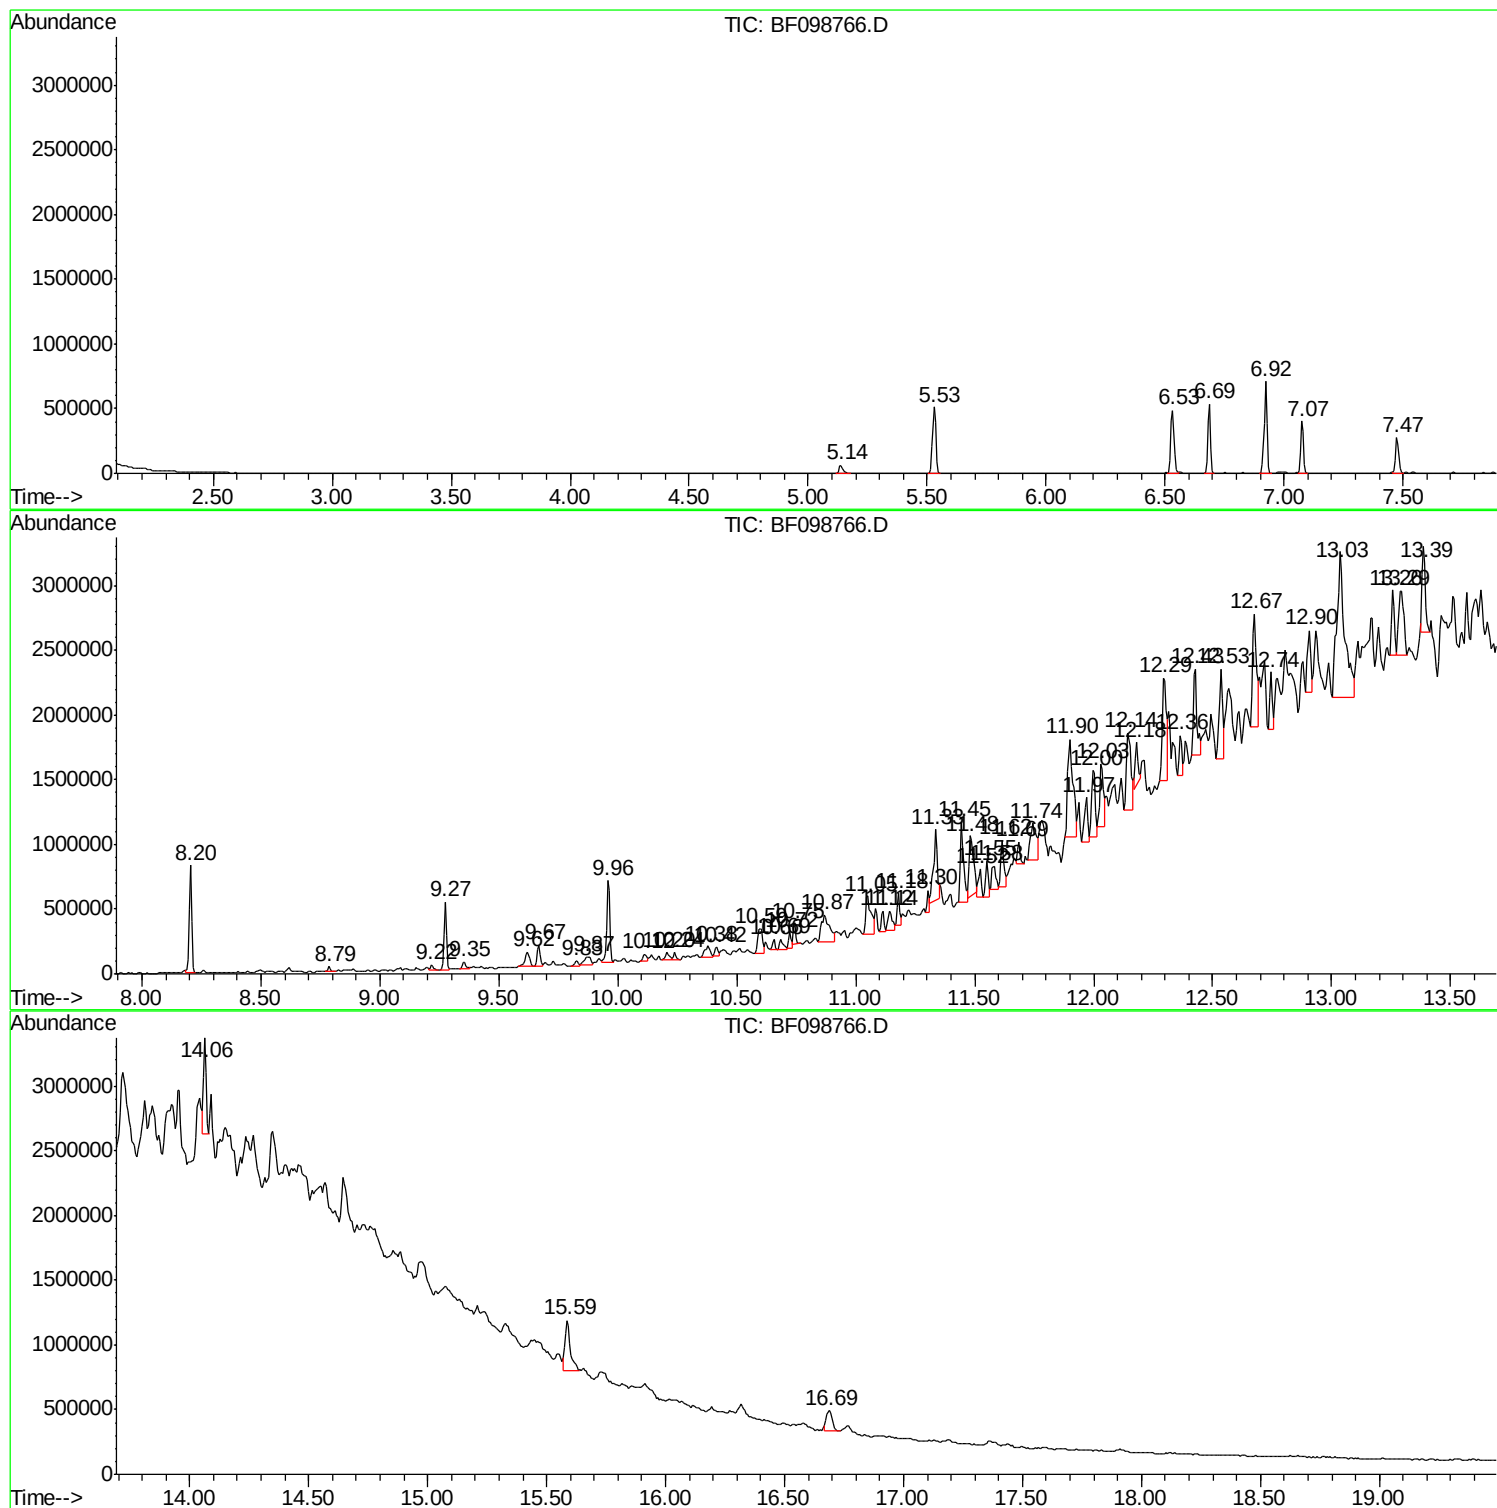

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF092317\
Data_File : BF098766.D
Acq_On : 24 Sep 2017 5:022
Operator : SJ/JUU
Sample : I5288-01DL_10XX
Misc :
ALS_Vial : 28 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
DRUM-A-OILYSTONESDL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
