

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092317\
 Data File : BF098767.D
 Acq On : 24 Sep 2017 5:30
 Operator : SJ/JU
 Sample : I5304-05DL 100X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SASP2P-ENV-118-6(5-10)DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	583	585	590	rVB	30971	26187	1.07%	0.144%
2	6.528	753	755	759	rBV	31926	25855	1.05%	0.142%
3	6.687	779	782	785	rBV	32372	25936	1.05%	0.142%
4	6.922	818	822	826	rVB	927260	721214	29.34%	3.952%
5	8.204	1036	1040	1043	rBV	1009206	796088	32.38%	4.363%
6	9.957	1334	1338	1341	rBV2	784160	688542	28.01%	3.773%
7	9.992	1341	1344	1347	rVB	94092	75696	3.08%	0.415%
8	10.504	1428	1431	1437	rBV2	38007	37167	1.51%	0.204%
9	11.339	1571	1573	1578	rVB	55700	48421	1.97%	0.265%
10	11.445	1587	1591	1593	rBV	853863	718506	29.23%	3.938%
11	11.469	1593	1595	1599	rVV	1165247	941110	38.28%	5.158%
12	11.522	1599	1604	1607	rVB	354439	287289	11.69%	1.574%
13	11.669	1623	1629	1633	rBV2	111051	118628	4.83%	0.650%
14	11.775	1643	1647	1651	rVB2	31127	26270	1.07%	0.144%
15	11.945	1670	1676	1678	rBV	138796	119557	4.86%	0.655%
16	11.975	1678	1681	1685	rVB	196126	163464	6.65%	0.896%
17	12.022	1685	1689	1692	rBV	82324	73939	3.01%	0.405%
18	12.063	1692	1696	1698	rVV2	279300	319233	12.98%	1.749%
19	12.080	1698	1699	1703	rVB	112557	63002	2.56%	0.345%
20	12.239	1722	1726	1728	rBV	133798	117852	4.79%	0.646%
21	12.263	1728	1730	1734	rVB2	68765	58536	2.38%	0.321%
22	12.498	1766	1770	1773	rBV	87025	96930	3.94%	0.531%
23	12.533	1773	1776	1778	rVV3	48841	57877	2.35%	0.317%
24	12.580	1781	1784	1789	rBV2	75219	75541	3.07%	0.414%
25	12.663	1793	1798	1801	rBV	2633092	2384994	97.01%	13.070%
26	12.722	1806	1808	1811	rVB2	50036	39806	1.62%	0.218%
27	12.780	1815	1818	1819	rBV2	25008	27460	1.12%	0.150%
28	12.810	1819	1823	1826	rVV2	103356	119974	4.88%	0.657%
29	12.892	1830	1837	1842	rBV	2250462	2458488	100.00%	13.473%
30	12.933	1842	1844	1849	rVB2	83265	97265	3.96%	0.533%
31	13.004	1852	1856	1858	rBV	135851	119530	4.86%	0.655%
32	13.045	1861	1863	1867	rVB	116611	98649	4.01%	0.541%
33	13.110	1867	1874	1876	rBV2	95106	171135	6.96%	0.938%
34	13.133	1876	1878	1881	rVB	57974	44943	1.83%	0.246%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092317\
 Data File : BF098767.D
 Acq On : 24 Sep 2017 5:30
 Operator : SJ/JU
 Sample : I5304-05DL 100X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SASP2P-ENV-118-6(5-10)DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.192	1885	1888	1889	rVV2	71187	82182	3.34%	0.450%
36	13.216	1889	1892	1895	rVB	264725	242175	9.85%	1.327%
37	13.280	1899	1903	1906	rBV	228722	190403	7.74%	1.043%
38	13.316	1906	1909	1912	rVV2	128649	153732	6.25%	0.842%
39	13.345	1912	1914	1917	rVB2	56358	45710	1.86%	0.251%
40	13.410	1922	1925	1928	rBV	69481	55929	2.27%	0.307%
41	13.439	1928	1930	1934	rBV2	76272	81053	3.30%	0.444%
42	13.516	1940	1943	1947	rVB3	33244	44072	1.79%	0.242%
43	13.616	1953	1960	1962	rBV5	28420	53606	2.18%	0.294%
44	13.721	1974	1978	1982	rVB	80202	101123	4.11%	0.554%
45	13.833	1992	1997	2000	rBV3	138685	177912	7.24%	0.975%
46	13.863	2000	2002	2004	rVV	158011	130545	5.31%	0.715%
47	13.886	2004	2006	2010	rVV2	147896	188212	7.66%	1.031%
48	13.927	2010	2013	2020	rVB2	118345	129225	5.26%	0.708%
49	14.004	2020	2026	2031	rBV	47926	96808	3.94%	0.531%
50	14.080	2031	2039	2042	rVV3	1204088	1801422	73.27%	9.872%
51	14.110	2042	2044	2050	rVB	792729	706291	28.73%	3.871%
52	14.192	2055	2058	2061	rBV	141936	111404	4.53%	0.611%
53	14.269	2068	2071	2074	rVB2	63482	69016	2.81%	0.378%
54	14.304	2074	2077	2081	rBV2	78346	91234	3.71%	0.500%
55	14.433	2096	2099	2101	rBV	30234	25229	1.03%	0.138%
56	14.468	2101	2105	2108	rVV	89236	100349	4.08%	0.550%
57	14.504	2108	2111	2115	rVV	54389	54129	2.20%	0.297%
58	14.563	2117	2121	2124	rVV2	55067	79521	3.23%	0.436%
59	14.592	2124	2126	2128	rVV	57345	62577	2.55%	0.343%
60	14.616	2128	2130	2134	rVV4	74179	77317	3.14%	0.424%
61	14.668	2134	2139	2143	rVB3	32960	60904	2.48%	0.334%
62	14.774	2154	2157	2161	rBV3	41841	57007	2.32%	0.312%
63	15.139	2214	2219	2222	rBV	330687	552136	22.46%	3.026%
64	15.245	2234	2237	2240	rBV	52857	55444	2.26%	0.304%
65	15.445	2267	2271	2277	rVB	163370	209900	8.54%	1.150%
66	15.510	2278	2282	2289	rVB	239936	290410	11.81%	1.592%
67	15.580	2289	2294	2297	rBV	468971	629310	25.60%	3.449%
68	17.080	2544	2549	2557	rVB2	61561	129683	5.27%	0.711%
69	17.533	2622	2626	2633	rVB2	35407	66158	2.69%	0.363%


Sum of corrected areas: 18247212

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092317\
Data File : BF098767.D
Acq On : 24 Sep 2017 5:30
Operator : SJ/JU
Sample : I5304-05DL 100X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SASP2P-ENV-118-6(5-10)DL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

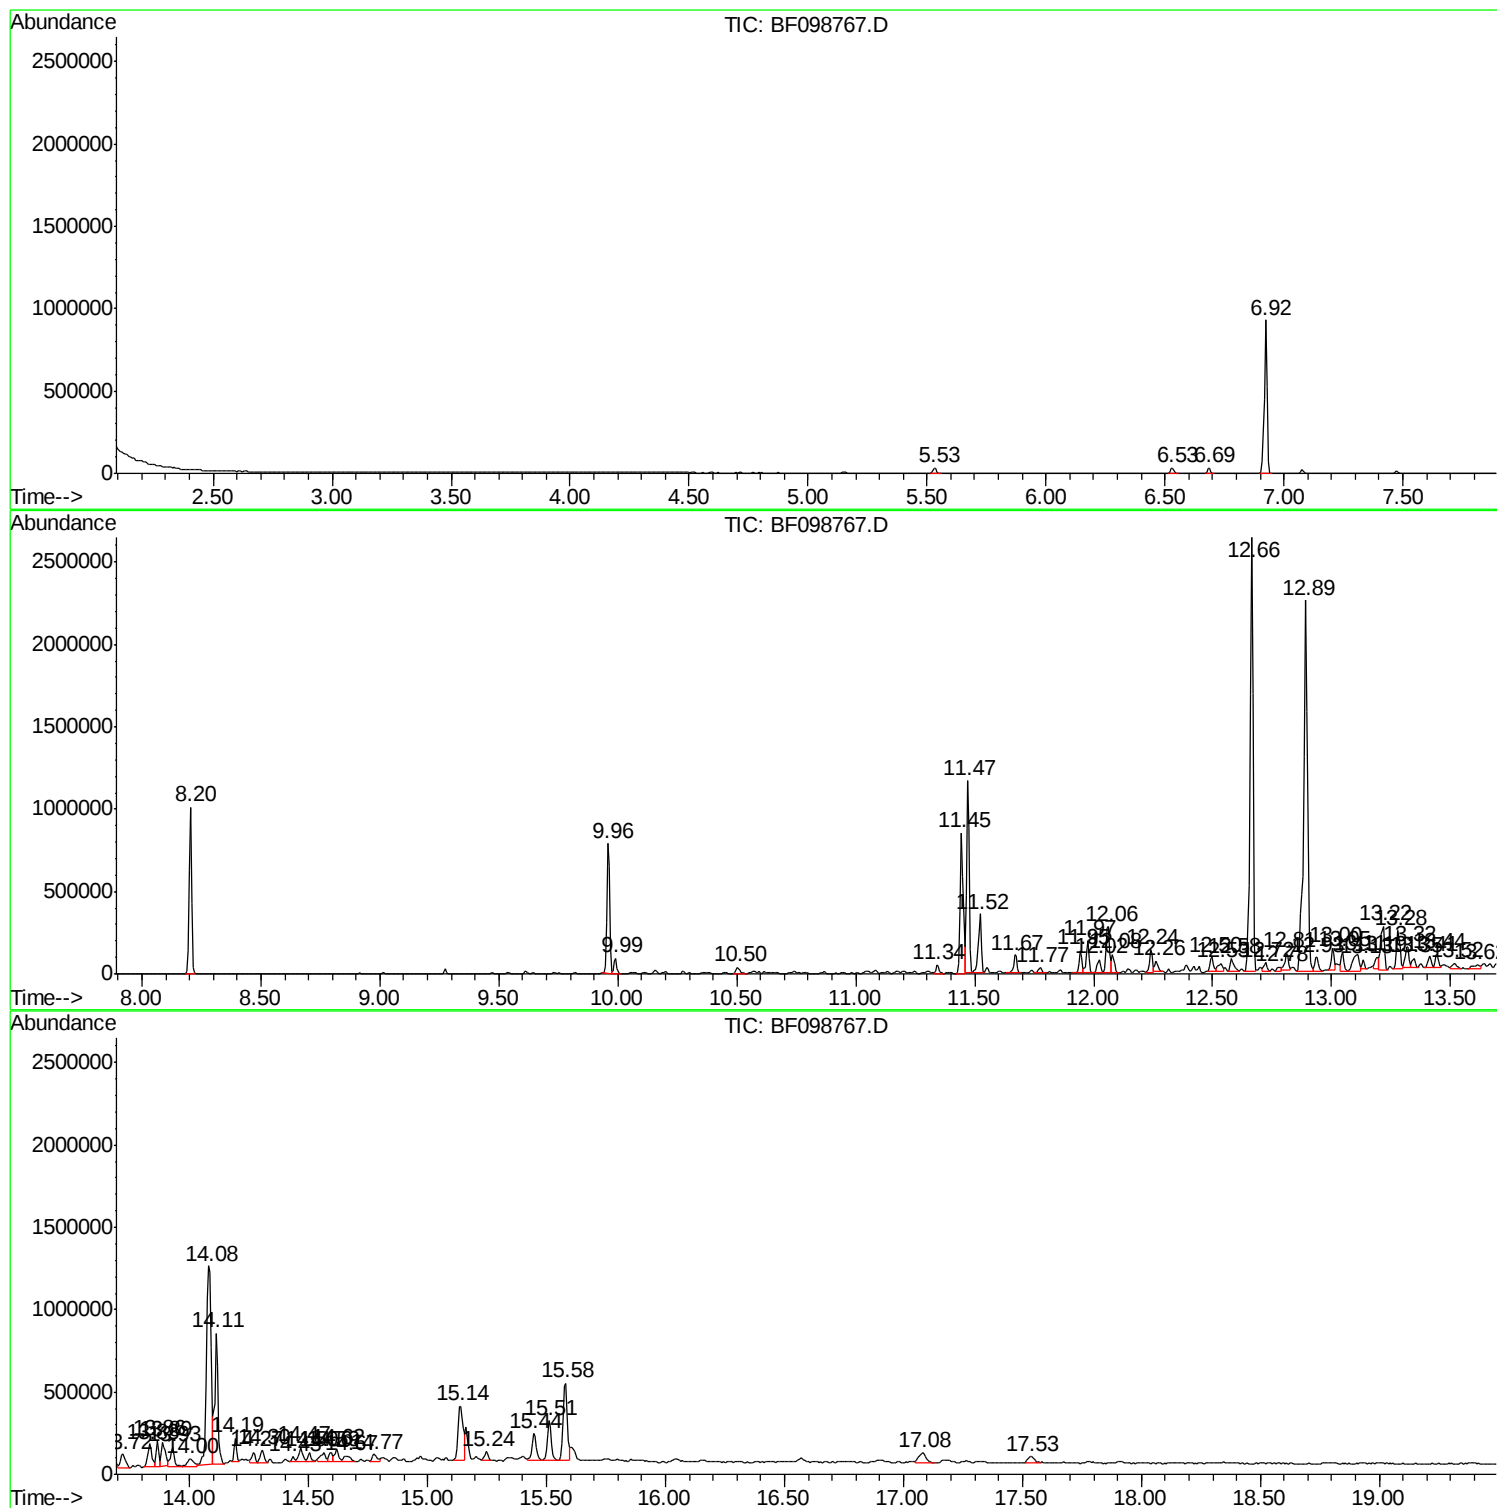

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF092317\
Data_File : BF098767.D
Acq_On : 24 Sep 2017 5:300
Operator : SJ/JUU
Sample : I5304-05DL_100XX
Misc :
ALS_Vial : 29 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SASP2P-ENV-118-6(5-10)DL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
