


Data Path : Z:\HPCHEM1\BNA F\Data\BF092317\
 Data File : BF098728.D
 Acq On : 23 Sep 2017 10:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

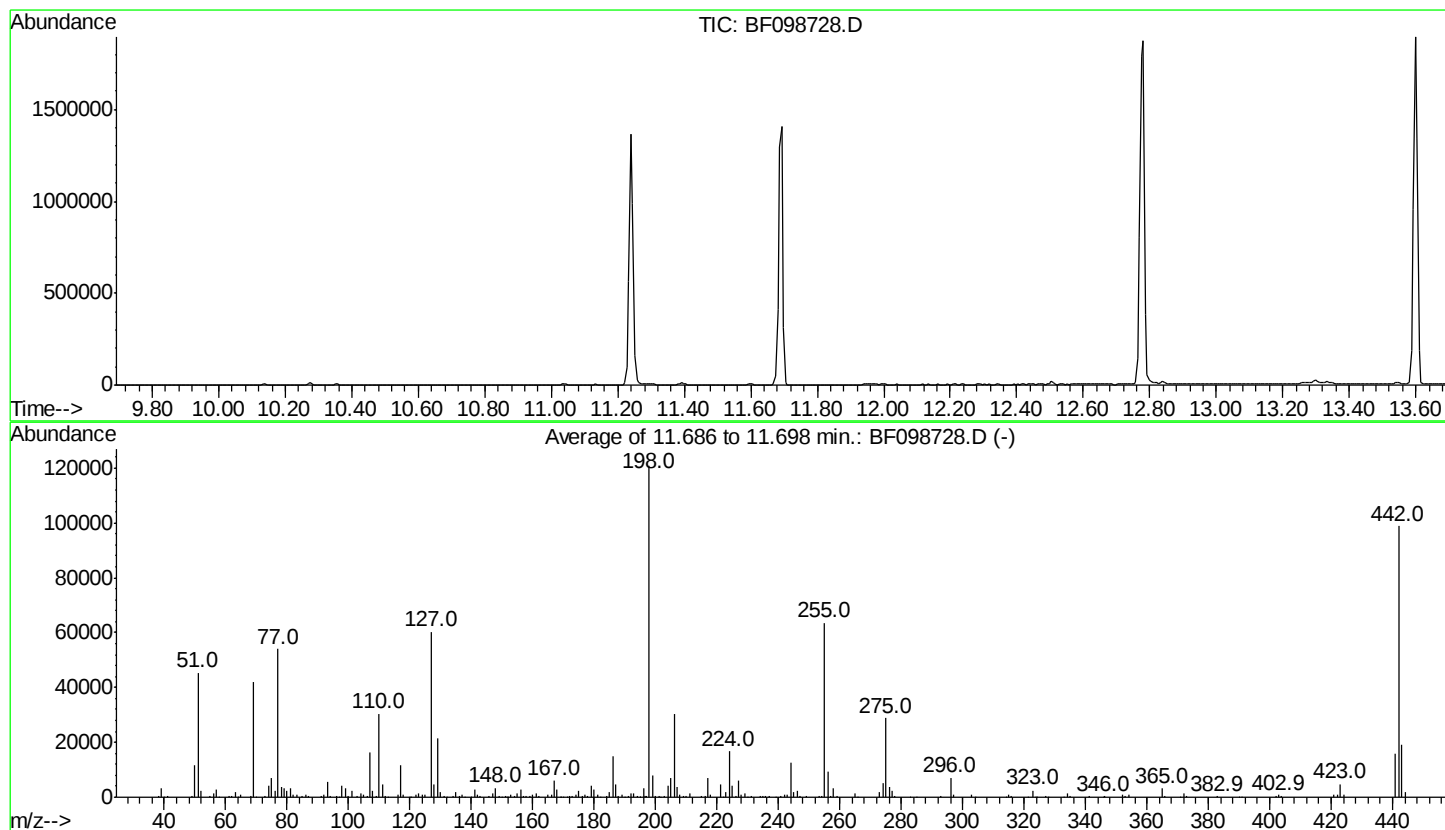

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	45378	PASS
68	69	0.00	2	1.6	692	PASS
69	198	0.00	100	34.9	42232	PASS
70	69	0.00	2	0.3	110	PASS
127	198	10	80	49.9	60347	PASS
197	198	0.00	2	0.5	570	PASS
198	198	100	100	100.0	120898	PASS
199	198	5	9	6.5	7907	PASS
275	198	10	60	23.8	28778	PASS
365	198	1	100	2.6	3104	PASS
441	442	0.01	24	16.1	15965	PASS
442	198	50	100	81.8	98912	PASS
443	442	15	24	19.4	19146	PASS