


Data Path : Z:\HPCHEM1\BNA F\Data\BF092317\
 Data File : BF098737.D
 Acq On : 23 Sep 2017 14:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

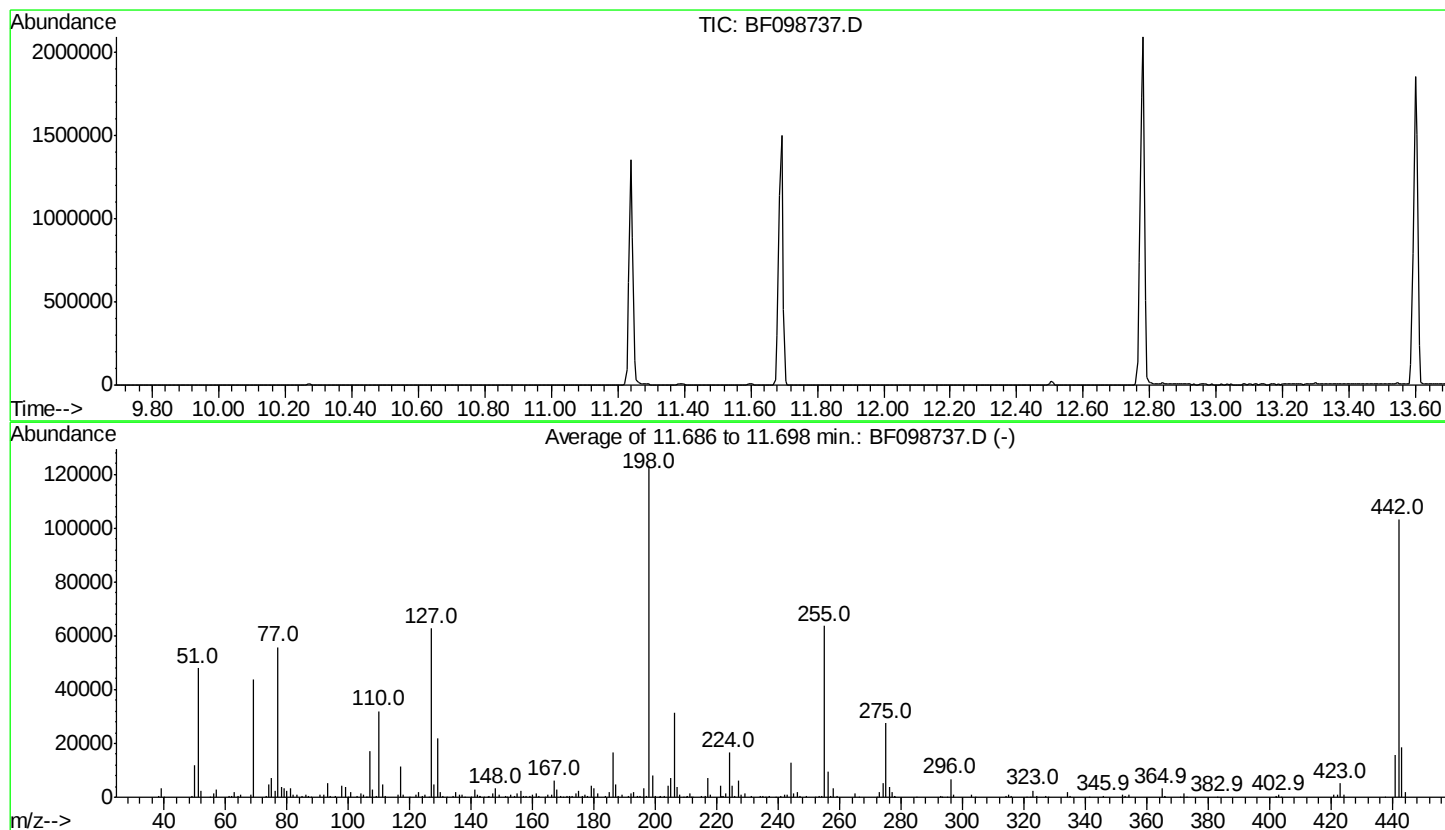

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	47814	PASS
68	69	0.00	2	1.7	750	PASS
69	198	0.00	100	35.4	43565	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	62538	PASS
197	198	0.00	2	0.5	658	PASS
198	198	100	100	100.0	123154	PASS
199	198	5	9	6.6	8164	PASS
275	198	10	60	22.3	27417	PASS
365	198	1	100	2.6	3160	PASS
441	442	0.01	24	15.1	15603	PASS
442	198	50	100	83.7	103026	PASS
443	442	15	24	18.1	18652	PASS