


Data Path : Z:\HPCHEM1\BNA F\Data\BF092317\
 Data File : BF098763.D
 Acq On : 24 Sep 2017 3:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

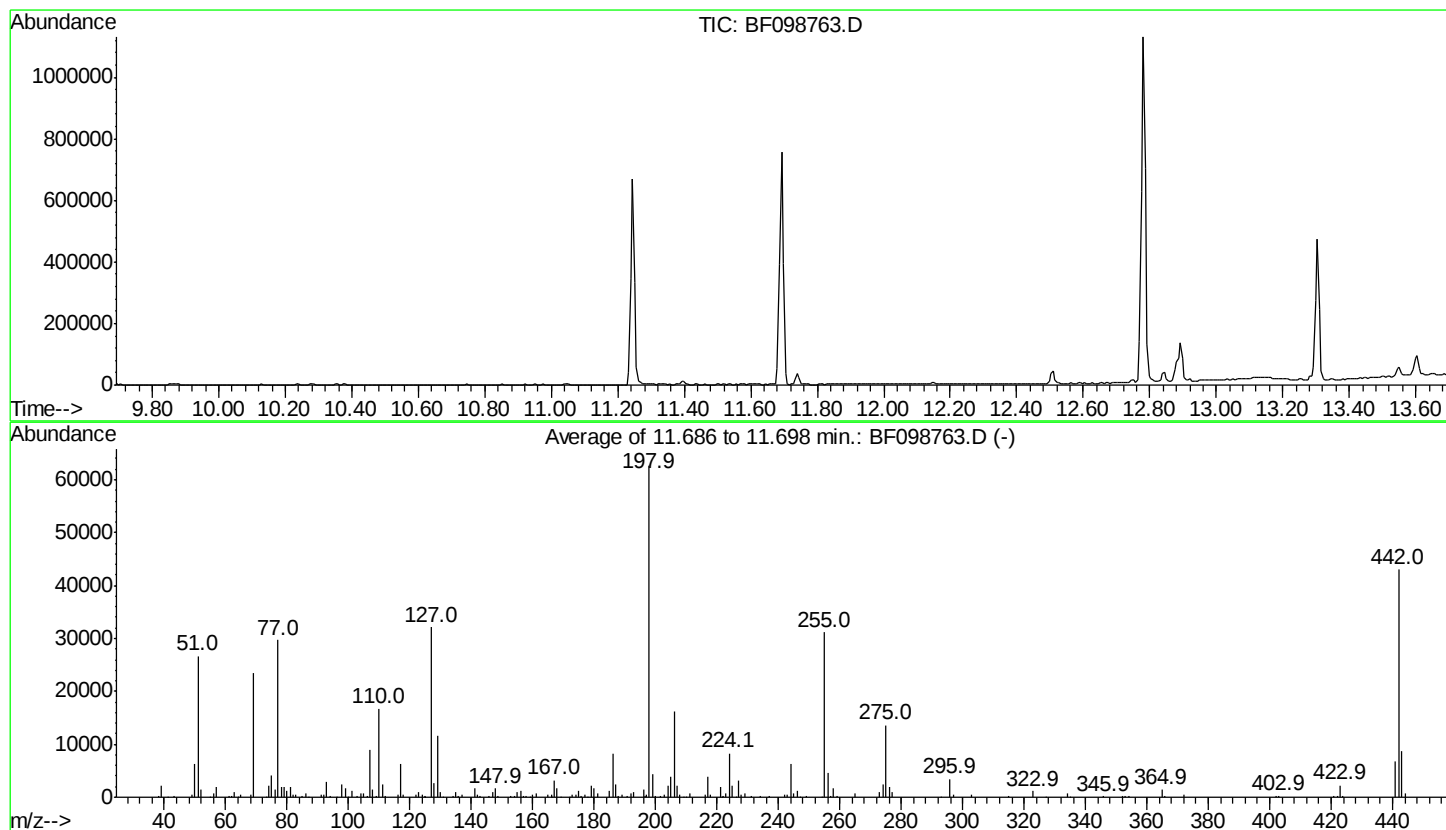

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	26708	PASS
68	69	0.00	2	2.0	478	PASS
69	198	0.00	100	37.3	23395	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	32064	PASS
197	198	0.00	2	0.6	406	PASS
198	198	100	100	100.0	62666	PASS
199	198	5	9	7.1	4446	PASS
275	198	10	60	21.6	13566	PASS
365	198	1	100	2.3	1416	PASS
441	442	0.01	24	15.8	6785	PASS
442	198	50	100	68.7	43038	PASS
443	442	15	24	20.1	8636	PASS