
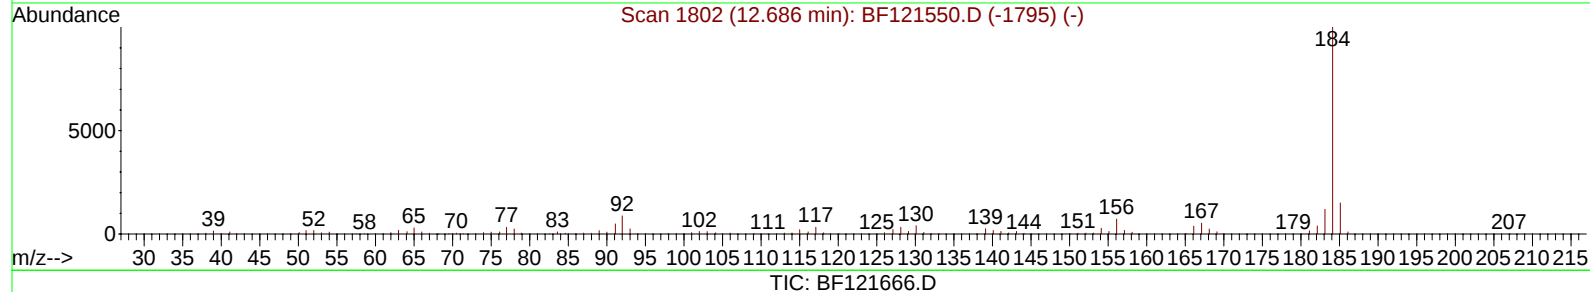
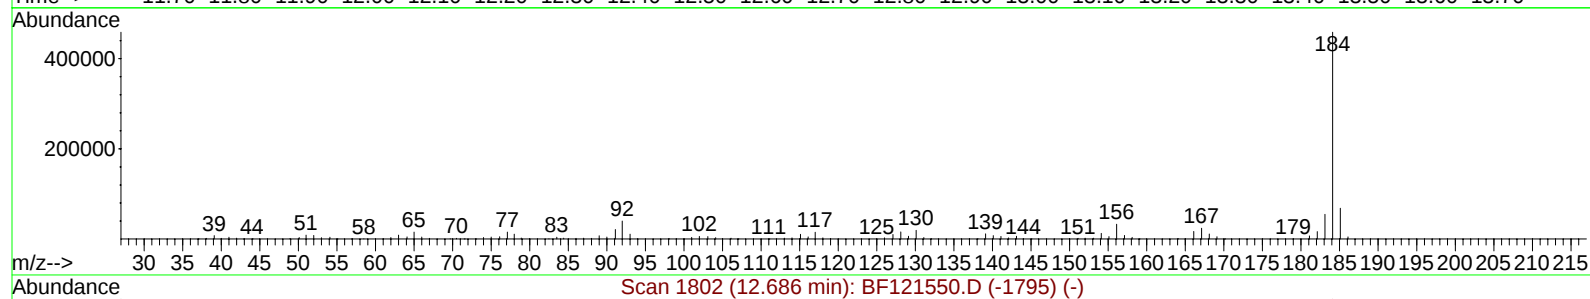


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092320\
Data File : BF121666.D
Acq On : 23 Sep 2020 12:54
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 18:38:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 22 17:53:26 2020
Response via : Initial Calibration

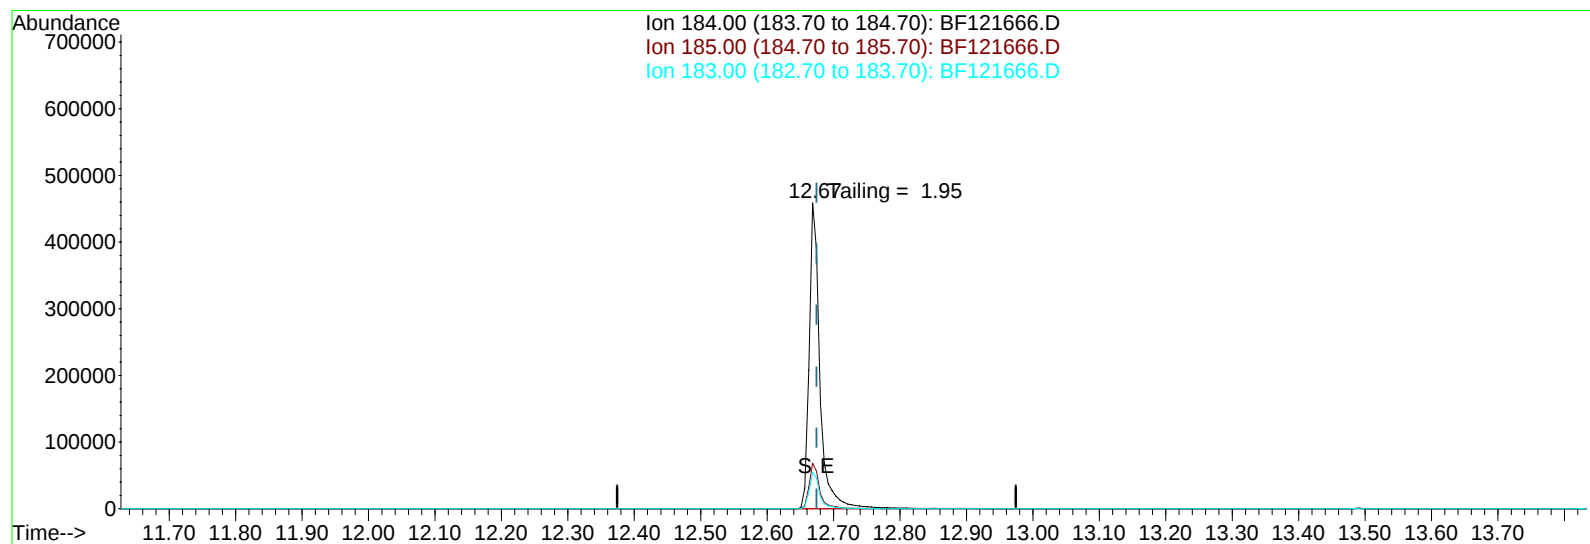

(77) Benzidine




12.668min (-0.006) 0.00ng

response 517416

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.91
183.00	12.00	11.98
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092320\
Data File : BF121666.D
Acq On : 23 Sep 2020 12:54
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 18:38:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 22 17:53:26 2020
Response via : Initial Calibration

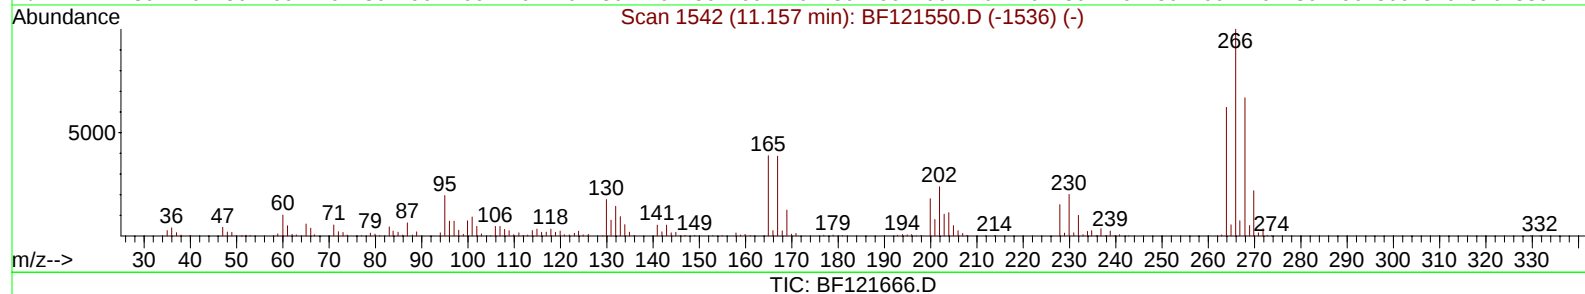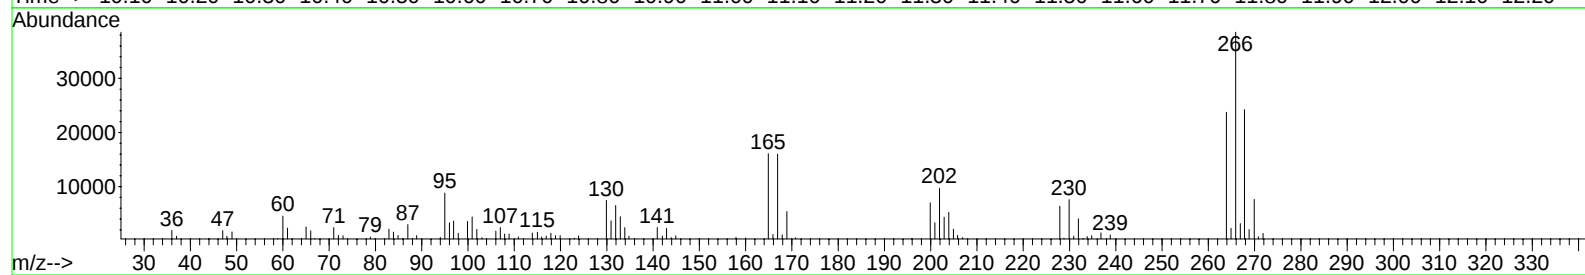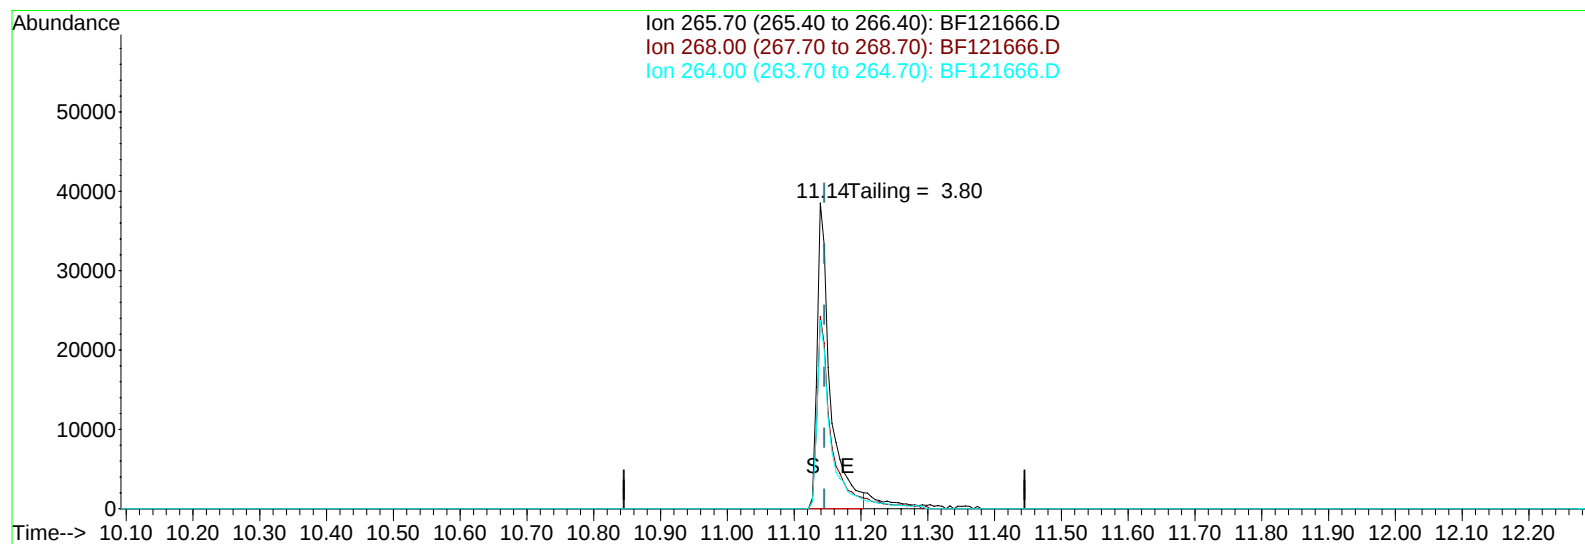

(70) Pentachlorophenol (C)

11.139min (-0.006) 64766.18ng

response 57127

Ion	Exp%	Act%
265.70	100	100
268.00	68.20	62.85
264.00	63.90	61.61
0.00	0.00	0.00