

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092320\
 Data File : BF121668.D
 Acq On : 23 Sep 2020 15:30
 Operator : JU/CG
 Sample : PB131842BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB131842BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.181	14	16	31	rVB3	33001	65642	1.27%	0.214%
2	5.057	501	505	513	rBV	45354	61307	1.19%	0.200%
3	5.440	566	570	574	rBV	3599338	3855955	74.58%	12.563%
4	6.445	736	741	744	rBV	3357551	3916044	75.75%	12.759%
5	6.804	799	802	806	rBV	993004	878509	16.99%	2.862%
6	7.375	893	899	902	rBV	2514206	2729841	52.80%	8.894%
7	8.092	1015	1021	1041	rBV	1073029	1160366	22.44%	3.781%
8	9.169	1197	1204	1207	rBV	4286763	4731694	91.52%	15.417%
9	9.845	1313	1319	1329	rBV	1368473	1314392	25.42%	4.283%
10	10.639	1447	1454	1478	rBV	2913685	2972876	57.50%	9.686%
11	11.333	1565	1572	1590	rBV	1362371	1366250	26.43%	4.451%
12	12.921	1834	1842	1845	rBV	4727351	5170029	100.00%	16.845%
13	13.968	2016	2020	2032	rVB	1207041	1276765	24.70%	4.160%
14	15.427	2262	2268	2282	rBV	856573	1192465	23.06%	3.885%


Sum of corrected areas: 30692135

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092320\
Data File : BF121668.D
Acq On : 23 Sep 2020 15:30
Operator : JU/CG
Sample : PB131842BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131842BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

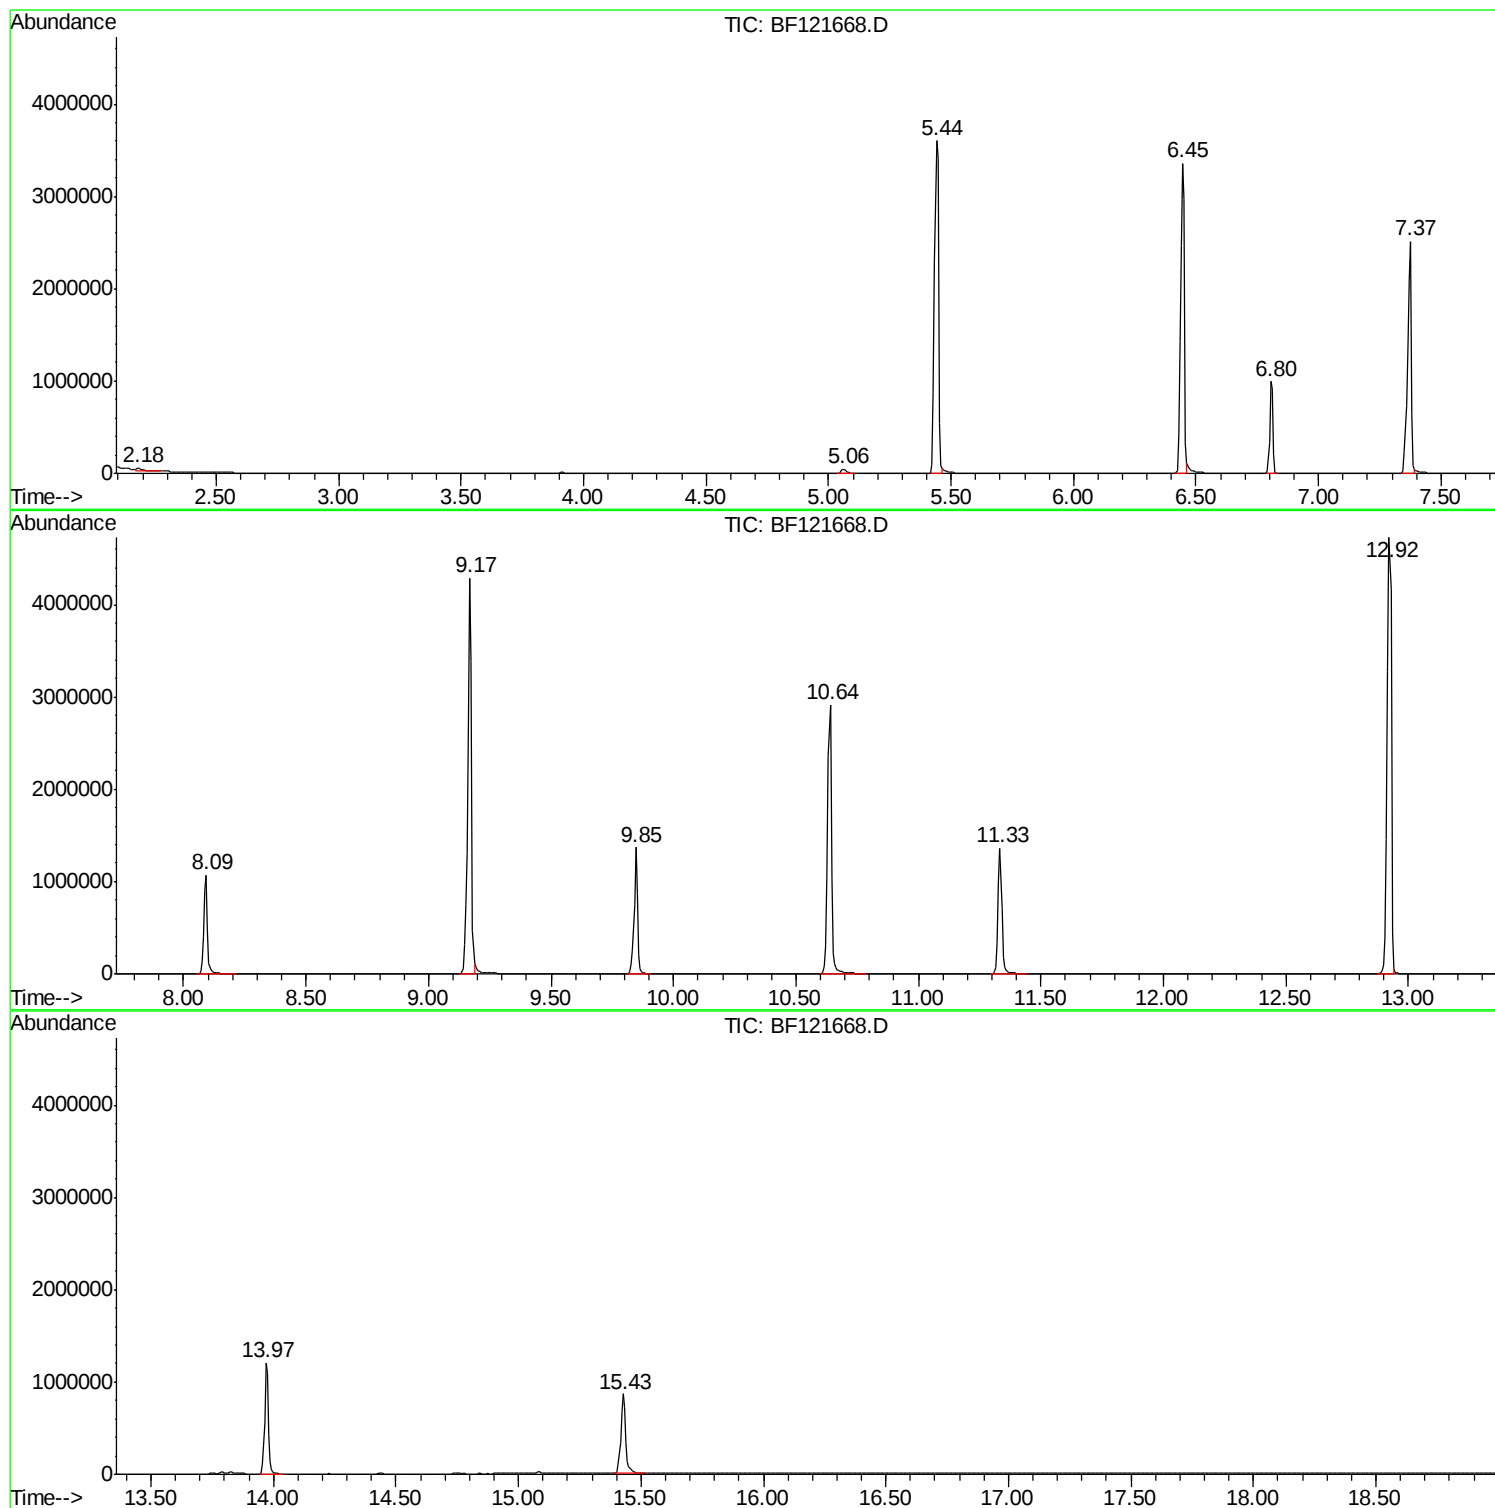

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092320\
Data File : BF121668.D
Acq On : 23 Sep 2020 15:30
Operator : JU/CG
Sample : PB131842BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131842BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092320\
Data File : BF121668.D
Acq On : 23 Sep 2020 15:30
Operator : JU/CG
Sample : PB131842BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB131842BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc