


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092320\
 Data File : BF121666.D
 Acq On : 23 Sep 2020 12:54
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 17:53:26 2020

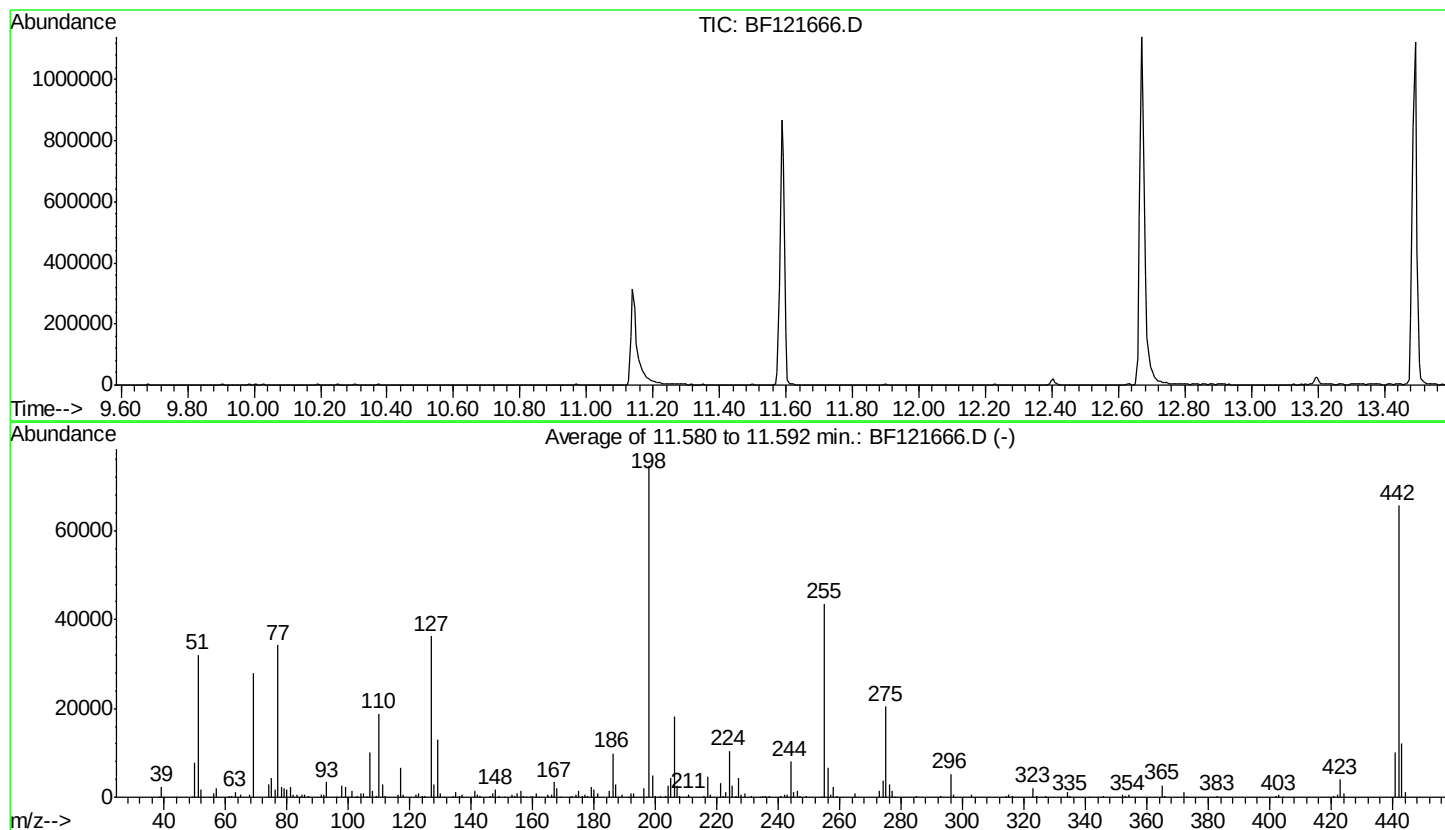

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	32061	PASS
68	69	0.00	2	1.7	484	PASS
69	198	0.00	100	37.3	27874	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	36298	PASS
197	198	0.00	2	0.1	109	PASS
198	198	100	100	100.0	74706	PASS
199	198	5	9	6.6	4948	PASS
275	198	10	60	27.3	20404	PASS
365	198	1	100	3.6	2678	PASS
441	198	0.01	100	13.6	10185	PASS
442	198	50	100	88.0	65710	PASS
443	442	15	24	18.3	12035	PASS