

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
 Data File : BF125584.D
 Acq On : 23 Sep 2021 10:40
 Operator : JU/CG
 Sample : PB139258BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139258BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.269	22	31	36	rVB	120255	165768	2.07%	0.339%
2	5.522	578	584	587	rBV	5367883	6294987	78.55%	12.856%
3	6.516	747	753	756	rBV	4905902	6213107	77.53%	12.689%
4	6.892	814	817	821	rVB	1789225	1568820	19.58%	3.204%
5	7.457	907	913	916	rBV	3826187	4133048	51.57%	8.441%
6	8.175	1030	1035	1039	rBV	2414572	2271277	28.34%	4.639%
7	9.257	1212	1219	1222	rBV	7424575	8014204	100.00%	16.367%
8	9.933	1328	1334	1337	rBV	3022698	2650162	33.07%	5.412%
9	10.722	1462	1468	1471	rBV	4759728	4645165	57.96%	9.487%
10	11.416	1582	1586	1590	rBV	2824033	2535812	31.64%	5.179%
11	13.010	1852	1857	1860	rBV	7308149	7355812	91.78%	15.022%
12	14.057	2031	2035	2038	rBV	1979132	1729144	21.58%	3.531%
13	15.539	2281	2287	2292	rBV	1013291	1388243	17.32%	2.835%




Sum of corrected areas: 48965549

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
Data File : BF125584.D
Acq On : 23 Sep 2021 10:40
Operator : JU/CG
Sample : PB139258BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139258BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

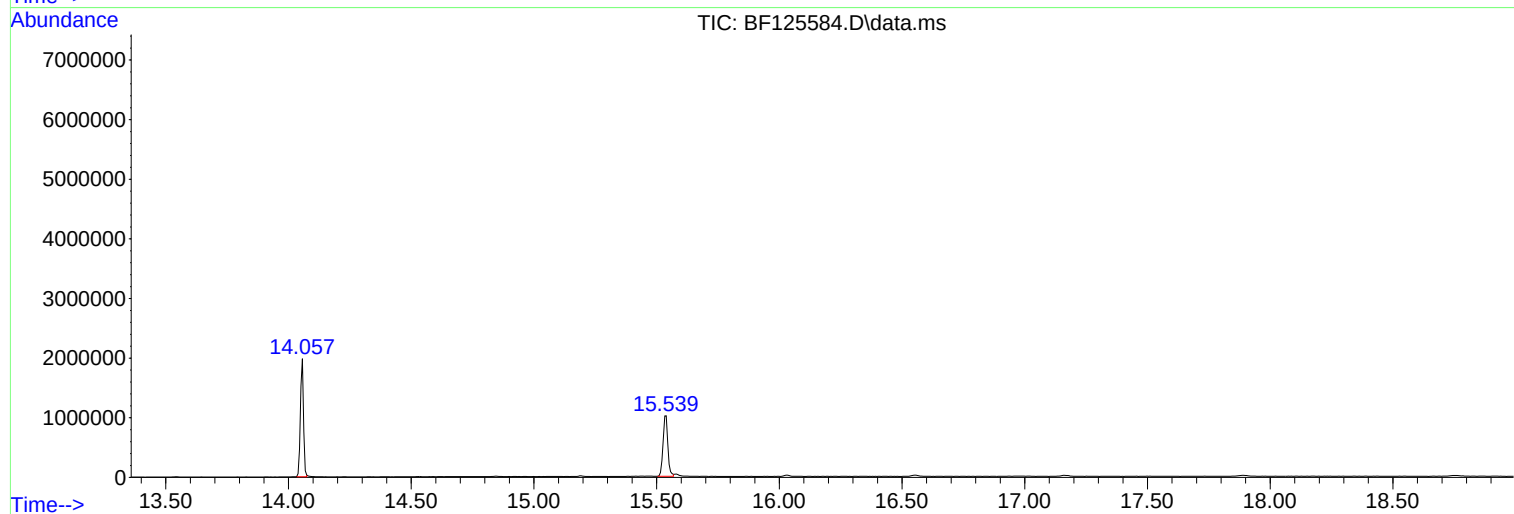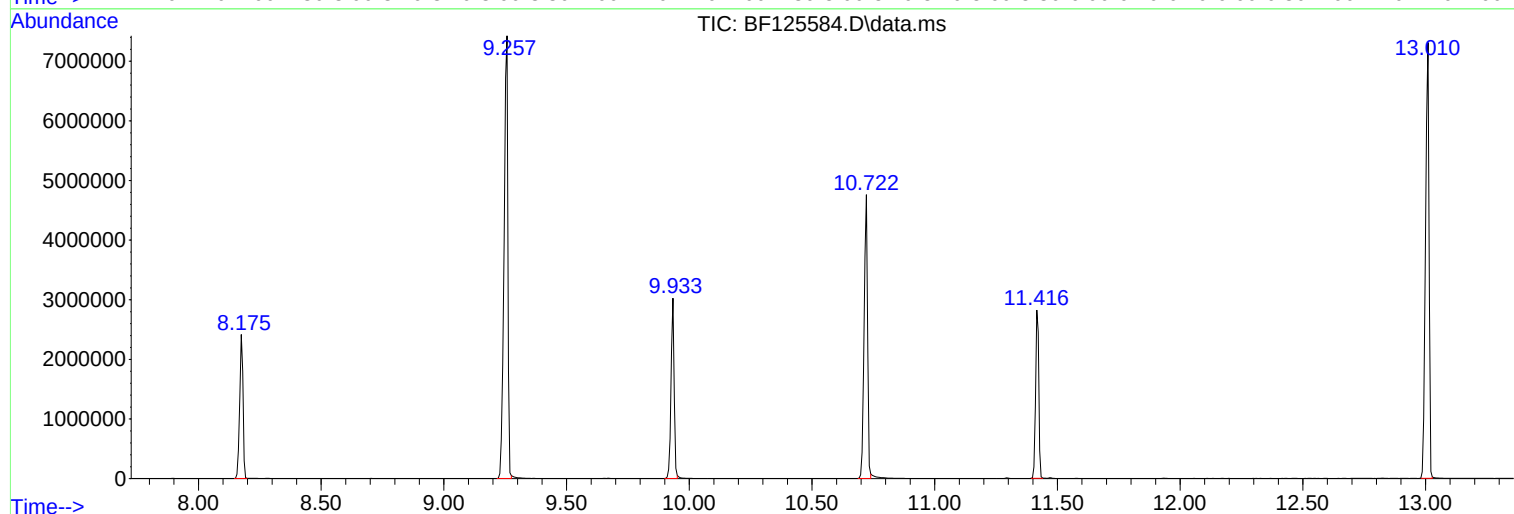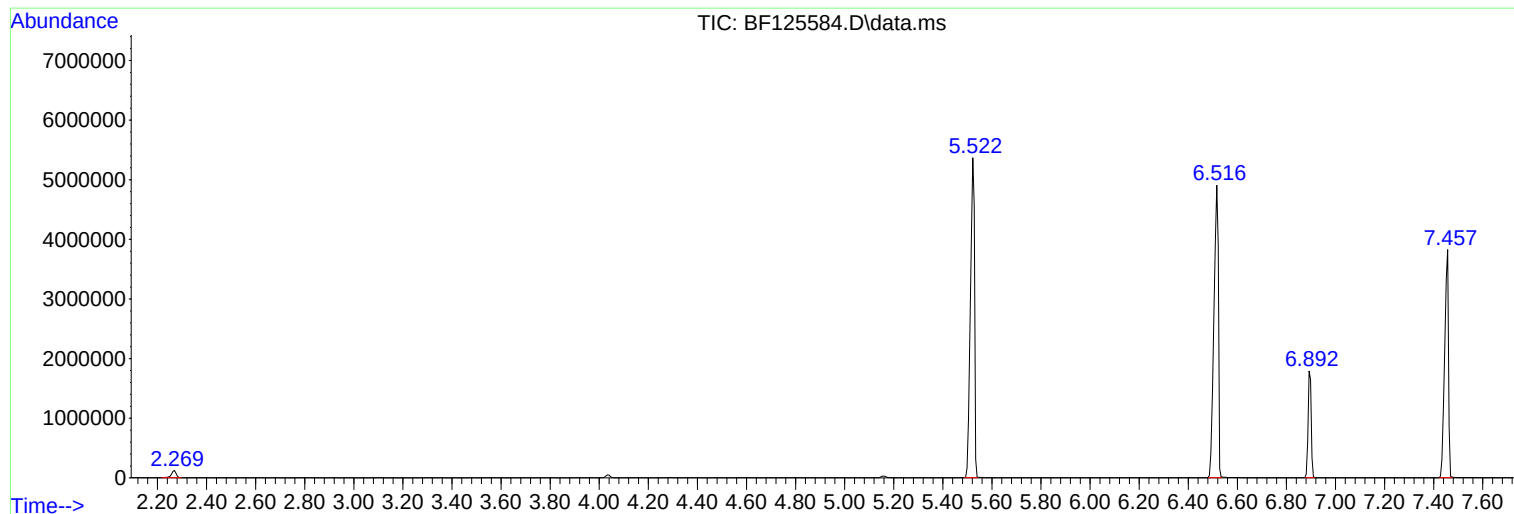

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
Data File : BF125584.D
Acq On : 23 Sep 2021 10:40
Operator : JU/CG
Sample : PB139258BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139258BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.269	2.11 ng	165768	1,4-Dichlorobenzene-d4	6.892

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Silane, tetramethyl-	88	C4H12Si	000075-76-3	38
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	17

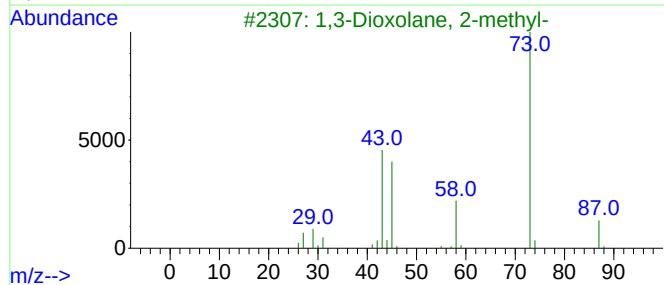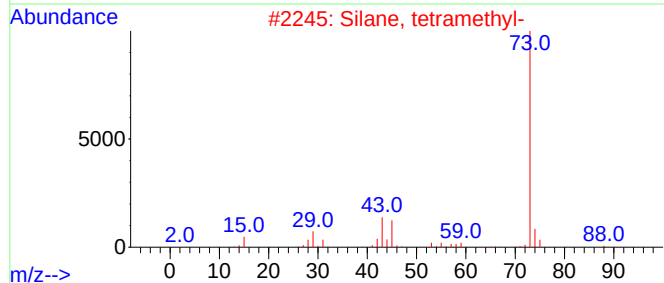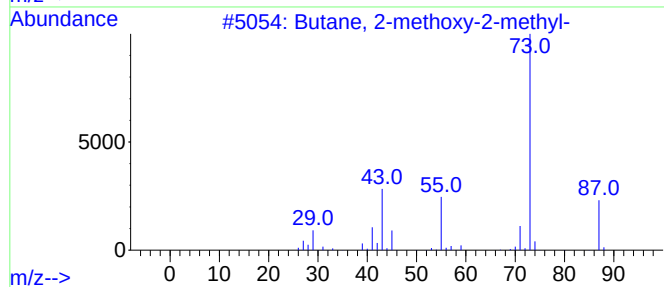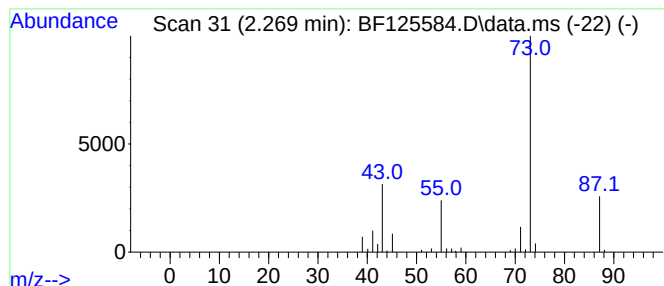

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
Data File : BF125584.D
Acq On : 23 Sep 2021 10:40
Operator : JU/CG
Sample : PB139258BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139258BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.269	2.1	ng	165768	1	6.892	1568820	20.0