

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
 Data File : BF125594.D
 Acq On : 23 Sep 2021 16:16
 Operator : JU/CG
 Sample : PB139286BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139286BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.269	20	31	36	rBV	119369	170028	2.11%	0.343%
2	5.522	578	584	587	rBV	5393536	6292537	78.19%	12.702%
3	6.516	747	753	756	rBV	4912599	6229641	77.41%	12.575%
4	6.892	814	817	821	rBV	1745938	1576917	19.59%	3.183%
5	7.457	907	913	916	rBV	3904675	4149548	51.56%	8.376%
6	8.175	1030	1035	1039	rBV	2373747	2282657	28.36%	4.608%
7	9.257	1212	1219	1222	rBV	7615488	8047615	100.00%	16.245%
8	9.933	1328	1334	1337	rBV	3129970	2649522	32.92%	5.348%
9	10.721	1462	1468	1471	rBV	4764133	4565904	56.74%	9.217%
10	11.421	1582	1587	1590	rBV	2871881	2563418	31.85%	5.174%
11	13.010	1852	1857	1860	rBV	7187472	7621383	94.70%	15.384%
12	14.057	2031	2035	2048	rVB	2046540	1843466	22.91%	3.721%
13	15.539	2281	2287	2293	rBV	1053349	1444770	17.95%	2.916%
14	17.192	2557	2568	2570	rBV6	33842	102348	1.27%	0.207%




Sum of corrected areas: 49539754

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
Data File : BF125594.D
Acq On : 23 Sep 2021 16:16
Operator : JU/CG
Sample : PB139286BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139286BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

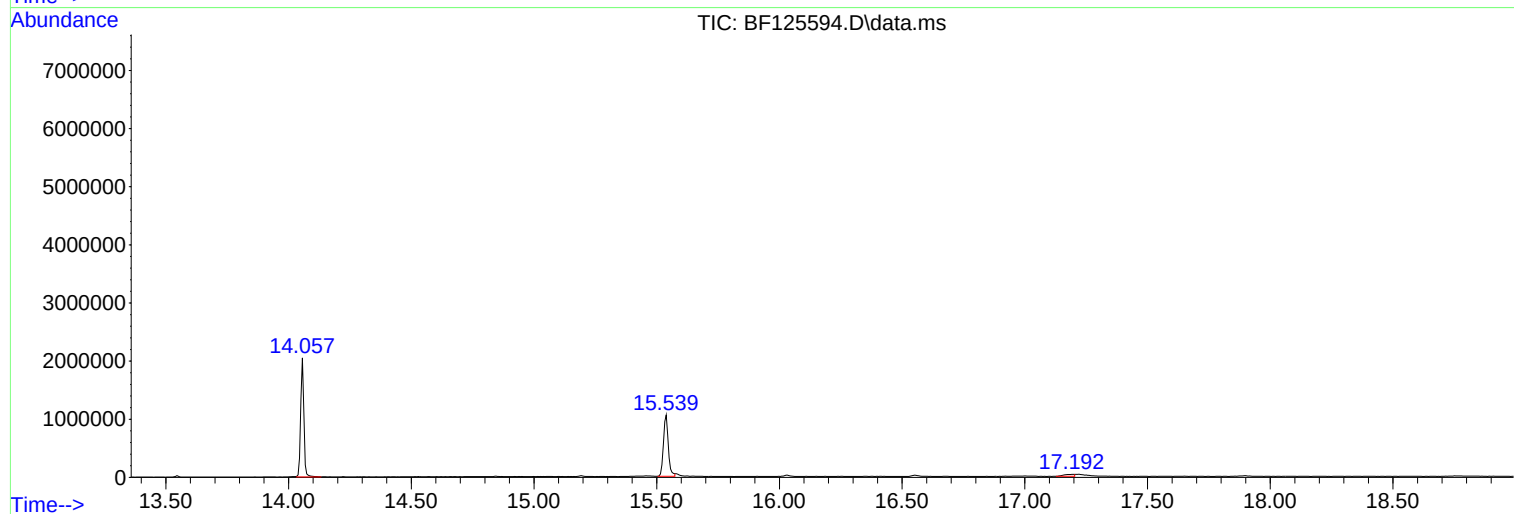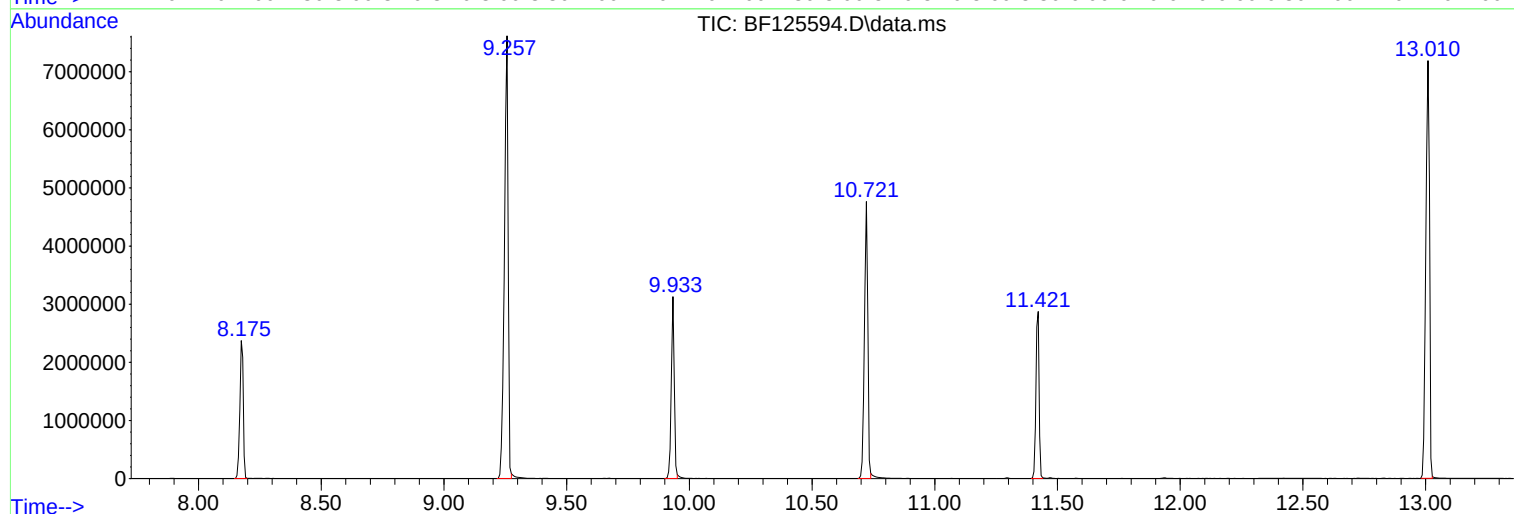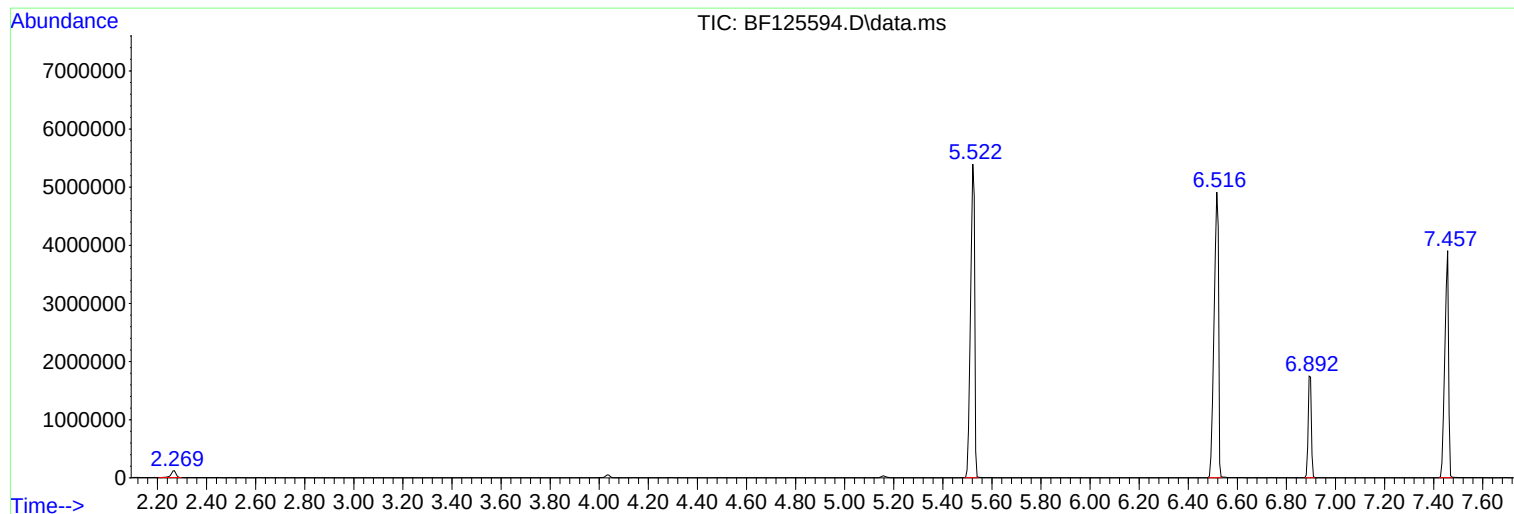

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
Data File : BF125594.D
Acq On : 23 Sep 2021 16:16
Operator : JU/CG
Sample : PB139286BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139286BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.269	2.16 ng	170028	1,4-Dichlorobenzene-d4	6.898

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	17

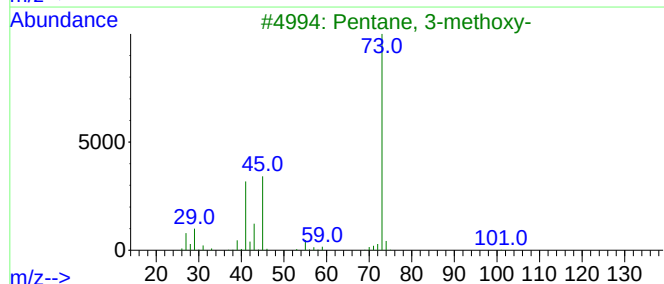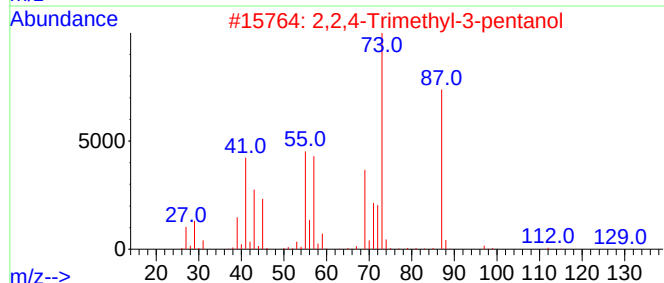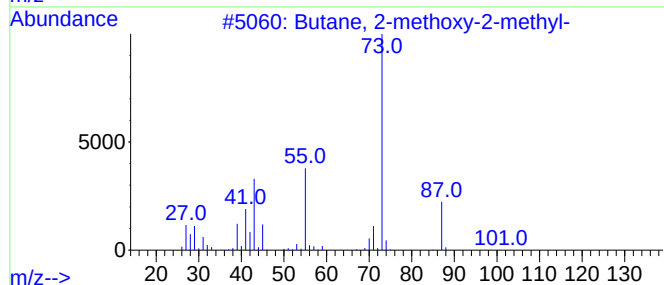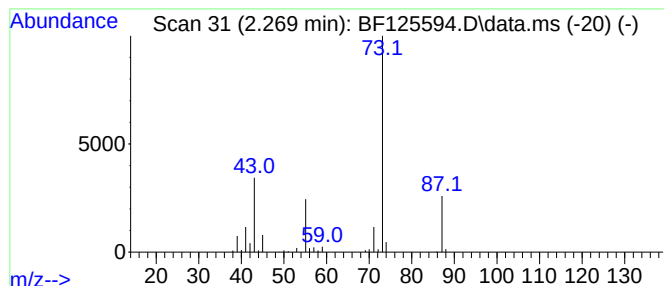

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
Data File : BF125594.D
Acq On : 23 Sep 2021 16:16
Operator : JU/CG
Sample : PB139286BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139286BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.269	2.2	ng	170028	1	6.898	1576920	20.0