
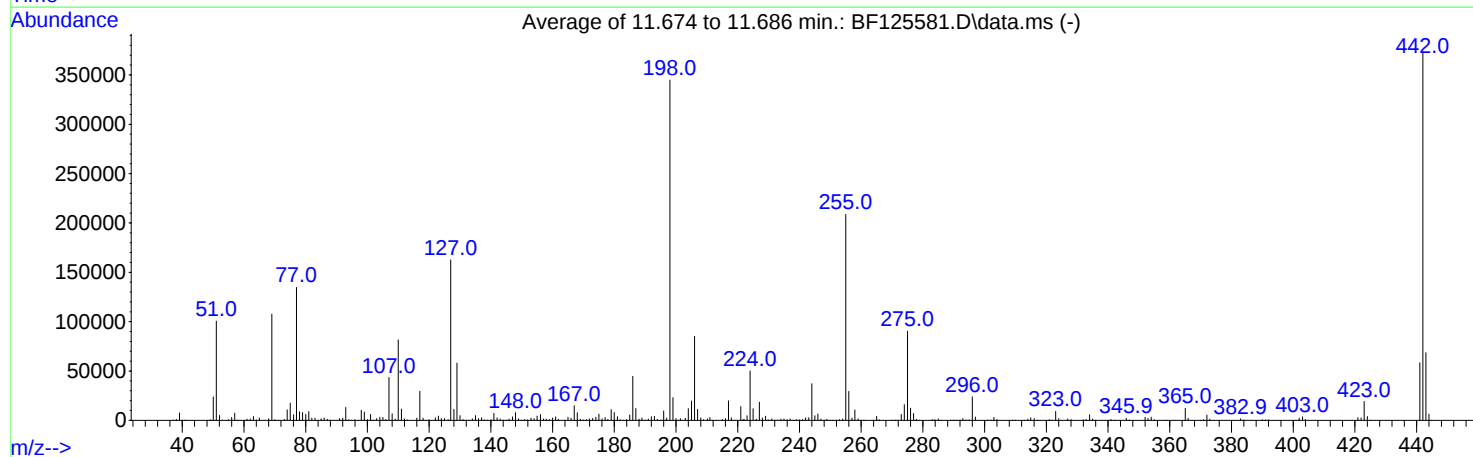


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
 Data File : BF125581.D
 Acq On : 23 Sep 2021 9:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 21 19:21:36 2021

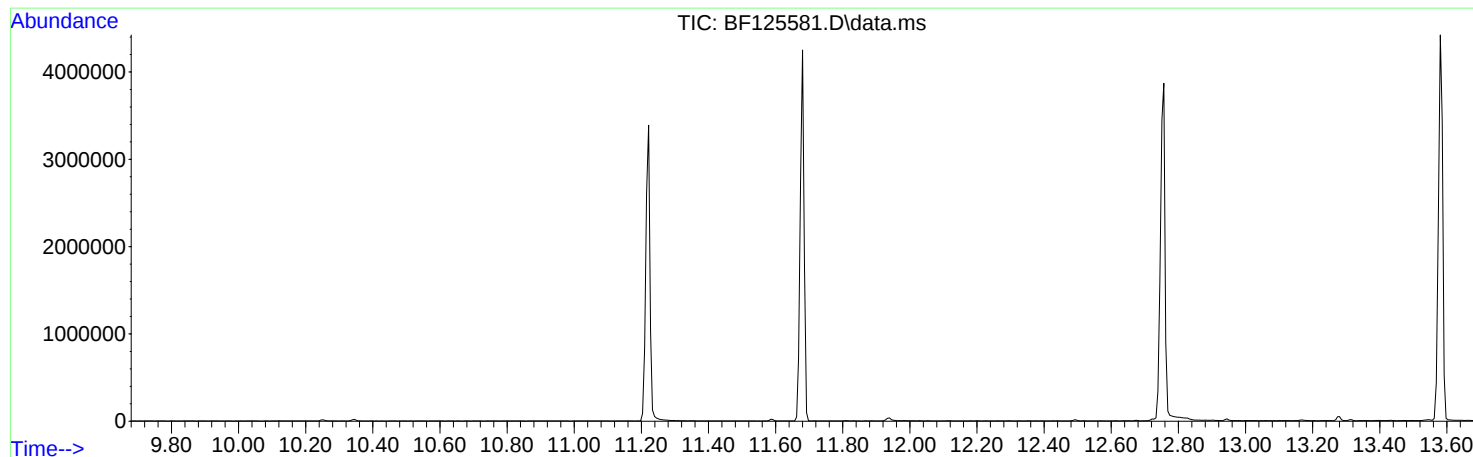




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	100477	PASS
68	69	0.00	2	1.5	1618	PASS
69	198	0.00	100	31.2	107592	PASS
70	69	0.00	2	0.6	652	PASS
127	198	10	80	47.2	162688	PASS
197	198	0.00	2	0.7	2367	PASS
198	198	100	100	100.0	344853	PASS
199	198	5	9	6.7	23112	PASS
275	198	10	60	26.2	90333	PASS
365	198	1	100	3.5	12176	PASS
441	198	0.01	100	16.9	58296	PASS
442	442	50	100	100.0	372736	PASS
443	442	15	24	18.4	68557	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
Data File : BF125581.D
Acq On : 23 Sep 2021 9:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 23 11:28:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 19:21:36 2021
Response via : Initial Calibration

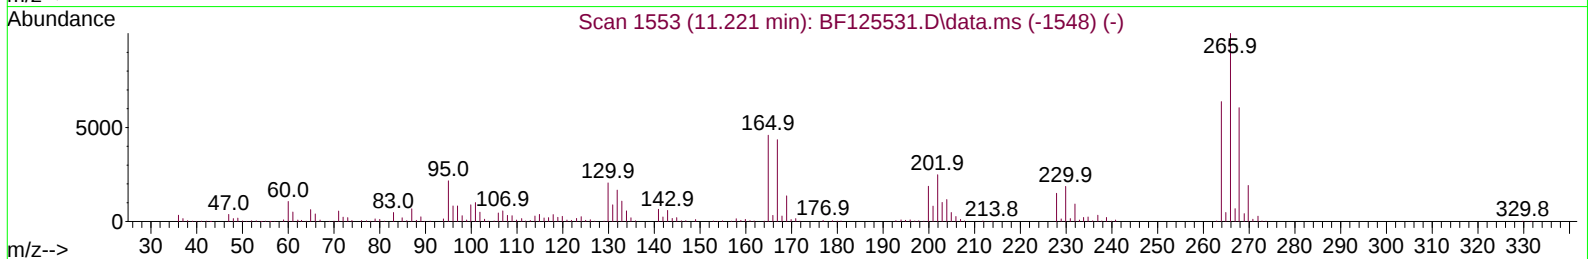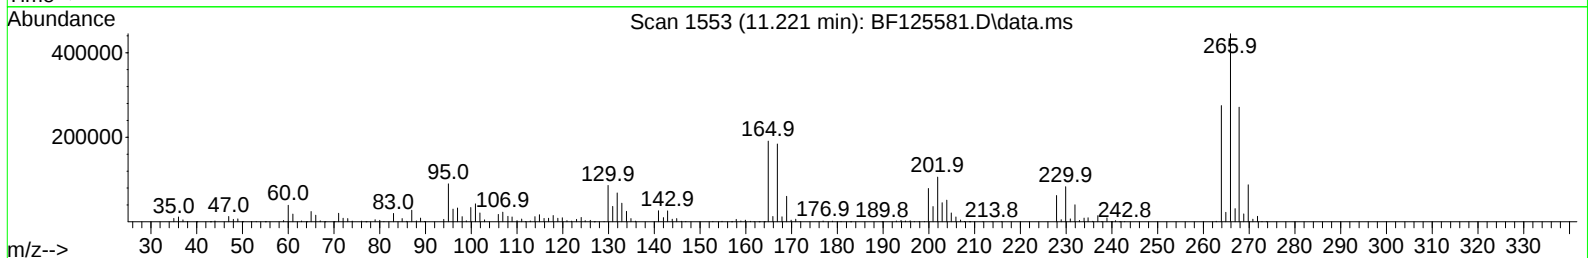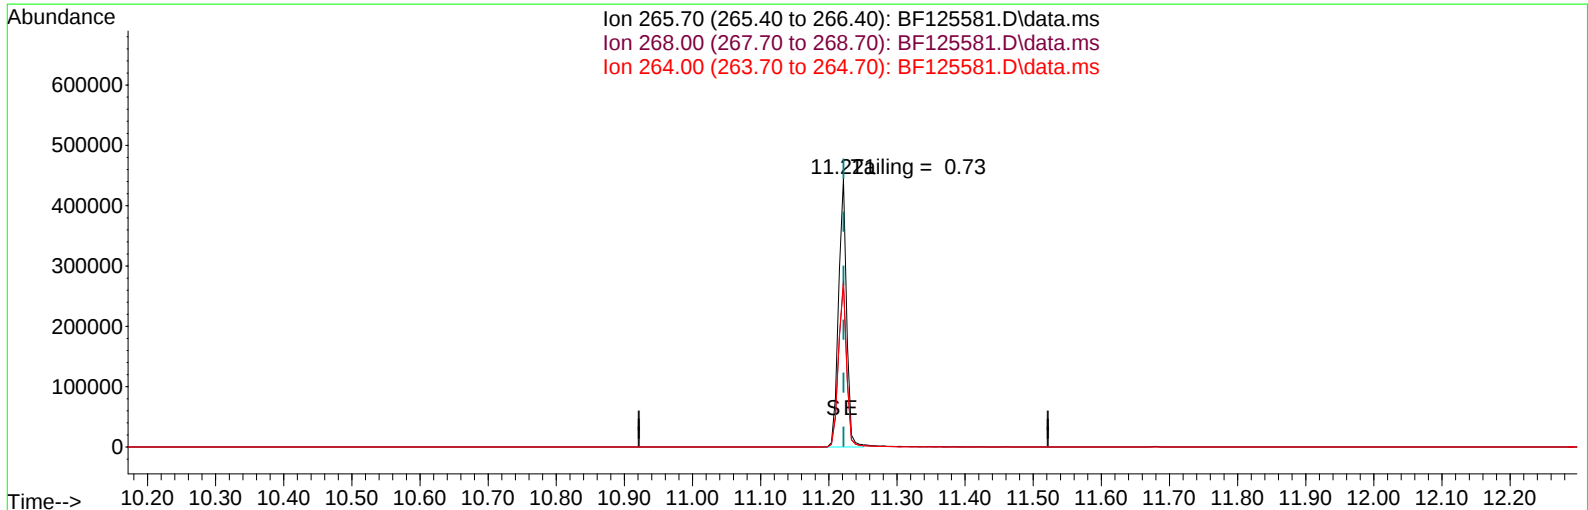

TIC: BF125581.D\data.ms

(70) Pentachlorophenol (C)

11.221min (+ 0.000) 32053.20 ng




response 369987

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	60.93
264.00	69.90	61.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
Data File : BF125581.D
Acq On : 23 Sep 2021 9:05
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 23 11:28:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 19:21:36 2021
Response via : Initial Calibration

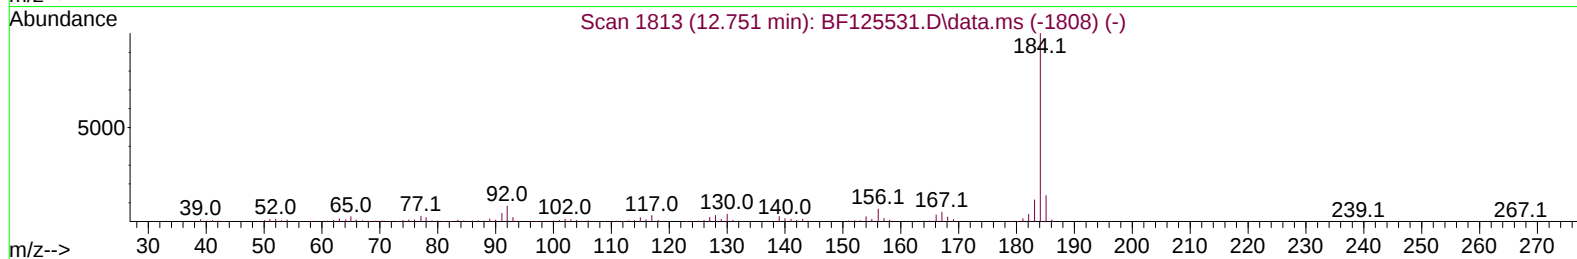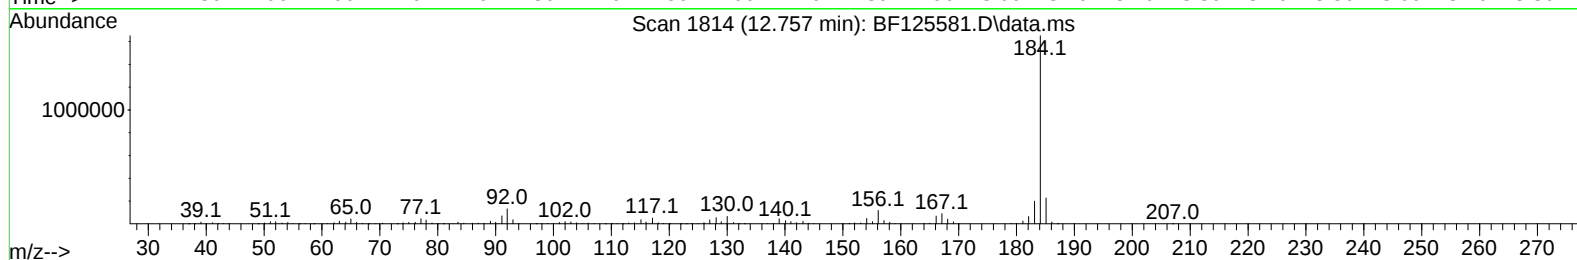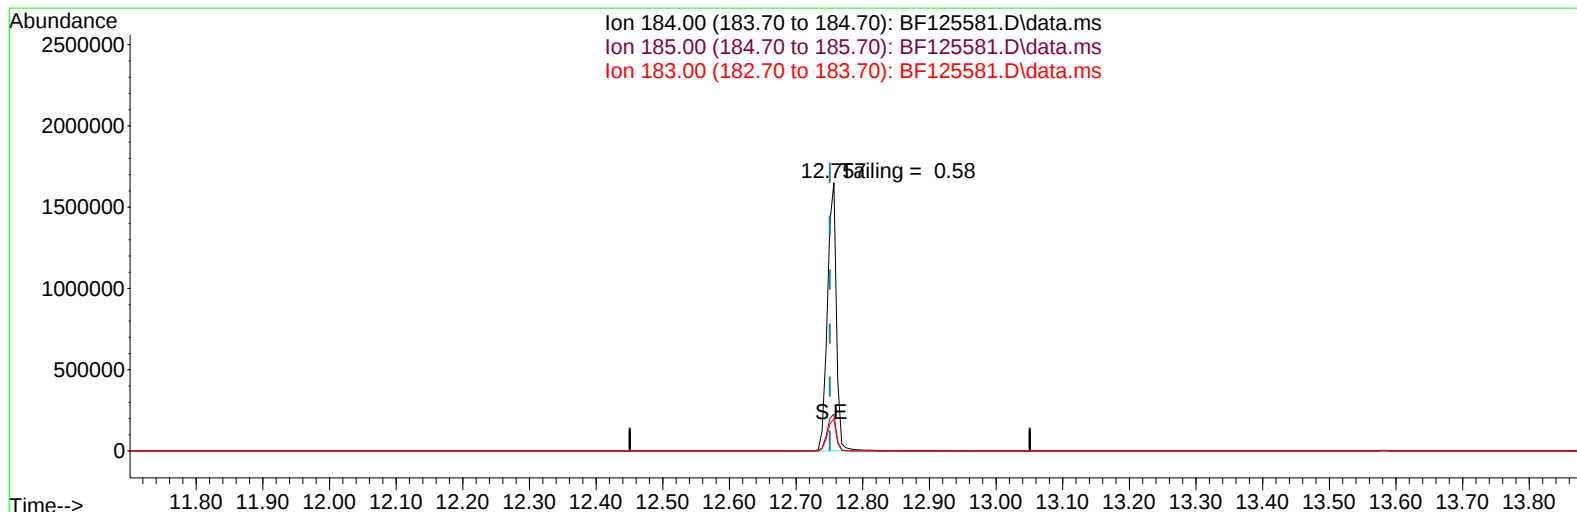

TIC: BF125581.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 1547240

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.71
183.00	10.10	12.05
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
9/23/2021	BNA_F	<u>BF125581.D</u>
Compound Name	Response	Retention Time
DDT	797655	13.58
DDD	9906	13.28
DDE	2716	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12622	810277	1.56