
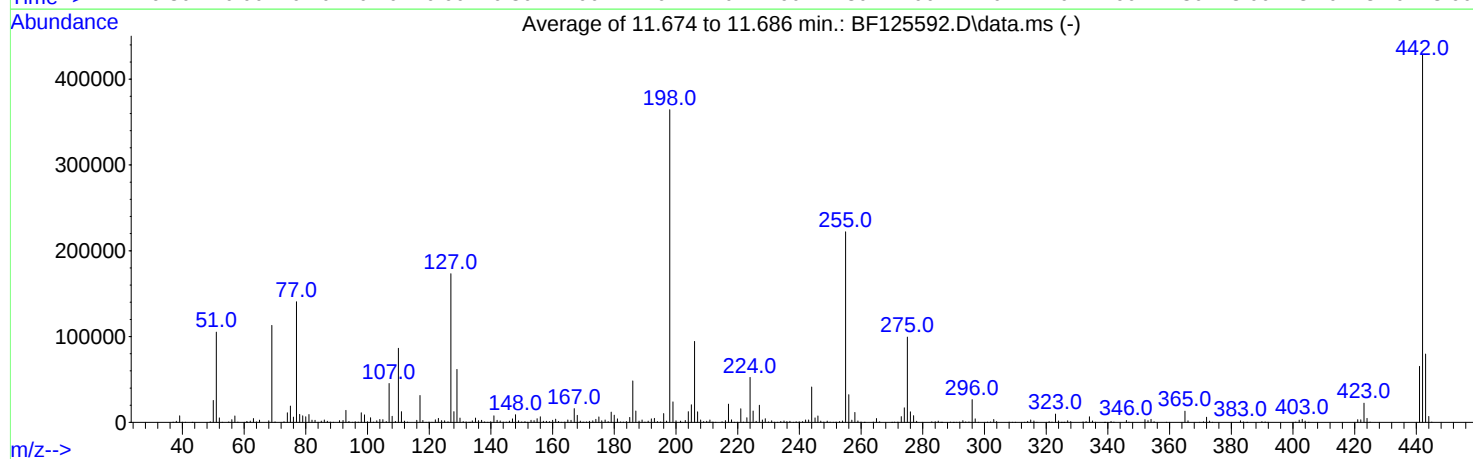


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
 Data File : BF125592.D
 Acq On : 23 Sep 2021 15:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 21 19:21:36 2021

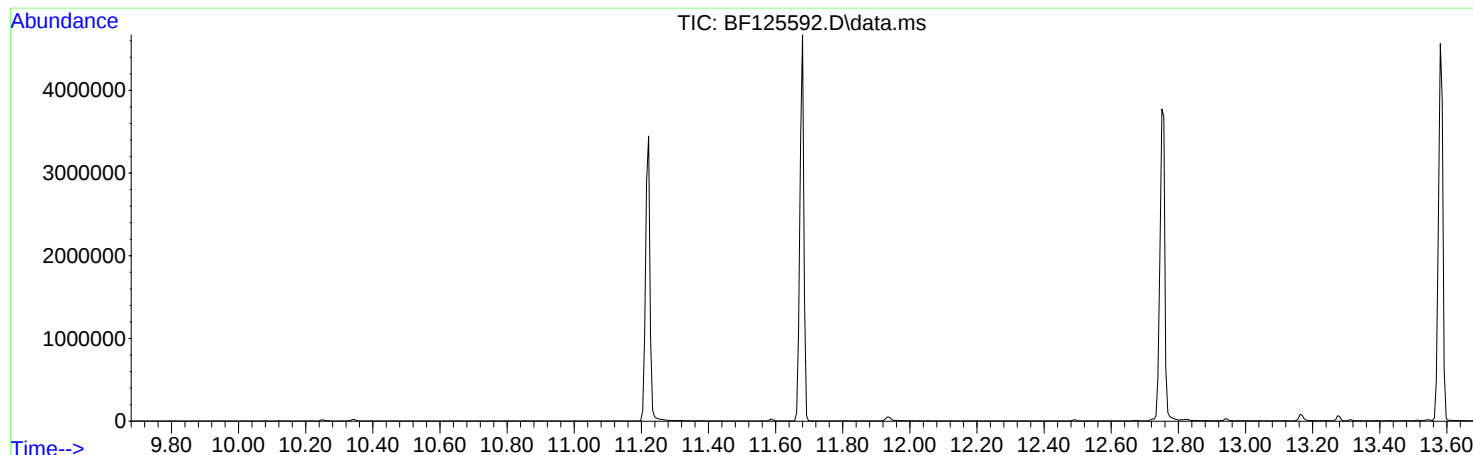




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	105181	PASS
68	69	0.00	2	1.6	1802	PASS
69	198	0.00	100	31.0	113107	PASS
70	69	0.00	2	0.4	491	PASS
127	198	10	80	47.6	173293	PASS
197	198	0.00	2	0.4	1524	PASS
198	198	100	100	100.0	364309	PASS
199	198	5	9	6.5	23856	PASS
275	198	10	60	27.3	99333	PASS
365	198	1	100	3.6	13047	PASS
441	198	0.01	100	17.9	65360	PASS
442	442	50	100	100.0	428736	PASS
443	442	15	24	18.6	79645	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
Data File : BF125592.D
Acq On : 23 Sep 2021 15:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 23 16:44:19 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 19:21:36 2021
Response via : Initial Calibration

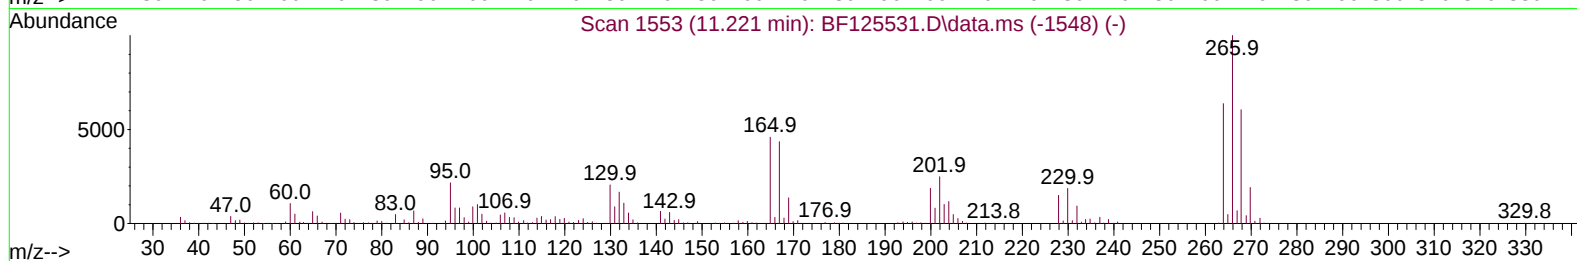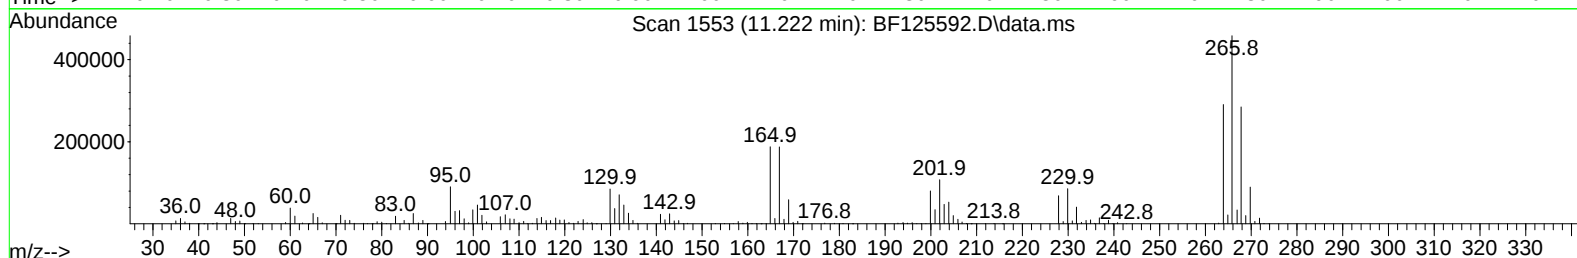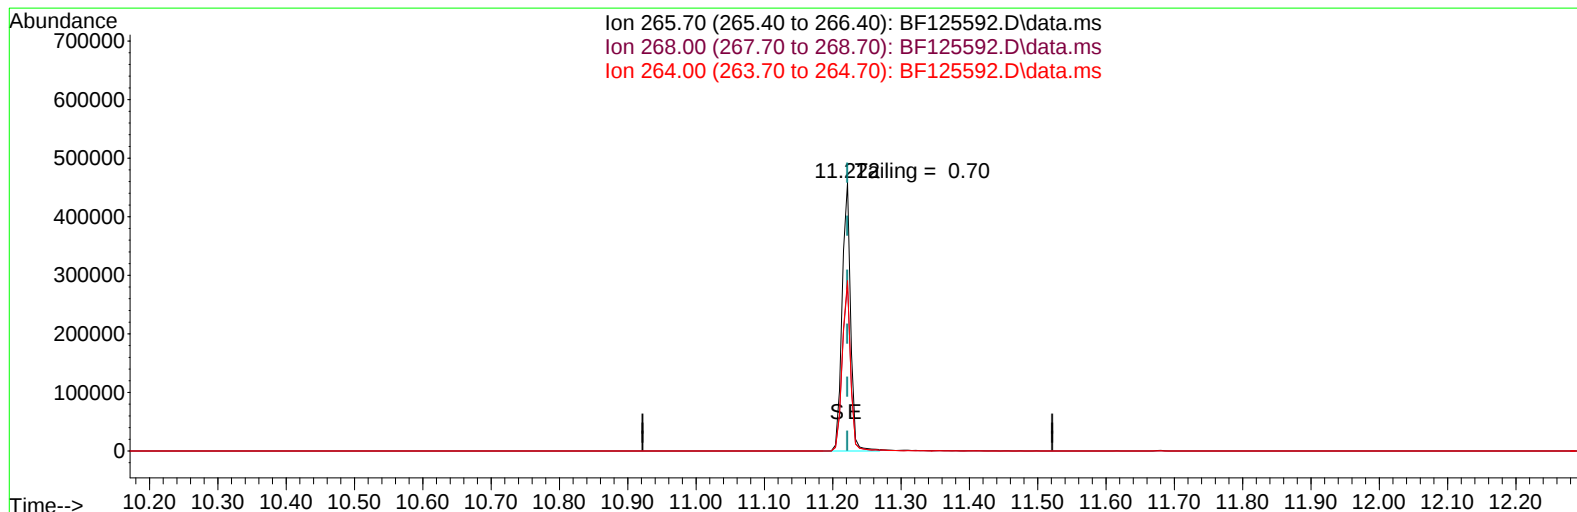

TIC: BF125592.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.000) 32497.77 ng




response 399697

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.15
264.00	69.90	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092321\
 Data File : BF125592.D
 Acq On : 23 Sep 2021 15:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 23 16:44:19 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 19:21:36 2021
 Response via : Initial Calibration

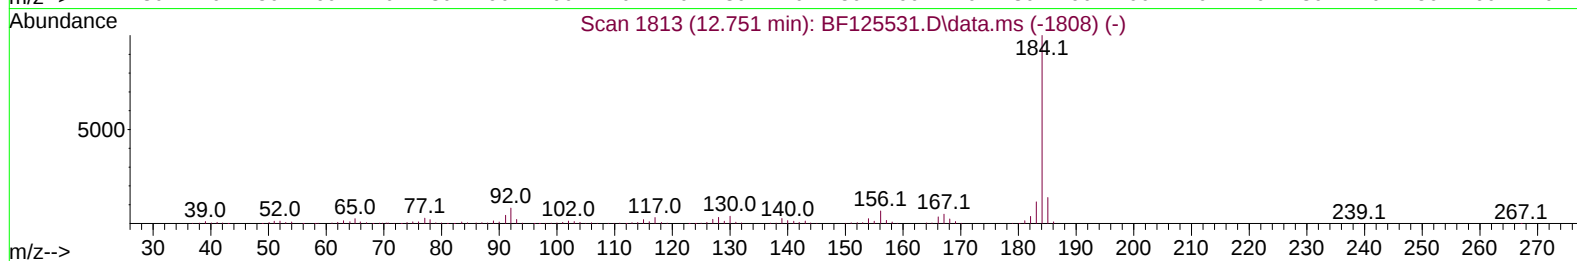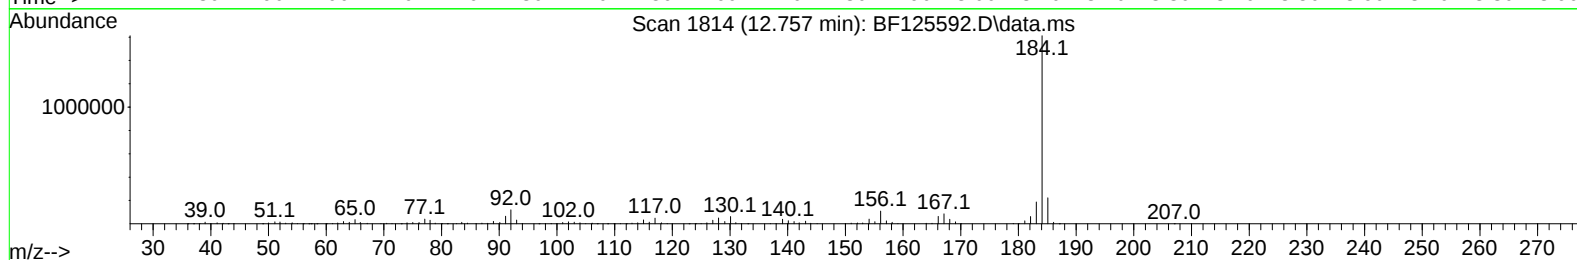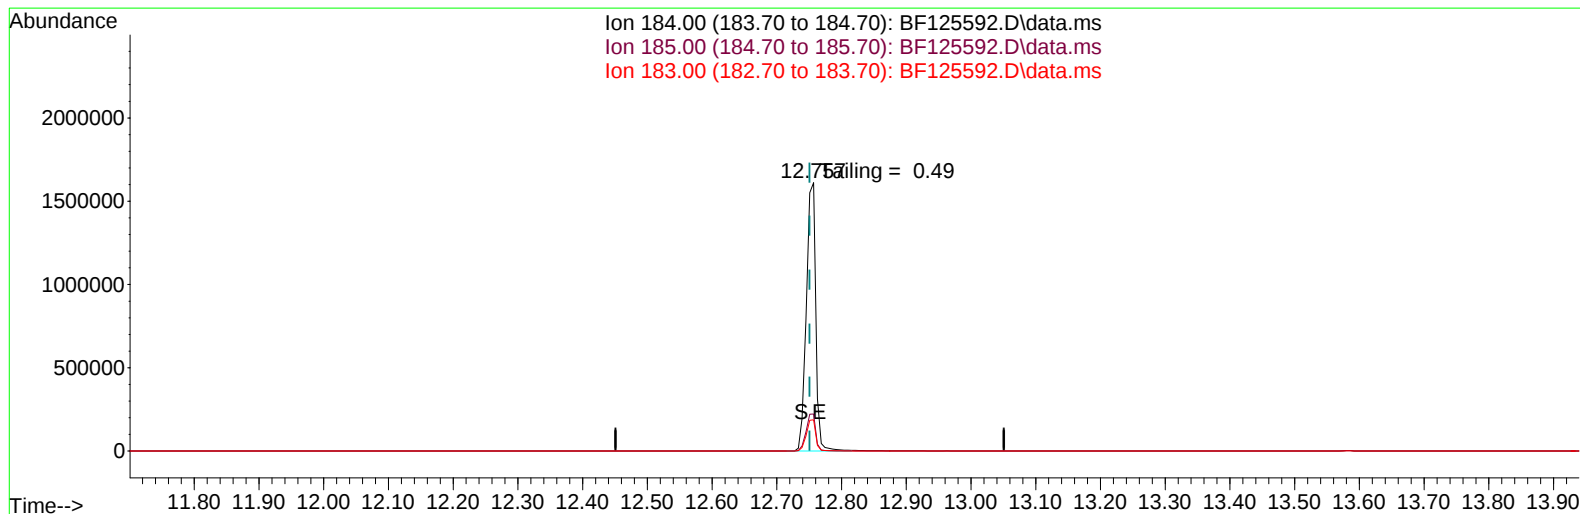

TIC: BF125592.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 1636968

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.79
183.00	10.10	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/23/2021	BNA_F	<u>BF125592.D</u>
Compound Name	Response	Retention Time
DDT	856140	13.58
DDD	12143	13.28
DDE	3326	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15469	871609	1.77