

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092322\
 Data File : BF130387.D
 Acq On : 23 Sep 2022 12:15
 Operator : CG\JU
 Sample : PB147862BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147862BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.857	465	471	479	rBV	33223	46275	1.23%	0.214%
2	5.263	535	540	543	rBV	2801028	2602930	69.23%	12.064%
3	6.293	710	715	718	rBV	2473810	2589255	68.87%	12.001%
4	6.651	772	776	779	rBV	761365	651259	17.32%	3.018%
5	7.216	866	872	875	rBV	1719435	1764609	46.94%	8.179%
6	7.934	989	994	997	rBV	920716	877382	23.34%	4.067%
7	9.016	1171	1178	1181	rBV	3358164	3497458	93.03%	16.210%
8	9.686	1286	1292	1295	rBV	1149150	1010106	26.87%	4.682%
9	10.475	1420	1426	1429	rBV	2668259	2198930	58.49%	10.192%
10	11.169	1540	1544	1547	rBV	1194992	1005369	26.74%	4.660%
11	12.757	1809	1814	1817	rBV	4162439	3759560	100.00%	17.425%
12	13.798	1987	1991	1995	rBV	975288	827559	22.01%	3.836%
13	13.898	2001	2008	2014	rBV	85013	109729	2.92%	0.509%
14	15.192	2223	2228	2233	rBV	571957	635375	16.90%	2.945%




Sum of corrected areas: 21575796

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092322\
Data File : BF130387.D
Acq On : 23 Sep 2022 12:15
Operator : CG\JU
Sample : PB147862BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147862BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

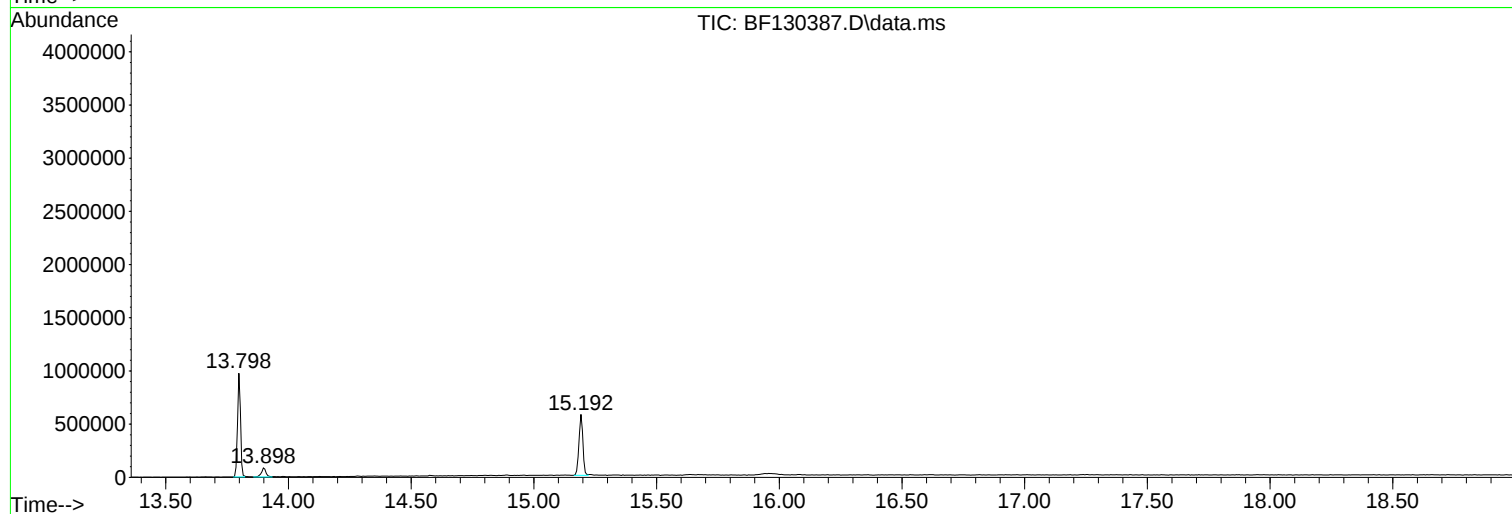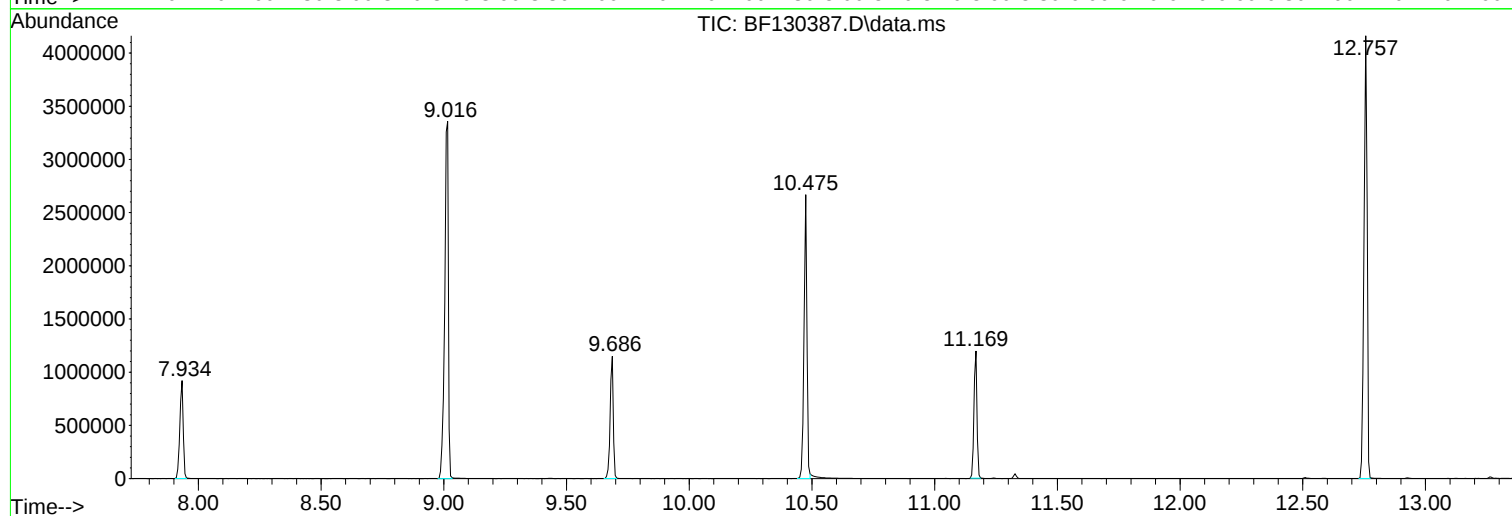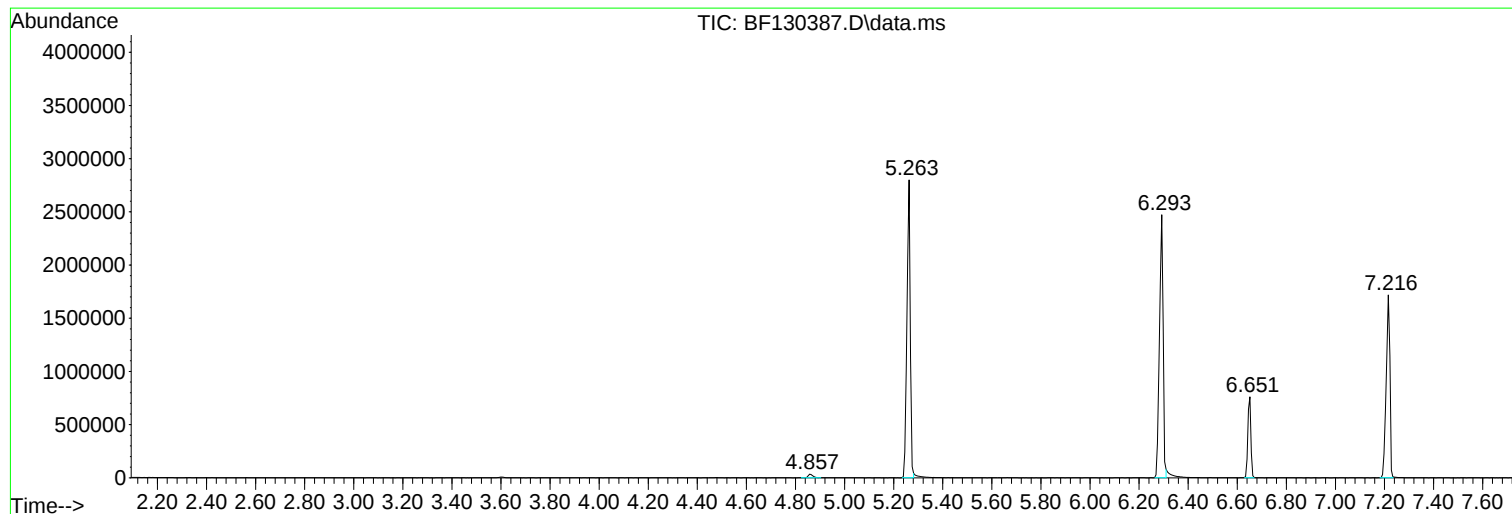

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092322\
Data File : BF130387.D
Acq On : 23 Sep 2022 12:15
Operator : CG\JU
Sample : PB147862BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147862BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.898	2.65 ng	109729	Chrysene-d12	13.798

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	95
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	53
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	45
4			1H-Indole-3-acetic acid, 5-[(tri...]	277	C14H19N03Si	072101-35-0	17
5			1H-Indol-4-ol, 2TMS derivative	277	C14H23N0Si2	1000485-28-1	17

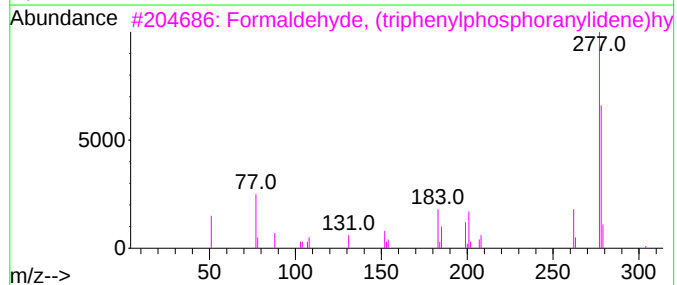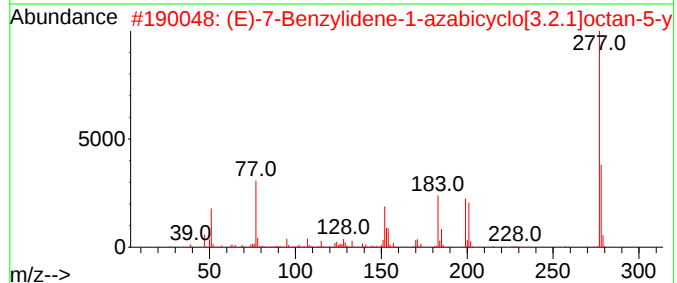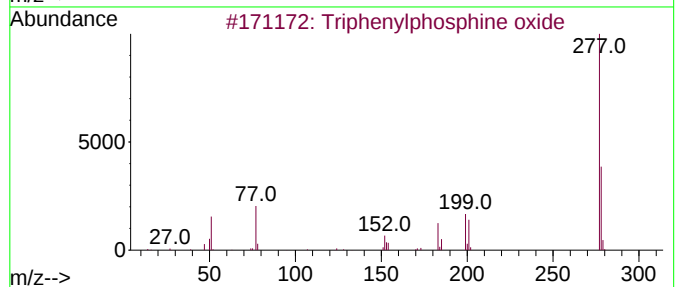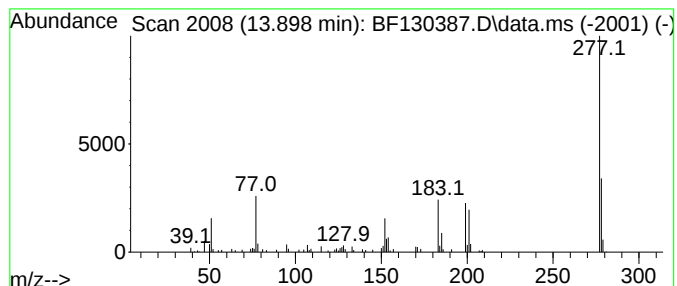

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092322\
Data File : BF130387.D
Acq On : 23 Sep 2022 12:15
Operator : CG\JU
Sample : PB147862BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147862BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	13.898	2.6	ng	109729	5	13.798	827559	20.0