


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092322\
 Data File : BF130385.D
 Acq On : 23 Sep 2022 11:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 19 15:06:14 2022

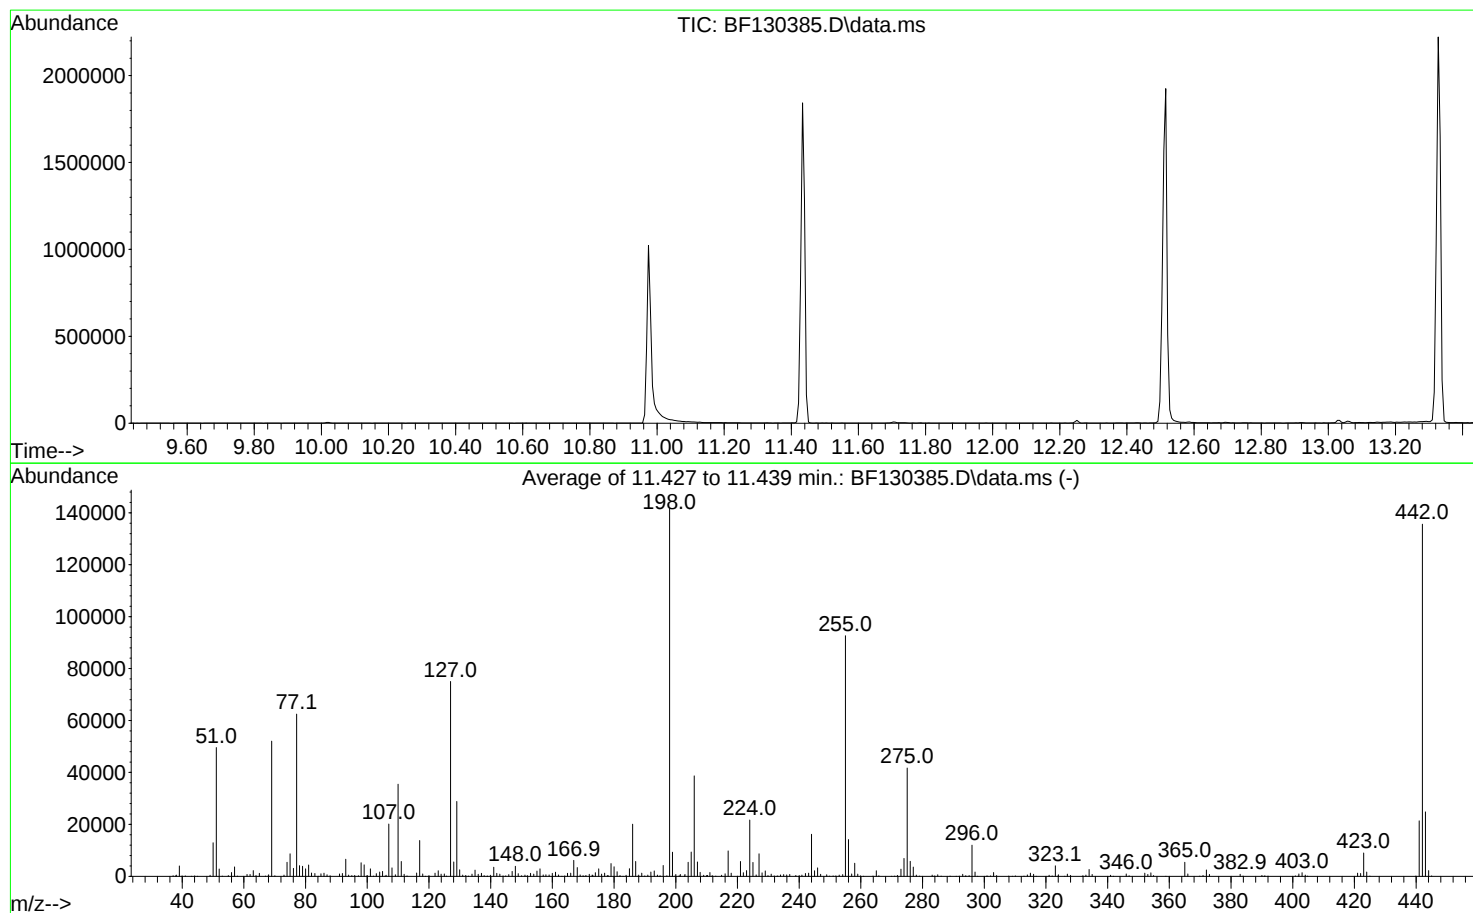




AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	49563	PASS
68	69	0.00	2	1.1	593	PASS
69	198	0.00	100	36.7	52037	PASS
70	69	0.00	2	0.5	243	PASS
127	198	10	80	53.0	75040	PASS
197	198	0.00	2	0.2	238	PASS
198	198	100	100	100.0	141688	PASS
199	198	5	9	6.6	9307	PASS
275	198	10	60	29.4	41680	PASS
365	198	1	100	3.8	5415	PASS
441	198	0.01	100	15.1	21391	PASS
442	442	50	100	100.0	135627	PASS
443	442	15	24	18.3	24834	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092322\
 Data File : BF130385.D
 Acq On : 23 Sep 2022 11:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 23 16:11:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 19 15:06:14 2022
 Response via : Initial Calibration

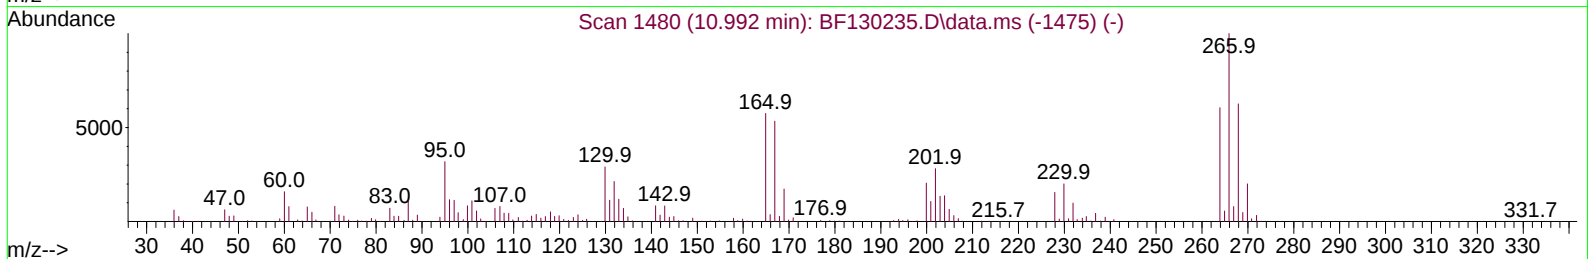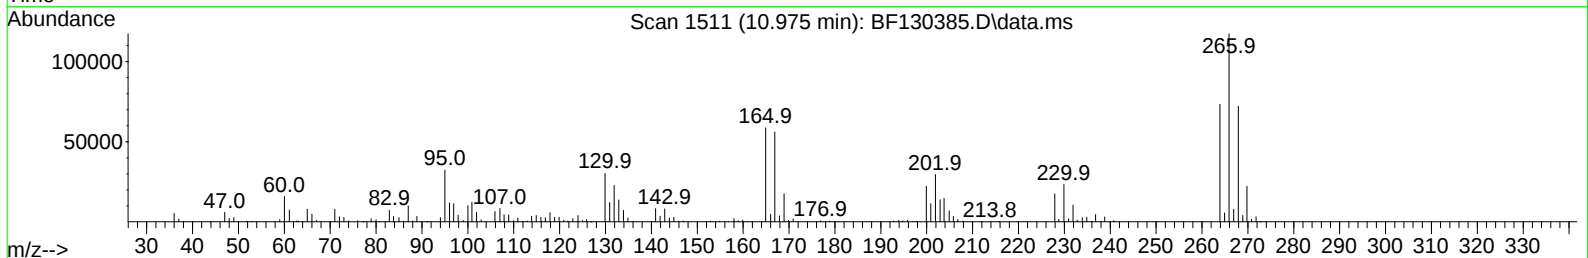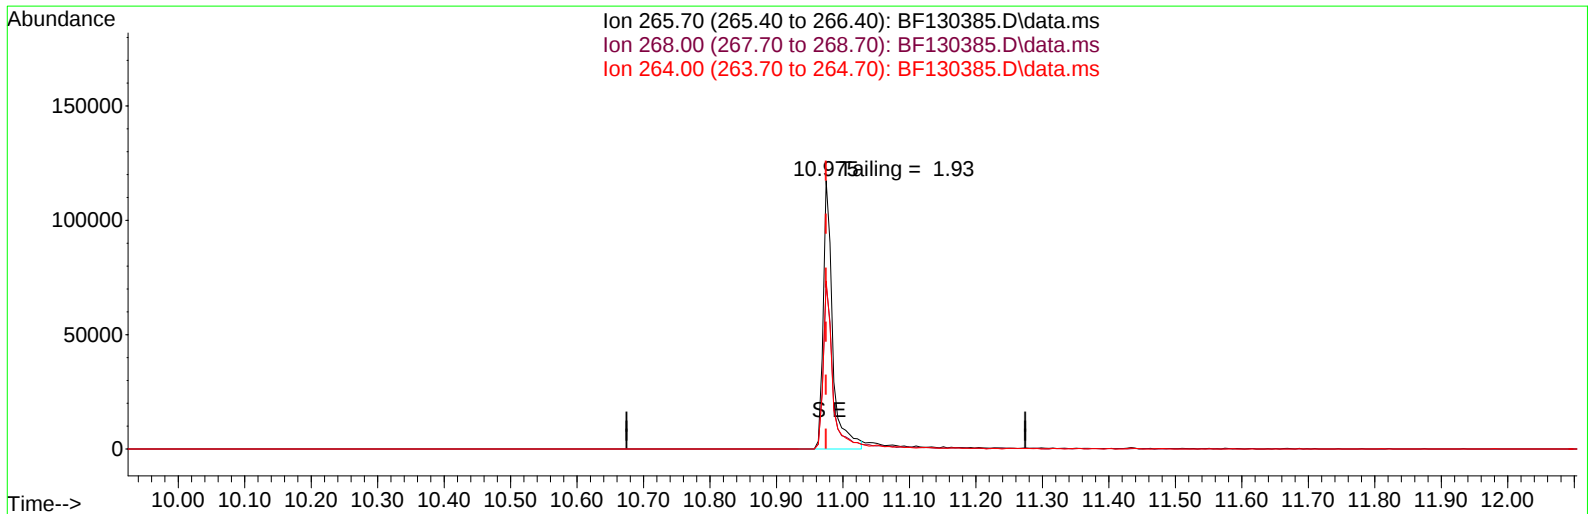

TIC: BF130385.D\data.ms

(70) Pentachlorophenol (C)

10.975min (+ 0.000) 30236.91 ng




response 124599

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.53
264.00	63.10	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092322\
Data File : BF130385.D
Acq On : 23 Sep 2022 11:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 23 16:11:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 15:06:14 2022
Response via : Initial Calibration

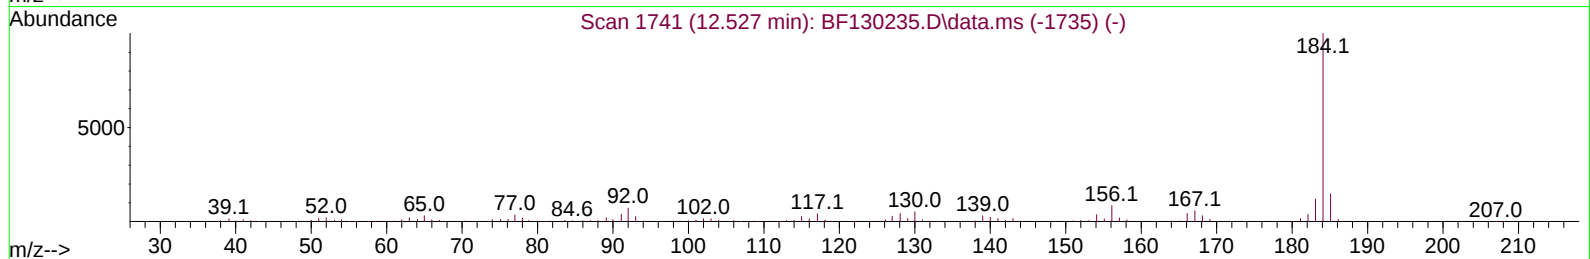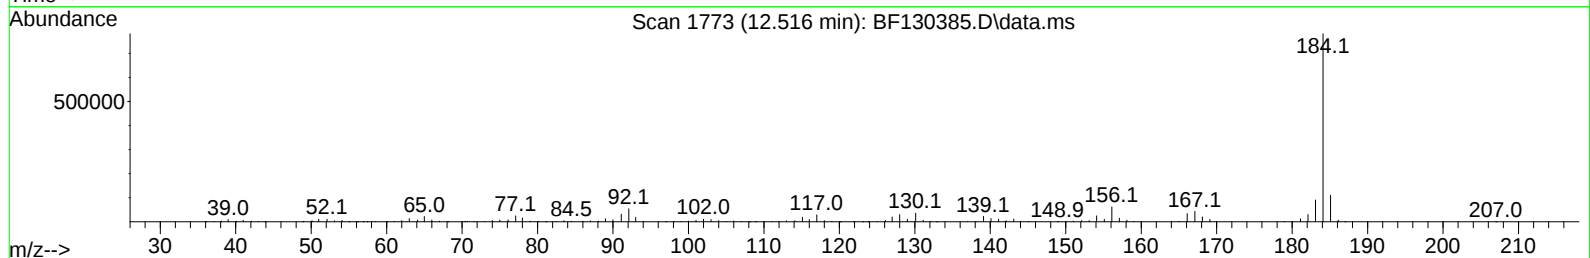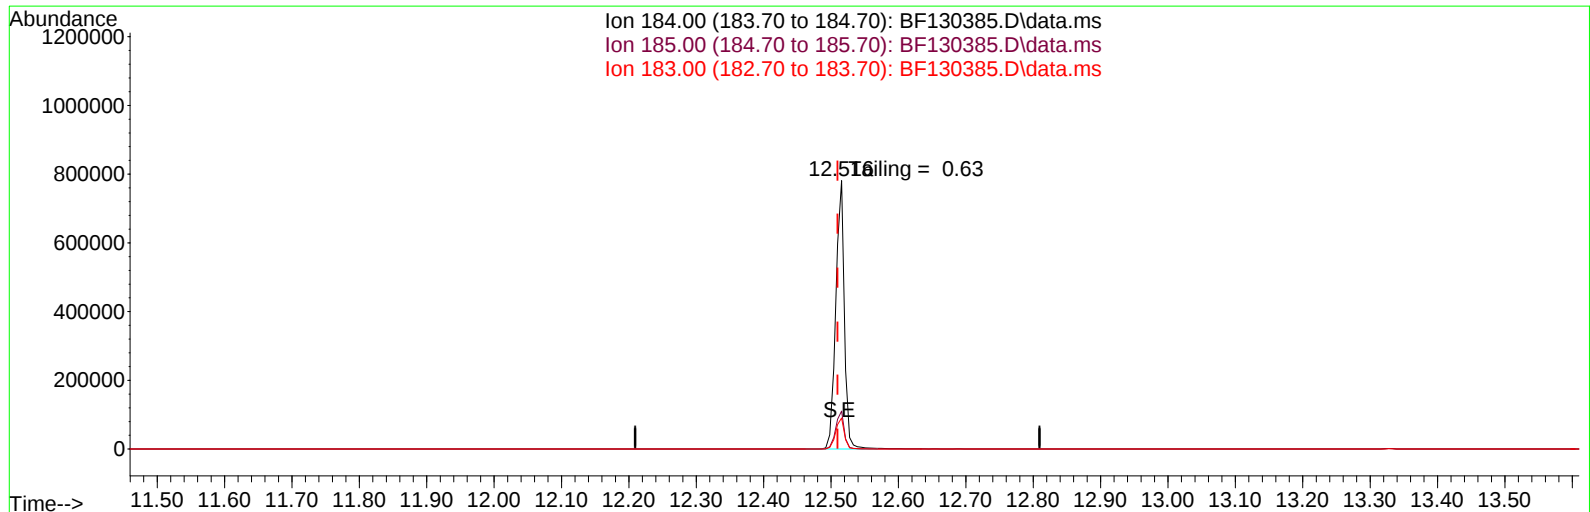

TIC: BF130385.D\data.ms

(77) Benzidine

12.516min (+ 0.006) 0.00 ng

response 690855

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.14
183.00	11.40	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/23/2022	BNA_F	<u>BF130385.D</u>
Compound Name	Response	Retention Time
DDT	354953	13.32
DDD	3029	13.03
DDE	741	12.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3770	358723	1.05

Instrument :
BNA_F
ClientSampleId :
DFTPP