
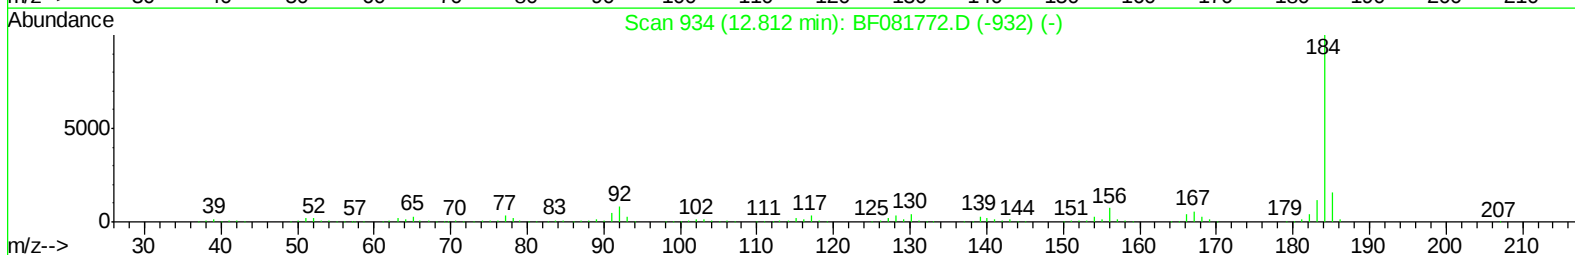
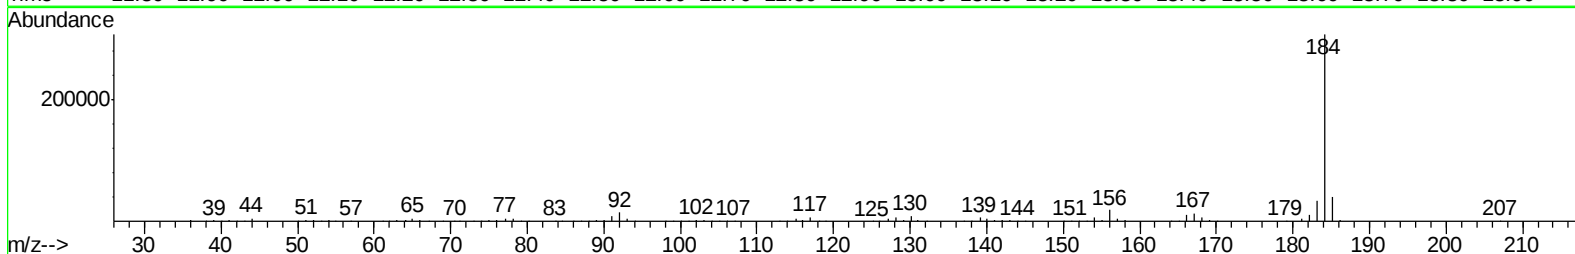


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092415\
 Data File : BF081768.D
 Acq On : 24 Sep 2015 17:22
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 08:34:10 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 25 07:13:40 2015
 Response via : Initial Calibration

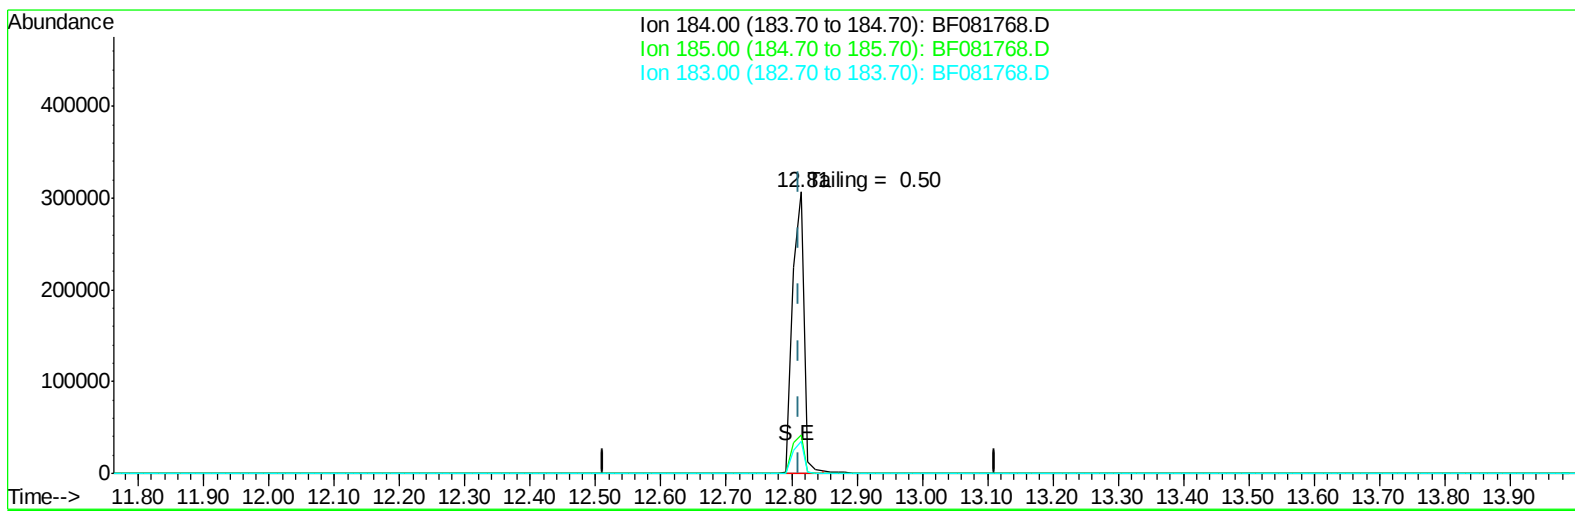

TIC: BF081768.D

(76) Benzidine




12.814min (+0.002) 0.00ng

response 384647

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.44
183.00	9.50	11.33
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092415\
Data File : BF081768.D
Acq On : 24 Sep 2015 17:22
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 08:34:10 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 07:13:40 2015
Response via : Initial Calibration

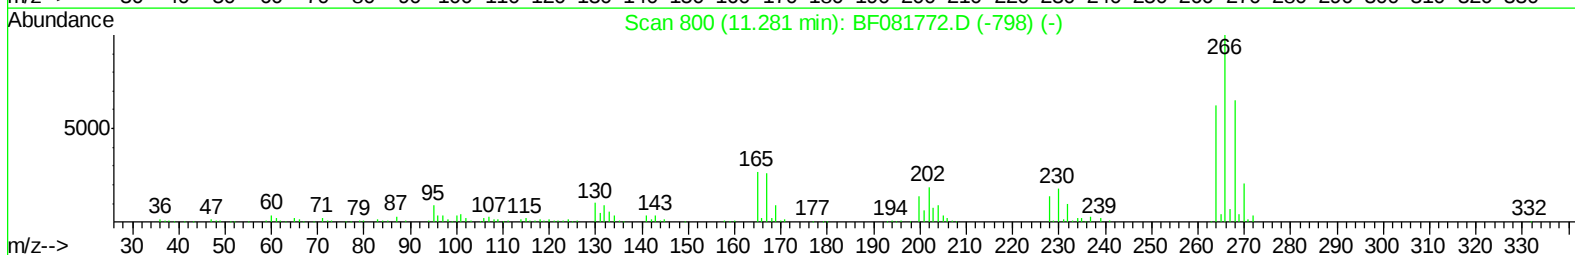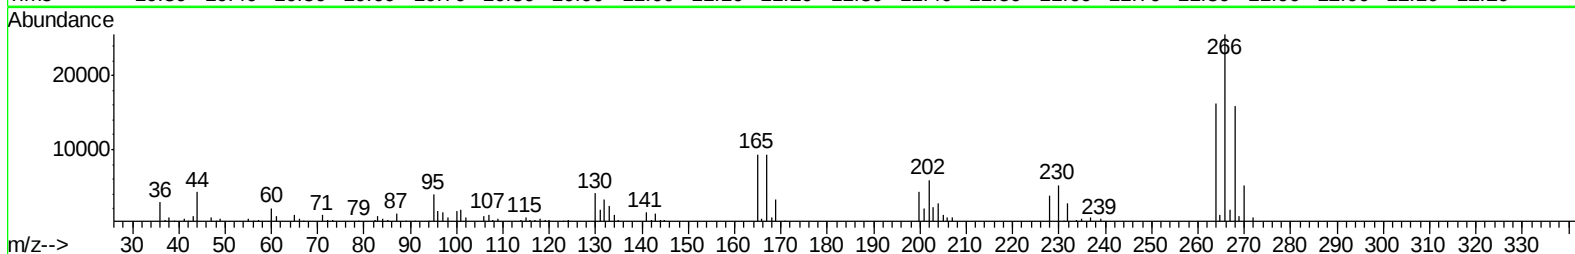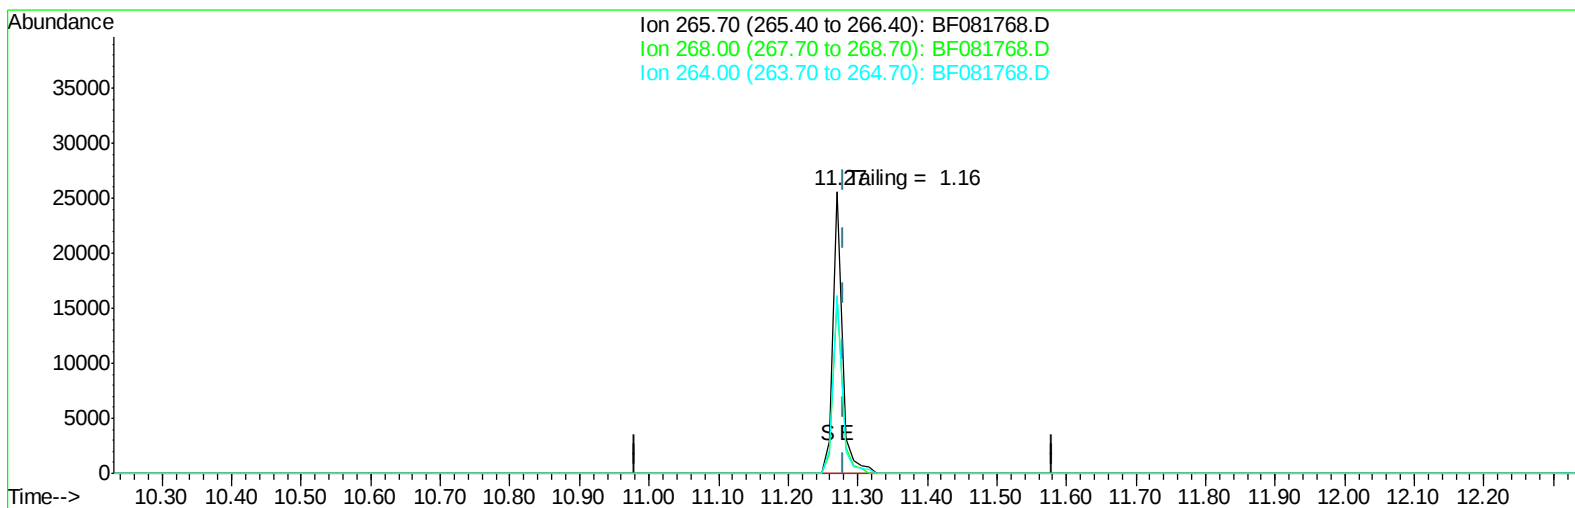

TIC: BF081768.D

(69) Pentachlorophenol (C)

11.271min (-0.010) 0.00ng

response 23379

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.39
264.00	62.70	63.29
0.00	0.00	0.00