
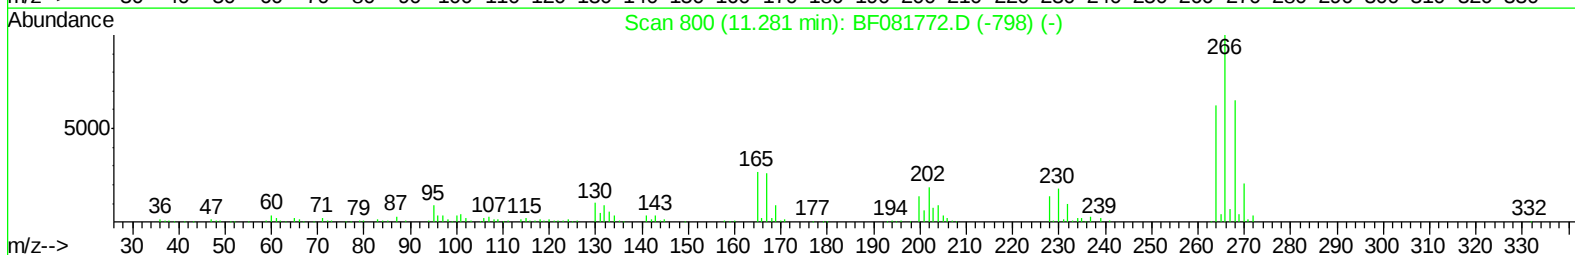
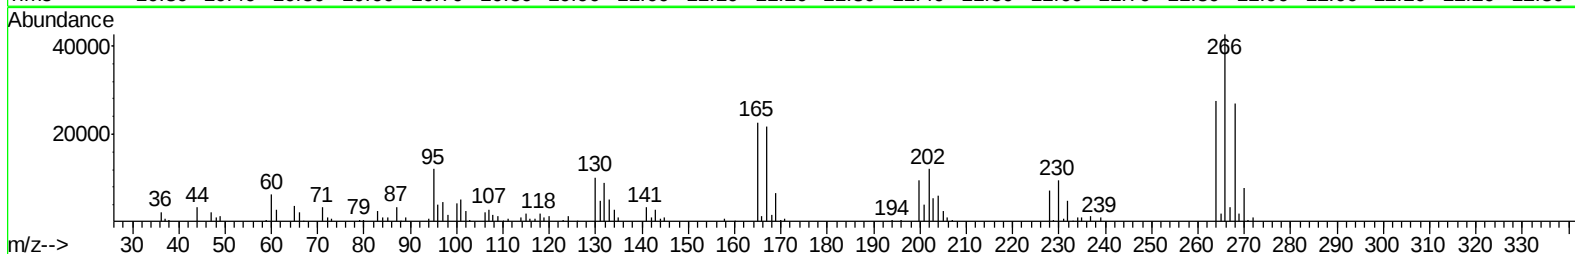


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092415\
Data File : BF081785.D
Acq On : 25 Sep 2015 3:36
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 08:36:21 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 07:13:40 2015
Response via : Initial Calibration

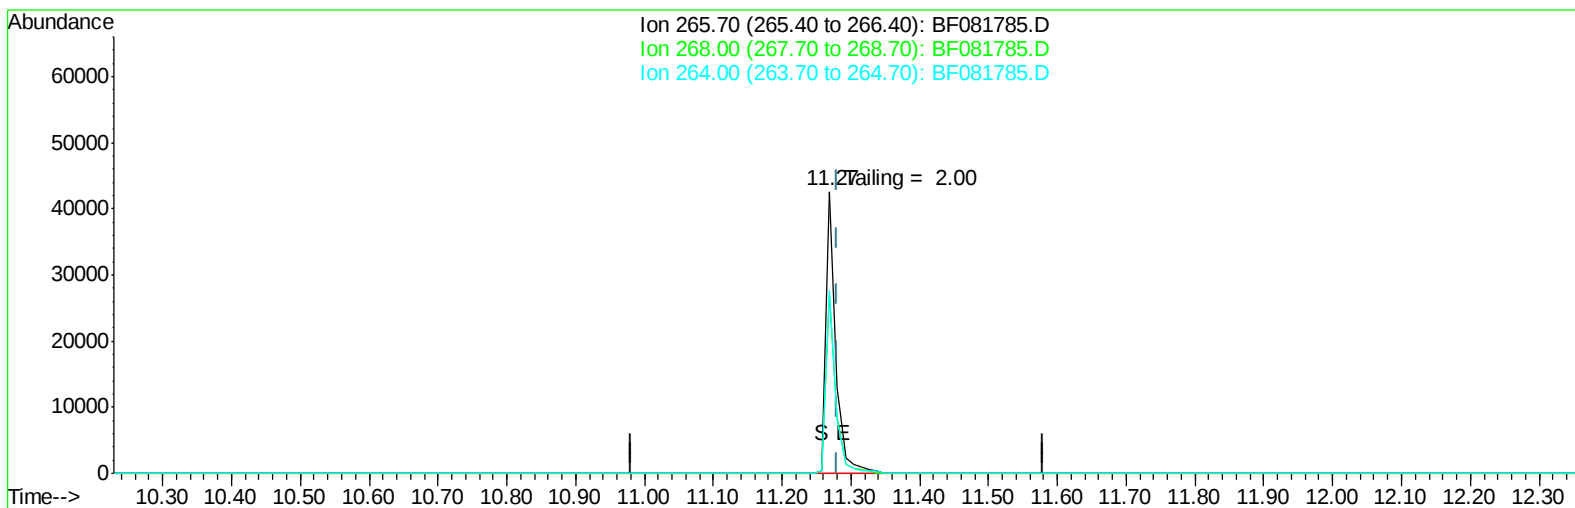

TIC: BF081785.D

(69) Pentachlorophenol (C)




11.269min (-0.012) 0.00ng

response 42292

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.24
264.00	62.70	64.87
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092415\
Data File : BF081785.D
Acq On : 25 Sep 2015 3:36
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 08:36:21 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 07:13:40 2015
Response via : Initial Calibration

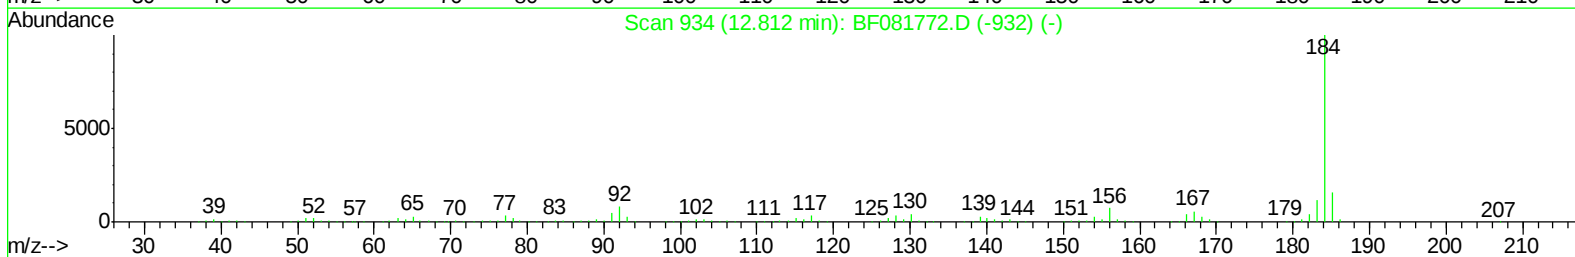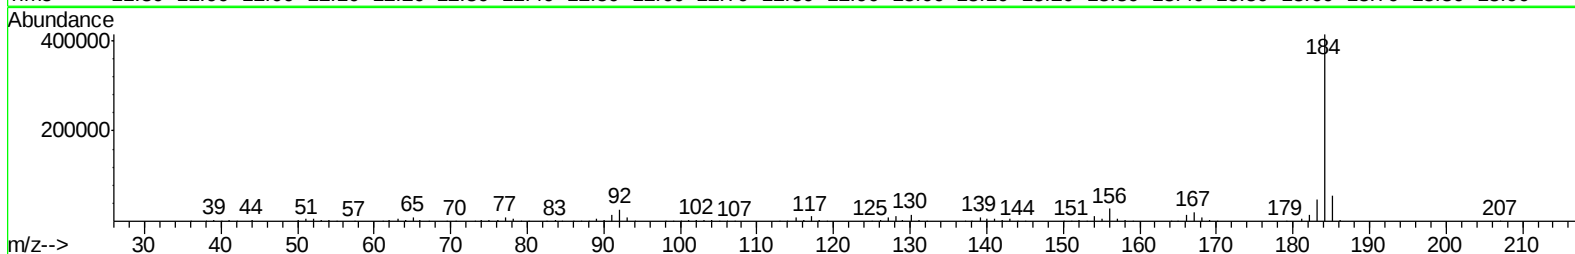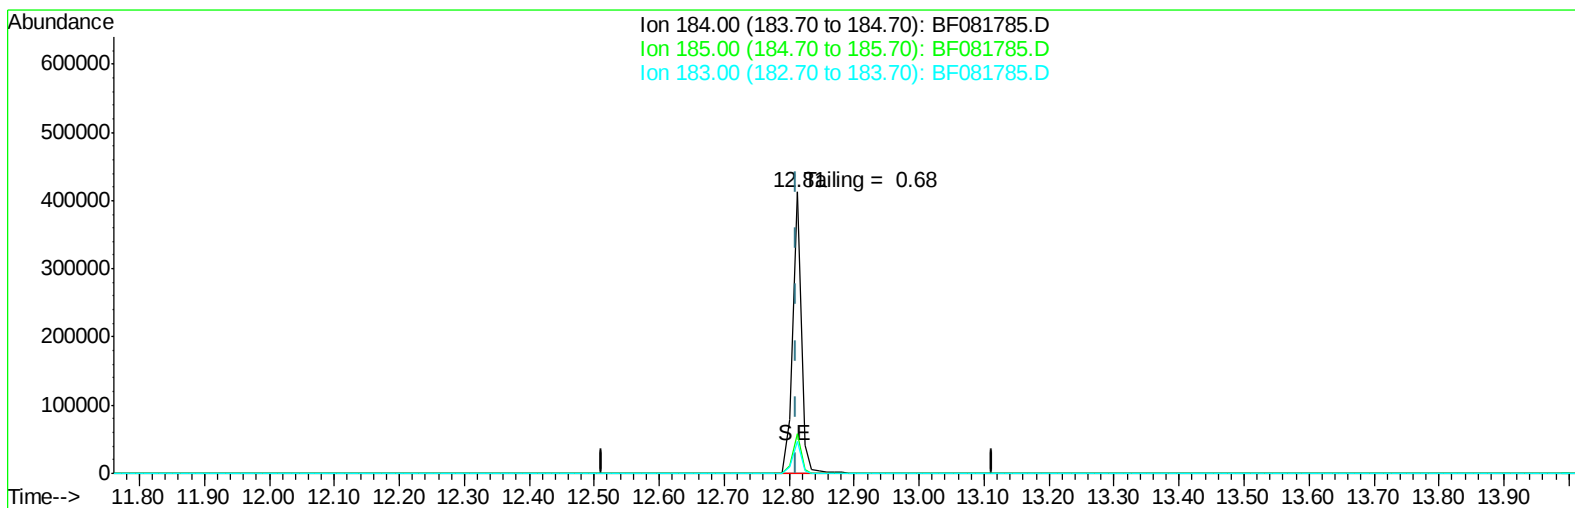

TIC: BF081785.D

(76) Benzidine

12.812min (-0.000) 0.00ng

response 378830

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.99
183.00	9.50	11.51#
0.00	0.00	0.00