

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092415\
 Data File : BF081780.D
 Acq On : 24 Sep 2015 23:31
 Operator : UM/IZ
 Sample : G3748-04DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MGP205-10-12DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.531	294	297	300	rVB2	838912	800667	7.11%	0.517%
2	6.560	384	387	389	rVB	572188	797984	7.09%	0.516%
3	6.709	397	400	402	rVB	857960	723693	6.43%	0.468%
4	6.777	404	406	409	rBV	285451	429410	3.81%	0.278%
5	6.949	419	421	423	rBV	1488822	1279025	11.36%	0.827%
6	7.109	432	435	436	rBV	500903	765326	6.80%	0.495%
7	7.132	436	437	439	rVB	1680245	1196656	10.63%	0.773%
8	7.212	439	444	447	rBV3	314189	389821	3.46%	0.252%
9	7.509	469	470	472	rVB2	557372	575789	5.11%	0.372%
10	7.909	501	505	507	rVB	463018	466838	4.15%	0.302%
11	7.977	507	511	513	rBV2	501341	801779	7.12%	0.518%
12	8.023	513	515	518	rVV	577600	1011318	8.98%	0.654%
13	8.275	530	537	539	rBV2	6855436	11262188	100.00%	7.279%
14	8.309	539	540	543	rVB	613219	768639	6.82%	0.497%
15	8.697	569	574	575	rBV2	278422	455673	4.05%	0.294%
16	8.903	591	592	594	rVB	445302	358745	3.19%	0.232%
17	8.960	594	597	599	rVB	5848005	6517060	57.87%	4.212%
18	9.052	602	605	608	rVB	3883725	5808632	51.58%	3.754%
19	9.315	625	628	630	rVB	843464	942671	8.37%	0.609%
20	9.418	634	637	638	rVB	1267971	1404432	12.47%	0.908%
21	9.509	640	645	648	rVB2	1368457	1897715	16.85%	1.226%
22	9.578	648	651	653	rBV	1979043	2780704	24.69%	1.797%
23	9.658	655	658	659	rBV	2440013	3529529	31.34%	2.281%
24	9.772	665	668	672	rVB	1283154	1990147	17.67%	1.286%
25	9.852	672	675	677	rBV	2180256	1935203	17.18%	1.251%
26	9.989	684	687	689	rBV2	1560717	2669101	23.70%	1.725%
27	10.023	689	690	692	rVB	2473090	2697430	23.95%	1.743%
28	10.092	694	696	698	rBV	469679	642700	5.71%	0.415%
29	10.195	701	705	707	rVB2	1010989	1294010	11.49%	0.836%
30	10.229	707	708	710	rVB	760381	603367	5.36%	0.390%
31	10.309	712	715	716	rBV	682426	858484	7.62%	0.555%
32	10.400	720	723	726	rBV2	466143	1147482	10.19%	0.742%
33	10.492	728	731	734	rVV4	369266	1062277	9.43%	0.687%
34	10.549	734	736	738	rVB	2586075	3601518	31.98%	2.328%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092415\
 Data File : BF081780.D
 Acq On : 24 Sep 2015 23:31
 Operator : UM/IZ
 Sample : G3748-04DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MGP205-10-12DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.606	738	741	743	rBV2	337754	925351	8.22%	0.598%
36	10.652	743	745	746	rVV2	441912	455396	4.04%	0.294%
37	10.698	746	749	750	rVV3	354889	494767	4.39%	0.320%
38	10.778	753	756	758	rVB2	805838	1475962	13.11%	0.954%
39	10.903	764	767	769	rBV2	439759	521612	4.63%	0.337%
40	11.086	780	783	784	rBV	1180159	1472356	13.07%	0.952%
41	11.109	784	785	789	rVV	616572	714388	6.34%	0.462%
42	11.166	789	790	792	rVB	631337	516135	4.58%	0.334%
43	11.372	806	808	811	rVB	1888094	2436950	21.64%	1.575%
44	11.521	815	821	823	rBV2	6456284	10837154	96.23%	7.004%
45	11.555	823	824	826	rVV	1881290	2686940	23.86%	1.737%
46	11.635	830	831	834	rVB	357325	379914	3.37%	0.246%
47	11.715	836	838	841	rBV3	248740	467602	4.15%	0.302%
48	11.772	841	843	845	rVV	394011	521955	4.63%	0.337%
49	11.806	845	846	849	rVV2	1027942	1138087	10.11%	0.736%
50	11.898	852	854	856	rVB	891595	1135496	10.08%	0.734%
51	11.978	859	861	863	rVV	1590903	2632949	23.38%	1.702%
52	12.012	863	864	866	rVB	2649438	1920201	17.05%	1.241%
53	12.058	866	868	869	rBV	1130847	1029779	9.14%	0.666%
54	12.092	869	871	875	rVB	2541450	4821085	42.81%	3.116%
55	12.275	885	887	888	rVV	1396554	1355544	12.04%	0.876%
56	12.309	888	890	893	rVV	380411	618789	5.49%	0.400%
57	12.378	893	896	897	rVV2	303576	463612	4.12%	0.300%
58	12.424	897	900	901	rVV2	388810	797612	7.08%	0.515%
59	12.458	901	903	906	rVV2	633688	1101906	9.78%	0.712%
60	12.538	907	910	911	rVV	1200549	1644249	14.60%	1.063%
61	12.572	911	913	916	rVV	1012661	1833582	16.28%	1.185%
62	12.641	916	919	920	rVV2	641776	1181916	10.49%	0.764%
63	12.675	920	922	923	rVV2	379487	595071	5.28%	0.385%
64	12.709	923	925	927	rVV	3063561	4218945	37.46%	2.727%
65	12.744	927	928	929	rVV	656228	662095	5.88%	0.428%
66	12.801	932	933	936	rVV	1092994	1399034	12.42%	0.904%
67	12.846	936	937	941	rVV2	742640	1445260	12.83%	0.934%
68	12.938	941	945	947	rVV	4295107	6113743	54.29%	3.951%
69	12.972	947	948	950	rVV2	460282	705492	6.26%	0.456%
70	13.064	954	956	960	rVV	973362	1647579	14.63%	1.065%
71	13.144	960	963	966	rVV2	673615	1401420	12.44%	0.906%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092415\
 Data File : BF081780.D
 Acq On : 24 Sep 2015 23:31
 Operator : UM/IZ
 Sample : G3748-04DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MGP205-10-12DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.189	966	967	969	rVV	366951	587868	5.22%	0.380%
73	13.246	969	972	974	rVV	1176224	1992927	17.70%	1.288%
74	13.292	974	976	977	rVV2	320944	512680	4.55%	0.331%
75	13.315	977	978	980	rVV	1118748	1070138	9.50%	0.692%
76	13.349	980	981	985	rVV	829782	1245669	11.06%	0.805%
77	13.441	988	989	991	rVV	581880	802450	7.13%	0.519%
78	13.475	991	992	997	rVB	846417	902636	8.01%	0.583%
79	13.647	1005	1007	1012	rVB3	195008	447231	3.97%	0.289%
80	13.864	1024	1026	1028	rBV	629483	773643	6.87%	0.500%
81	14.035	1039	1041	1045	rVB	275928	359908	3.20%	0.233%
82	14.115	1045	1048	1049	rVV2	2119943	3220618	28.60%	2.081%
83	14.149	1049	1051	1054	rVV	1451778	1886951	16.75%	1.220%
84	14.275	1058	1062	1064	rVV3	234762	613298	5.45%	0.396%
85	14.367	1066	1070	1074	rVB3	253168	527129	4.68%	0.341%
86	14.504	1079	1082	1083	rVV	625689	842185	7.48%	0.544%
87	14.538	1083	1085	1086	rVV	356395	414989	3.68%	0.268%
88	14.595	1086	1090	1091	rVV4	372229	634603	5.63%	0.410%
89	14.629	1091	1093	1096	rVV3	358122	727844	6.46%	0.470%
90	15.155	1136	1139	1146	rBV2	819600	2044015	18.15%	1.321%
91	15.258	1146	1148	1151	rVB	285252	366636	3.26%	0.237%
92	15.464	1163	1166	1169	rBV	632490	916996	8.14%	0.593%
93	15.521	1169	1171	1174	rVV	1111872	1528871	13.58%	0.988%
94	15.590	1174	1177	1178	rVV	954859	1243765	11.04%	0.804%
95	15.612	1178	1179	1182	rVB2	267844	385813	3.43%	0.249%
96	17.053	1301	1305	1309	rVB2	483095	1019565	9.05%	0.659%
97	17.281	1323	1325	1337	rVB	156007	510105	4.53%	0.330%
98	17.498	1339	1344	1348	rBV	460003	991521	8.80%	0.641%
99	17.727	1360	1364	1371	rVB	211959	516605	4.59%	0.334%
100	19.739	1534	1540	1550	rVB	88824	407634	3.62%	0.263%


Sum of corrected areas: 154730234

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092415\
Data File : BF081780.D
Acq On : 24 Sep 2015 23:31
Operator : UM/IZ
Sample : G3748-04DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MGP205-10-12DL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

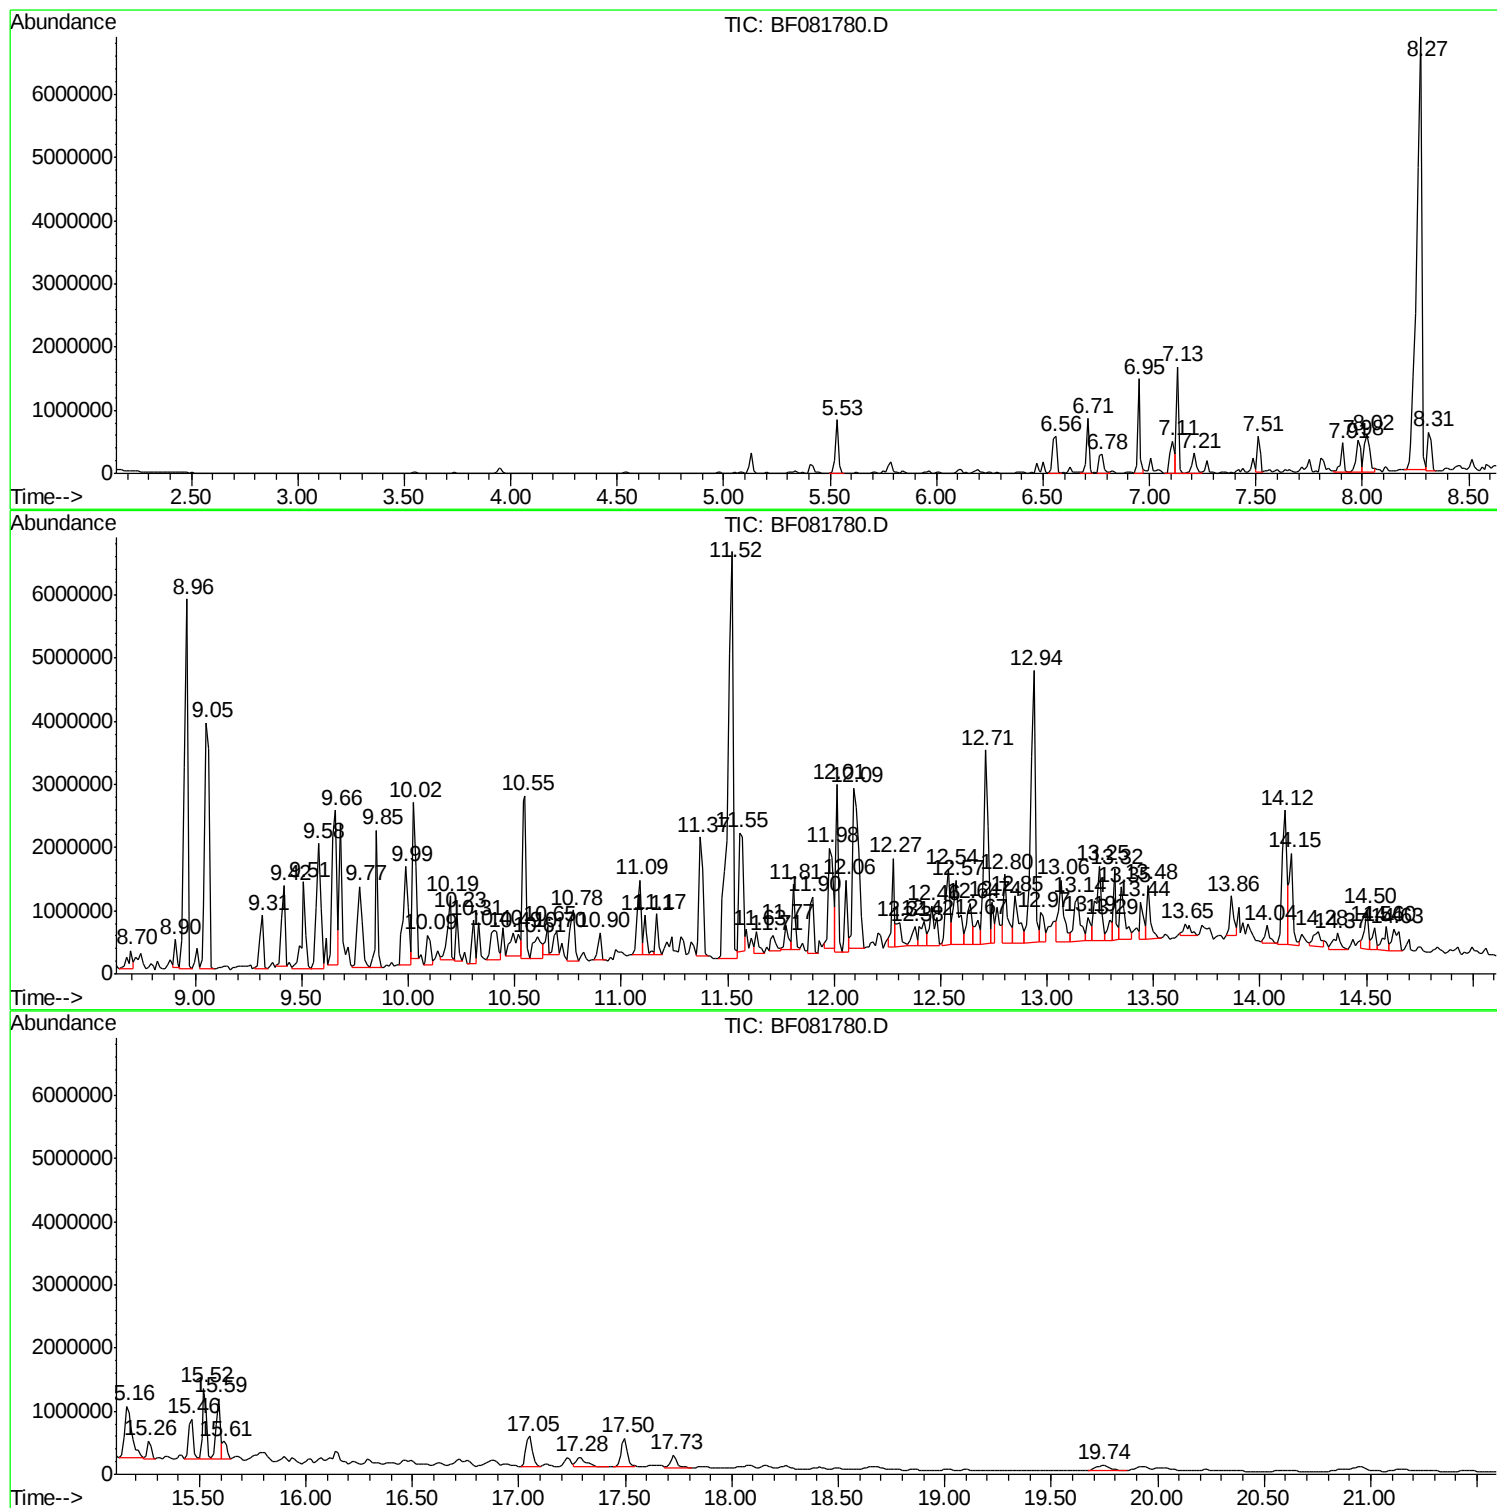

DbaaaPath::ZZ\NRPBMM1BNAFNDAAAB002215\
 DbaaaFile::BB003780DD
 Aeqq00n::24Spp20055 23331
 Oppaaaor::UMMIZ
 Sample::G6378000DL5X
 Misc::
 AASSVaal::133 SampleMultiplier:11

Instrument :
 BNA_F
 ClientSampleId :
 MGP205-10-12DL

QqaabMebbdd::ZZ\NRPBMM1BNAFMEH00S8270BB002215MM
 QqaabTitle::ASBPBNASSANDABBSF00R55P000NTCABBRATION

TICCLibbaay::CC\DAABASSEN0\$002LL
 TICIntegratíonPaaameess:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
