


Data Path : Z:\HPCHEM1\BNA_F\Data\BF092415\
 Data File : BF081768.D
 Acq On : 24 Sep 2015 17:22
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 25 06:02:49 2015

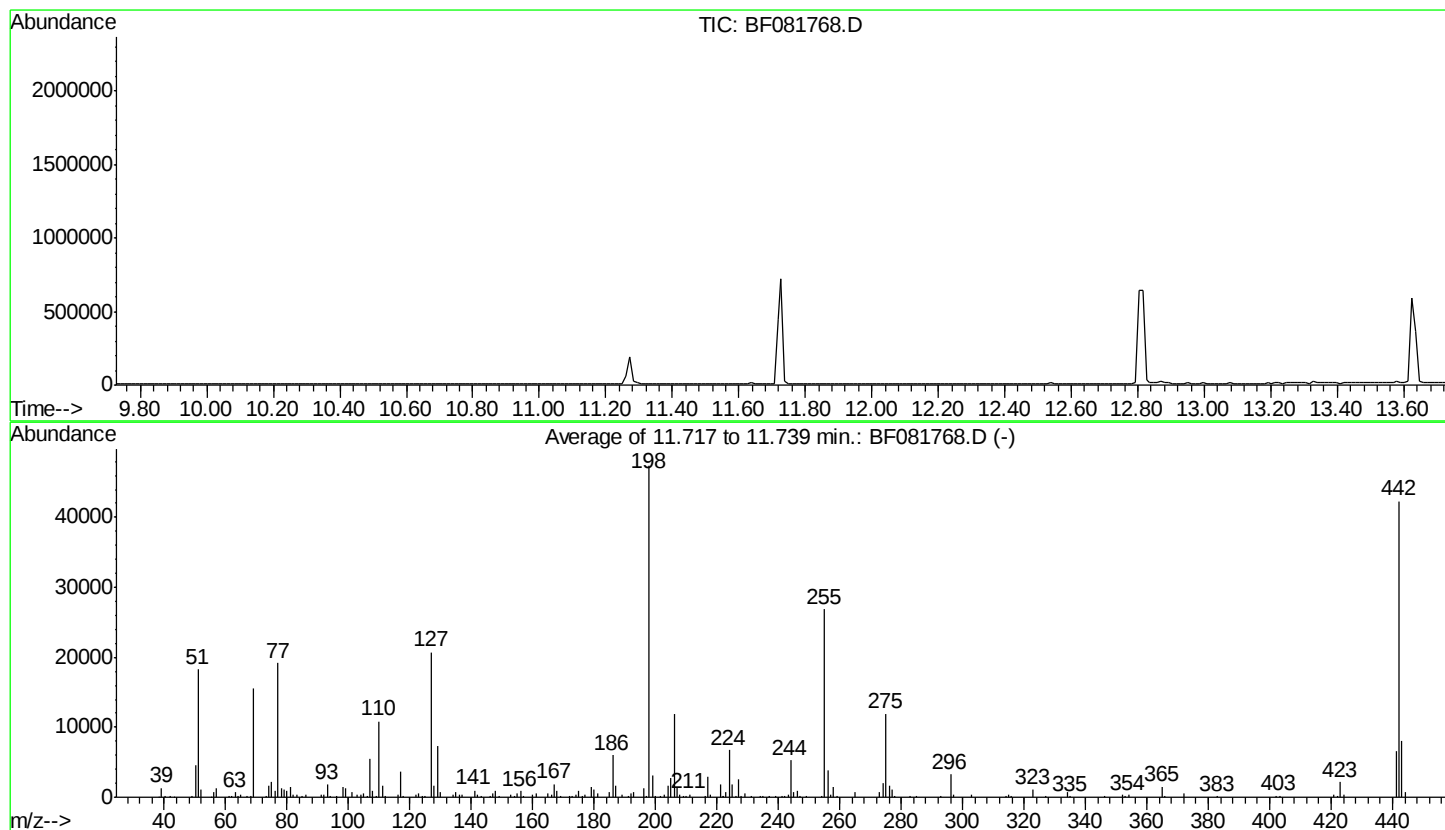

AutoFind: Scans 930, 931, 932; Background Corrected with Scan 927

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	18295	PASS
68	69	0.00	2	1.3	203	PASS
69	198	0.00	100	32.9	15604	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.7	20698	PASS
197	198	0.00	2	0.3	158	PASS
198	198	100	100	100.0	47393	PASS
199	198	5	9	6.7	3189	PASS
275	198	10	60	25.3	11984	PASS
365	198	1	100	3.2	1505	PASS
441	442	0.01	24	15.8	6664	PASS
442	198	50	100	89.2	42276	PASS
443	442	15	24	18.9	8008	PASS