


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092420\
 Data File : BF121677.D
 Acq On : 24 Sep 2020 11:44
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 17:53:26 2020

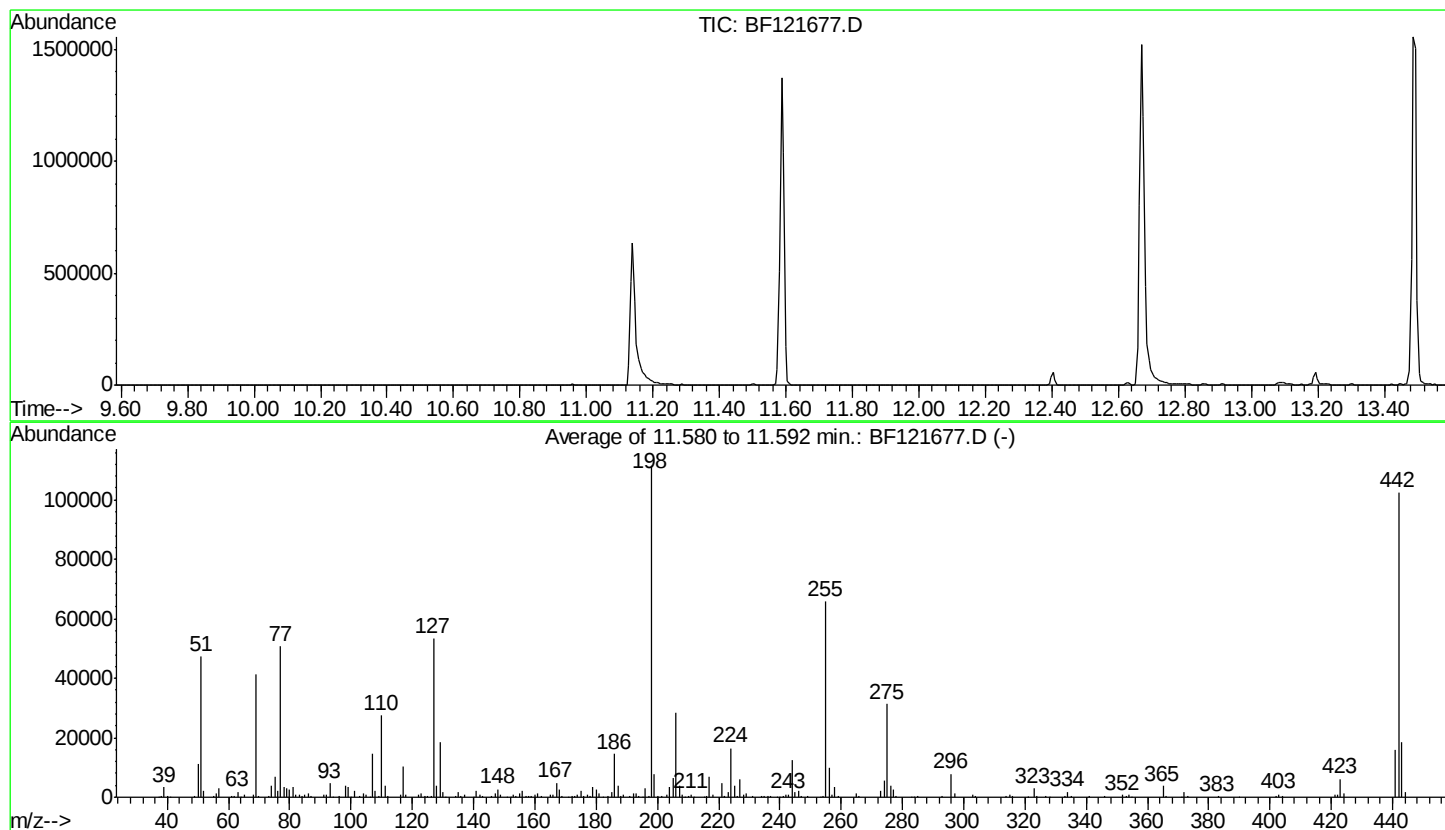

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	47200	PASS
68	69	0.00	2	1.9	772	PASS
69	198	0.00	100	36.9	41170	PASS
70	69	0.00	2	0.6	257	PASS
127	198	10	80	47.8	53306	PASS
197	198	0.00	2	0.4	417	PASS
198	198	100	100	100.0	111541	PASS
199	198	5	9	6.8	7594	PASS
275	198	10	60	28.1	31288	PASS
365	198	1	100	3.4	3807	PASS
441	198	0.01	100	14.4	16007	PASS
442	198	50	100	91.7	102293	PASS
443	442	15	24	18.1	18482	PASS