



Benzaldehyde

Response Ratio

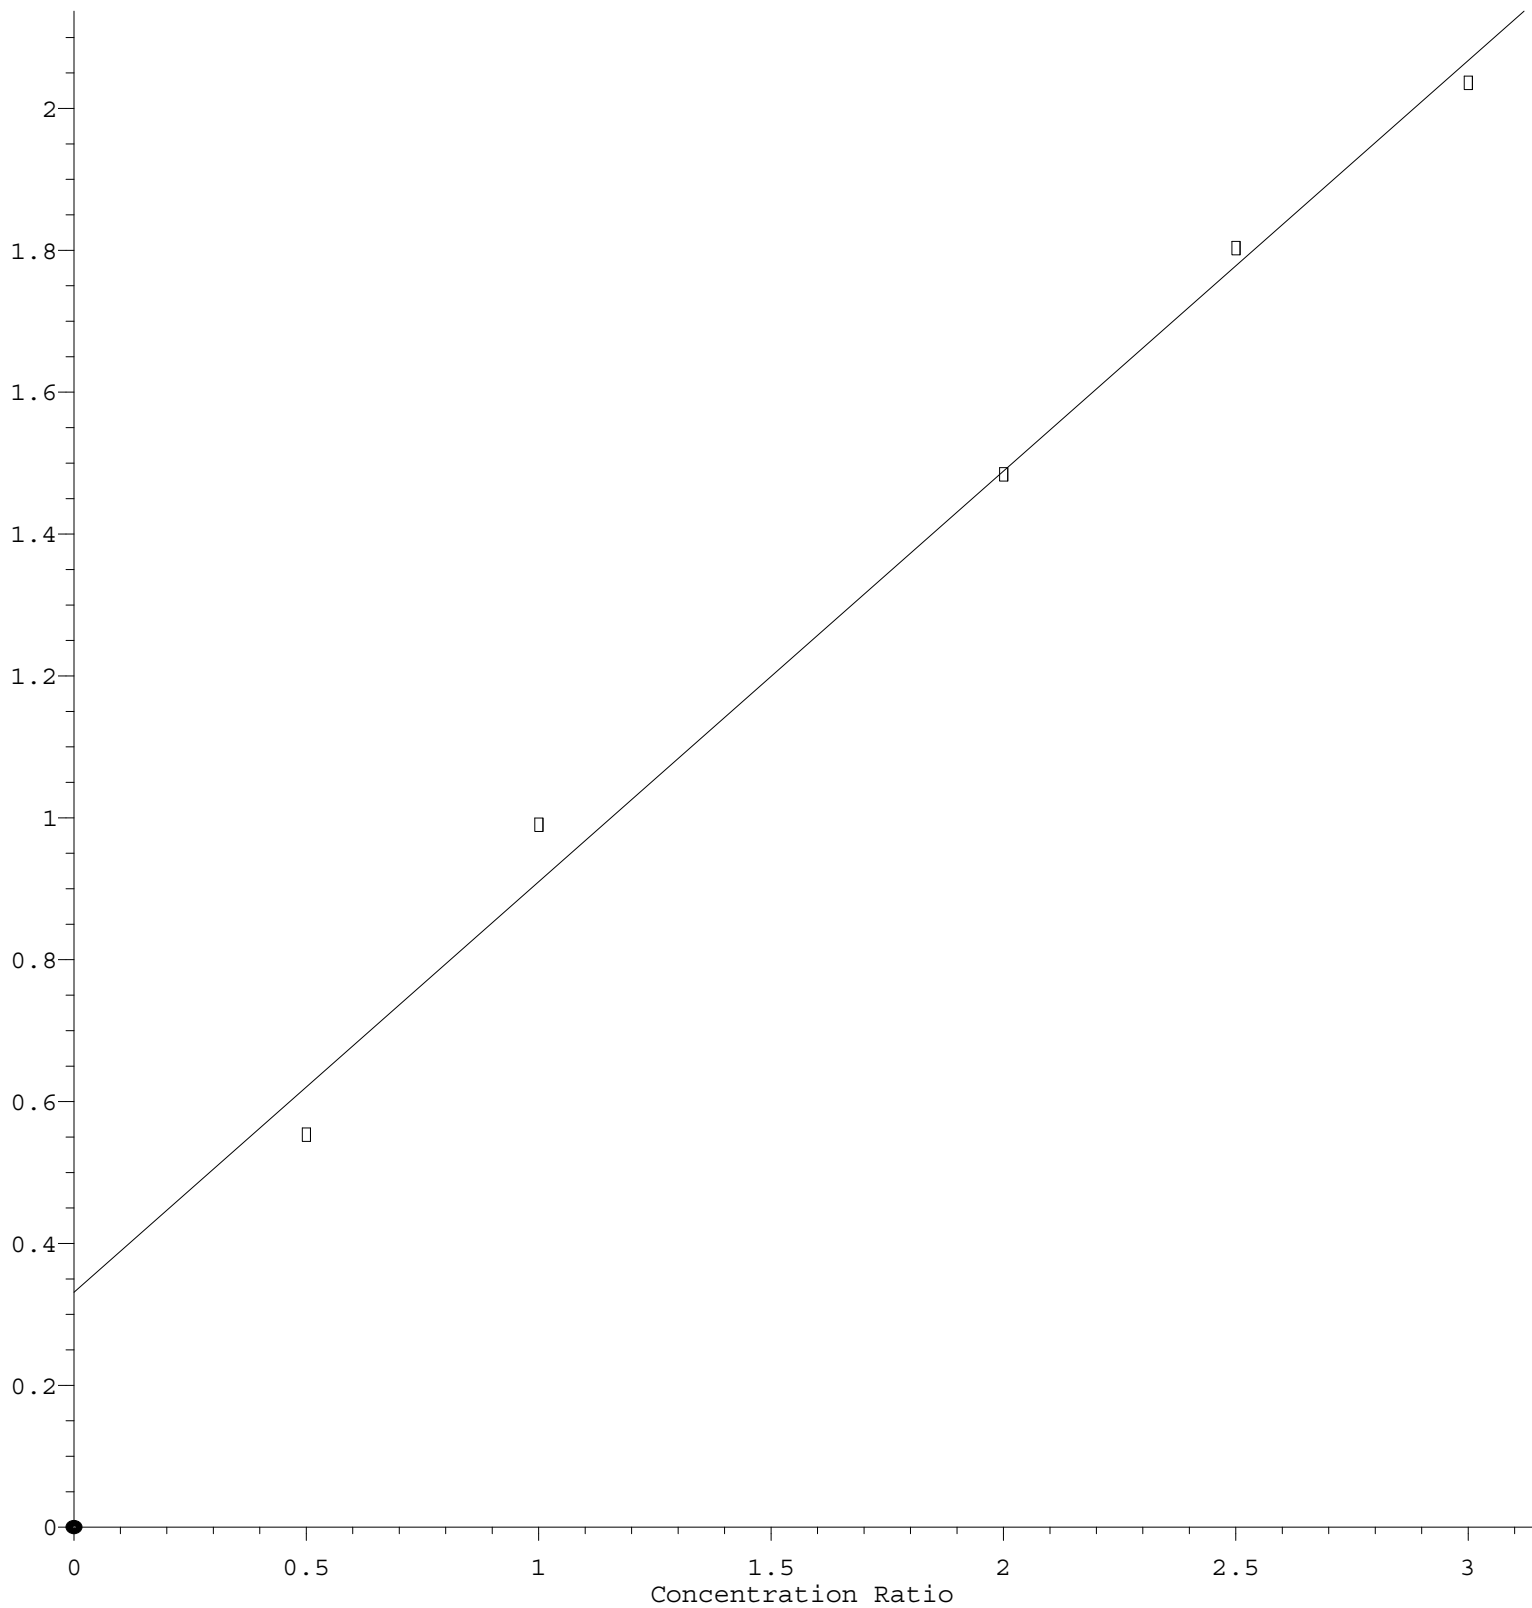

Response = 5.793e-001 * Amt + 3.306e-001
Coef of Det (r^2) = 0.991339 Curve Fit: Linear
Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M
Calibration Table Last Updated: Fri Sep 24 15:38:32 2021


2-Nitrophenol

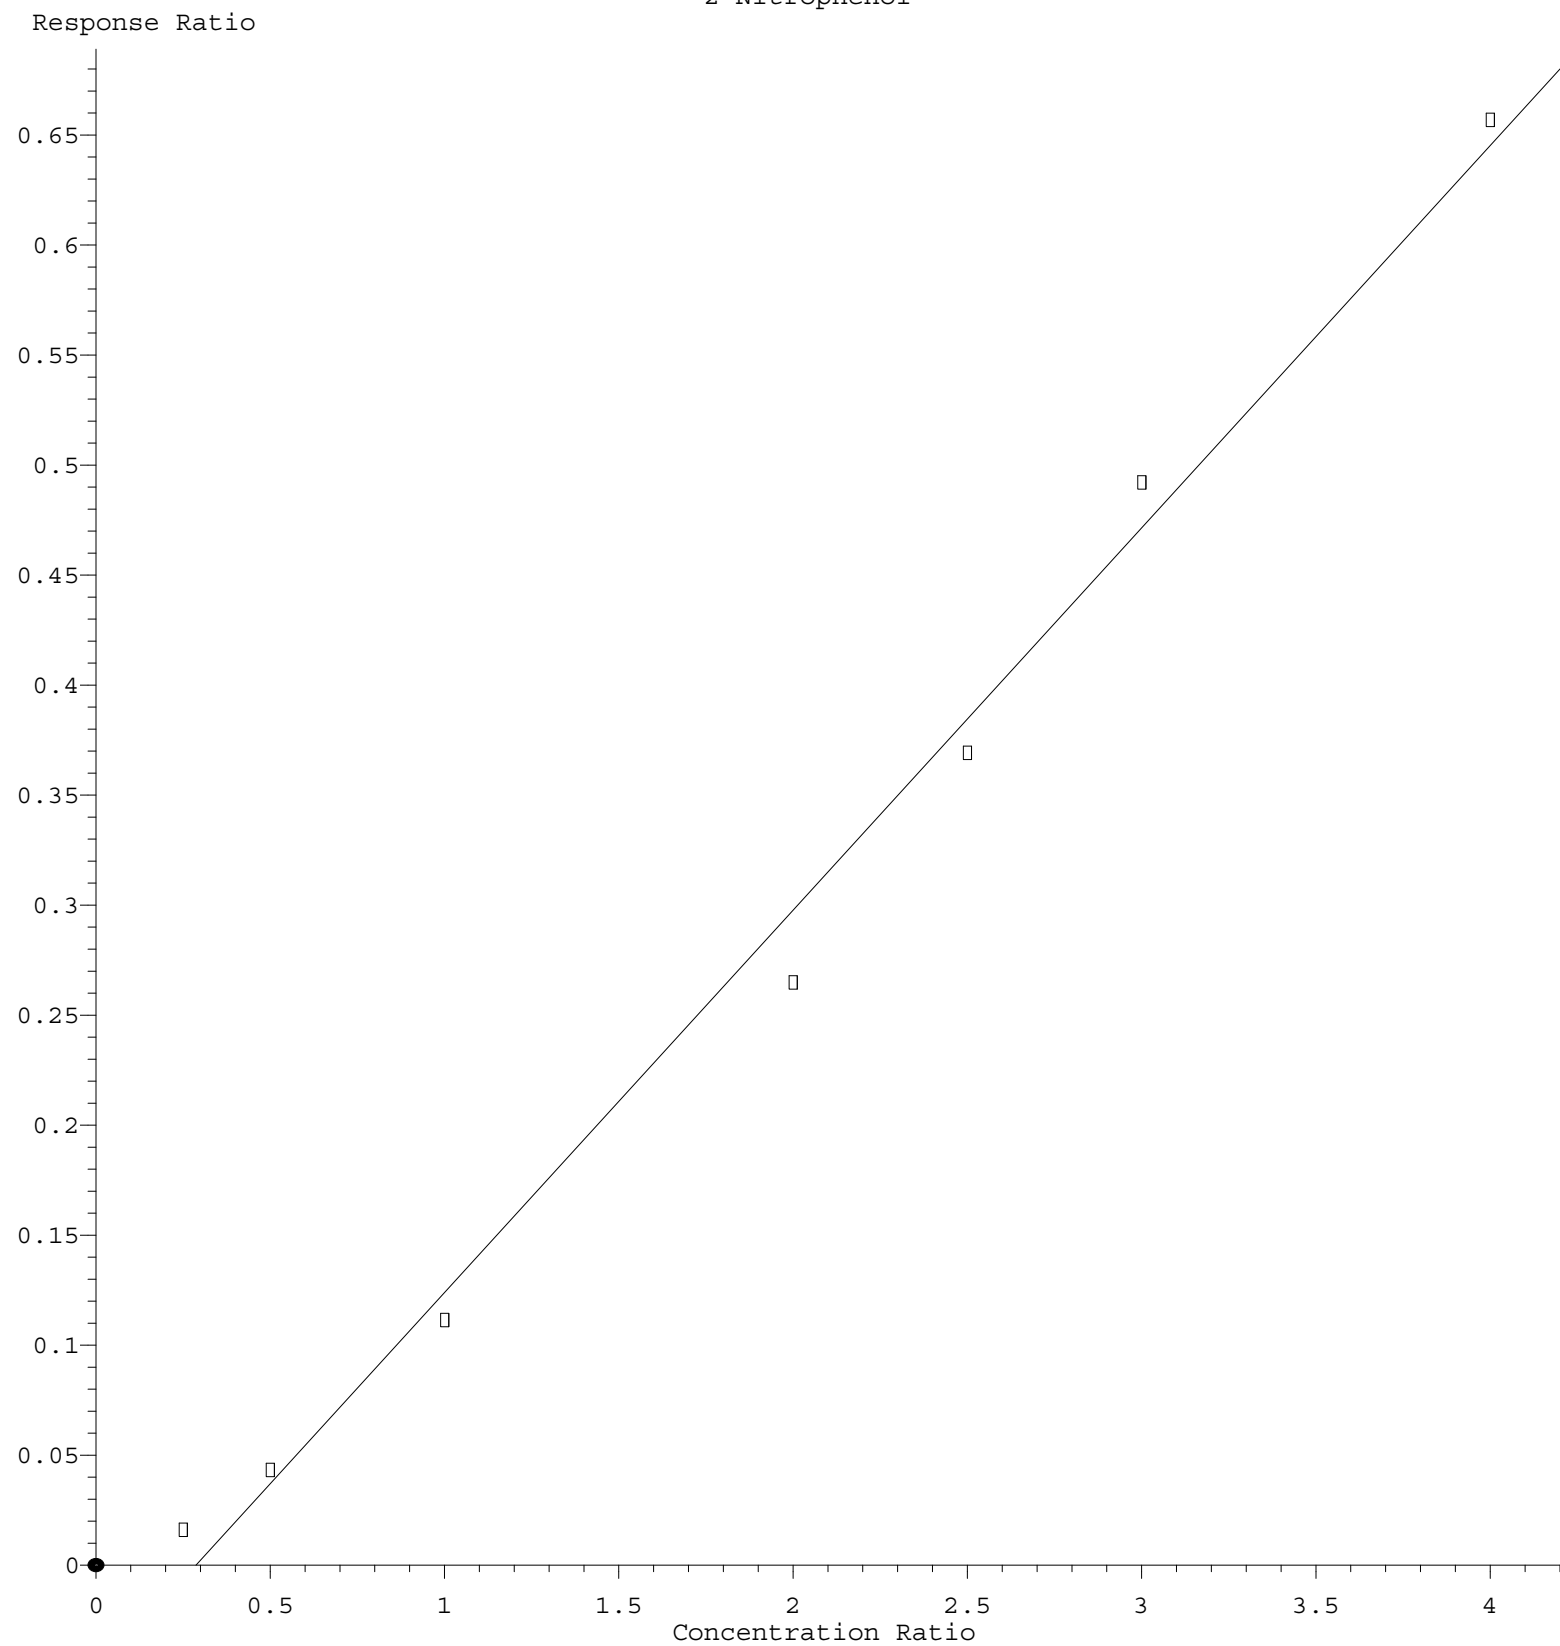

Response = 1.738e-001 * Amt - 4.982e-002
 Coef of Det (r^2) = 0.992630 Curve Fit: Linear
 Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M
 Calibration Table Last Updated: Fri Sep 24 15:38:32 2021

Benzoic acid

Response Ratio

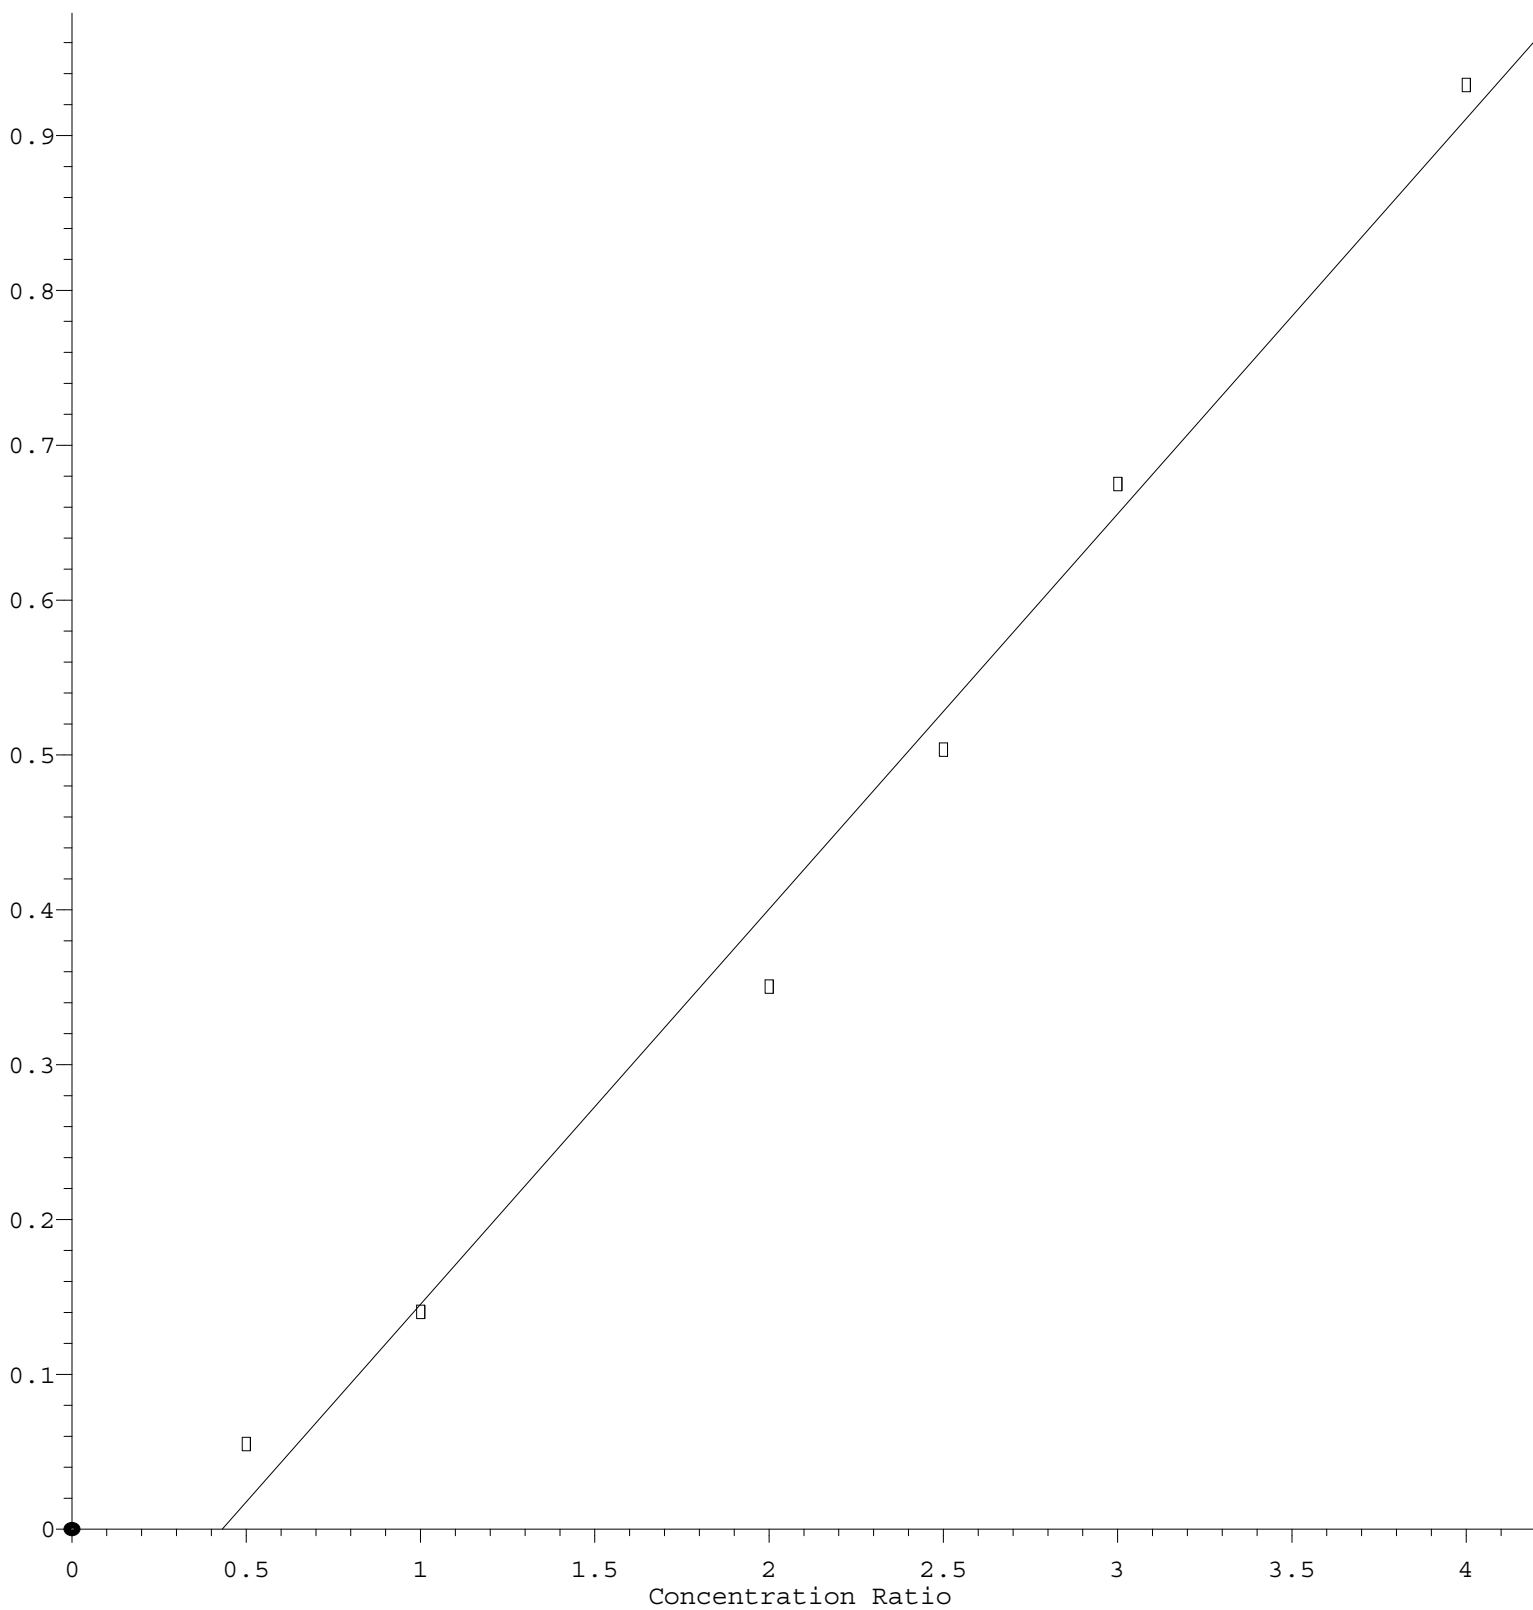

$$\text{Response} = 2.552\text{e-}001 * \text{Amt} - 1.101\text{e-}001$$


Coef of Det (r^2) = 0.990195 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M

Calibration Table Last Updated: Fri Sep 24 15:38:32 2021

2-Fluorobiphenyl

Response Ratio

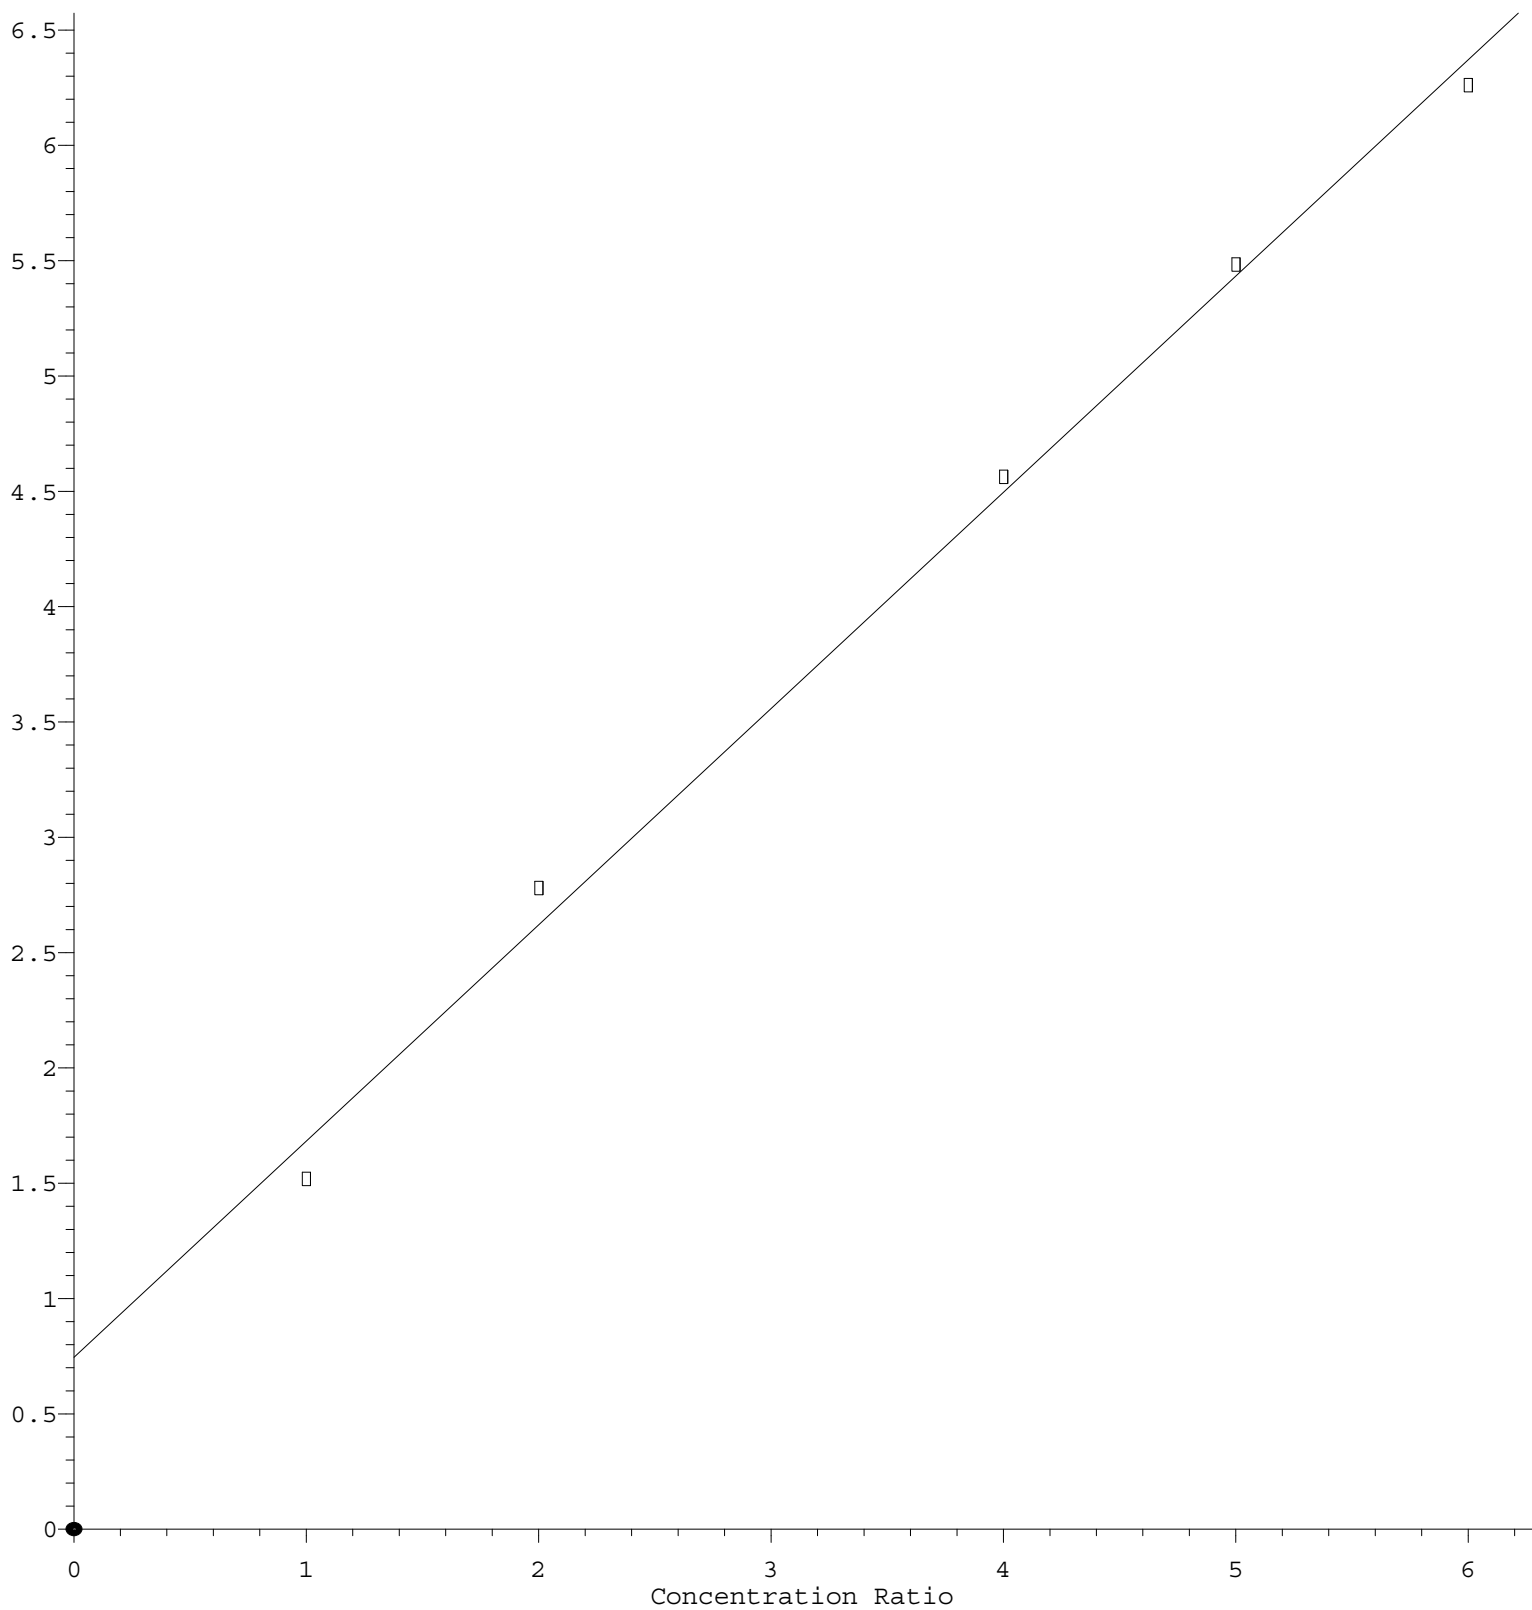

$$\text{Response} = 9.379\text{e-}001 * \text{Amt} + 7.445\text{e-}001$$


Coef of Det (r^2) = 0.995293 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M

Calibration Table Last Updated: Fri Sep 24 15:38:32 2021

2-Nitroaniline

Response Ratio

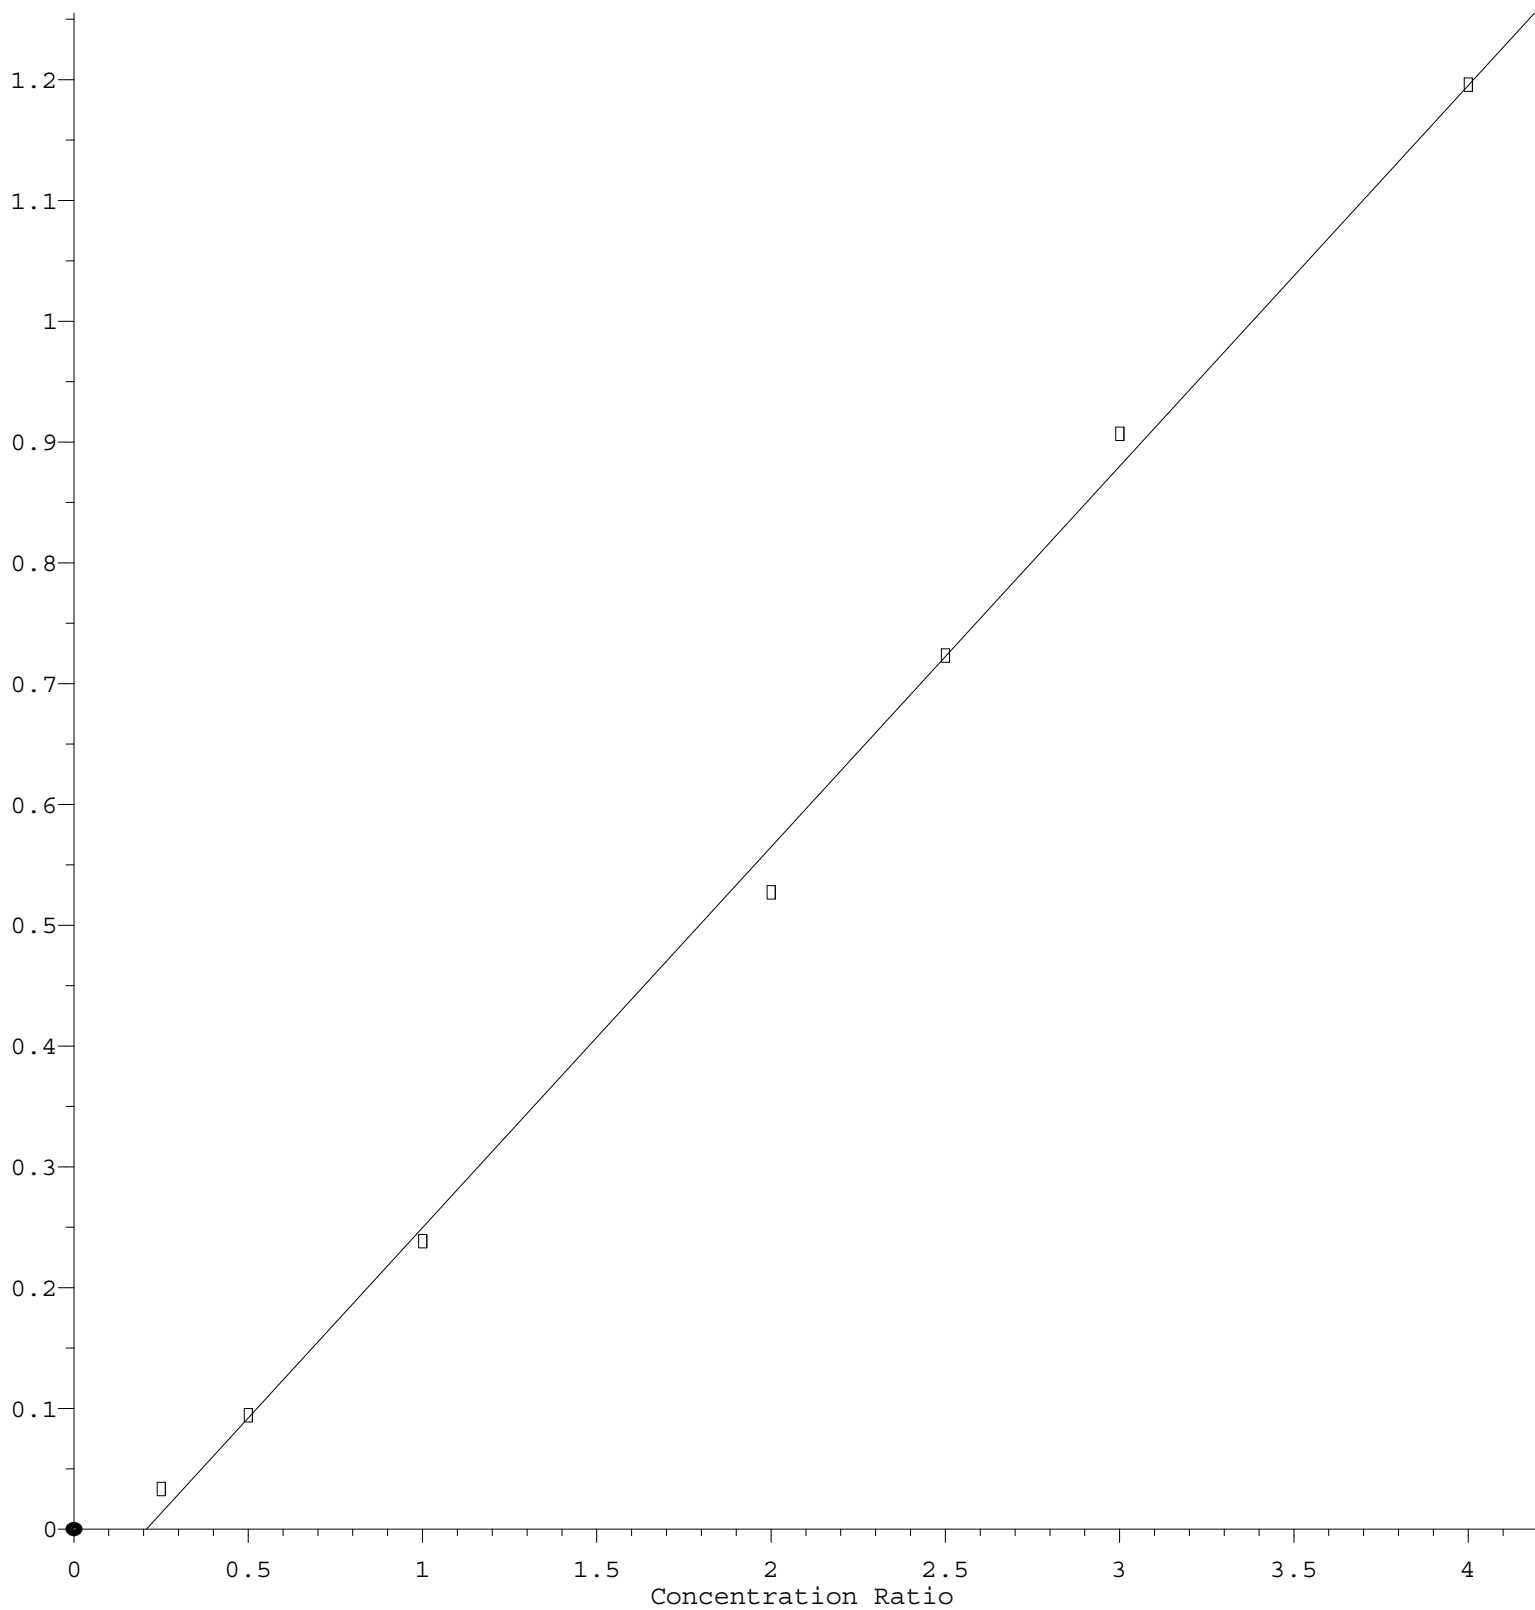

$$\text{Response} = 3.153\text{e-}001 * \text{Amt} - 6.554\text{e-}002$$


Coef of Det (r^2) = 0.997666 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M

Calibration Table Last Updated: Fri Sep 24 15:38:32 2021

2,6-Dinitrotoluene

Response Ratio

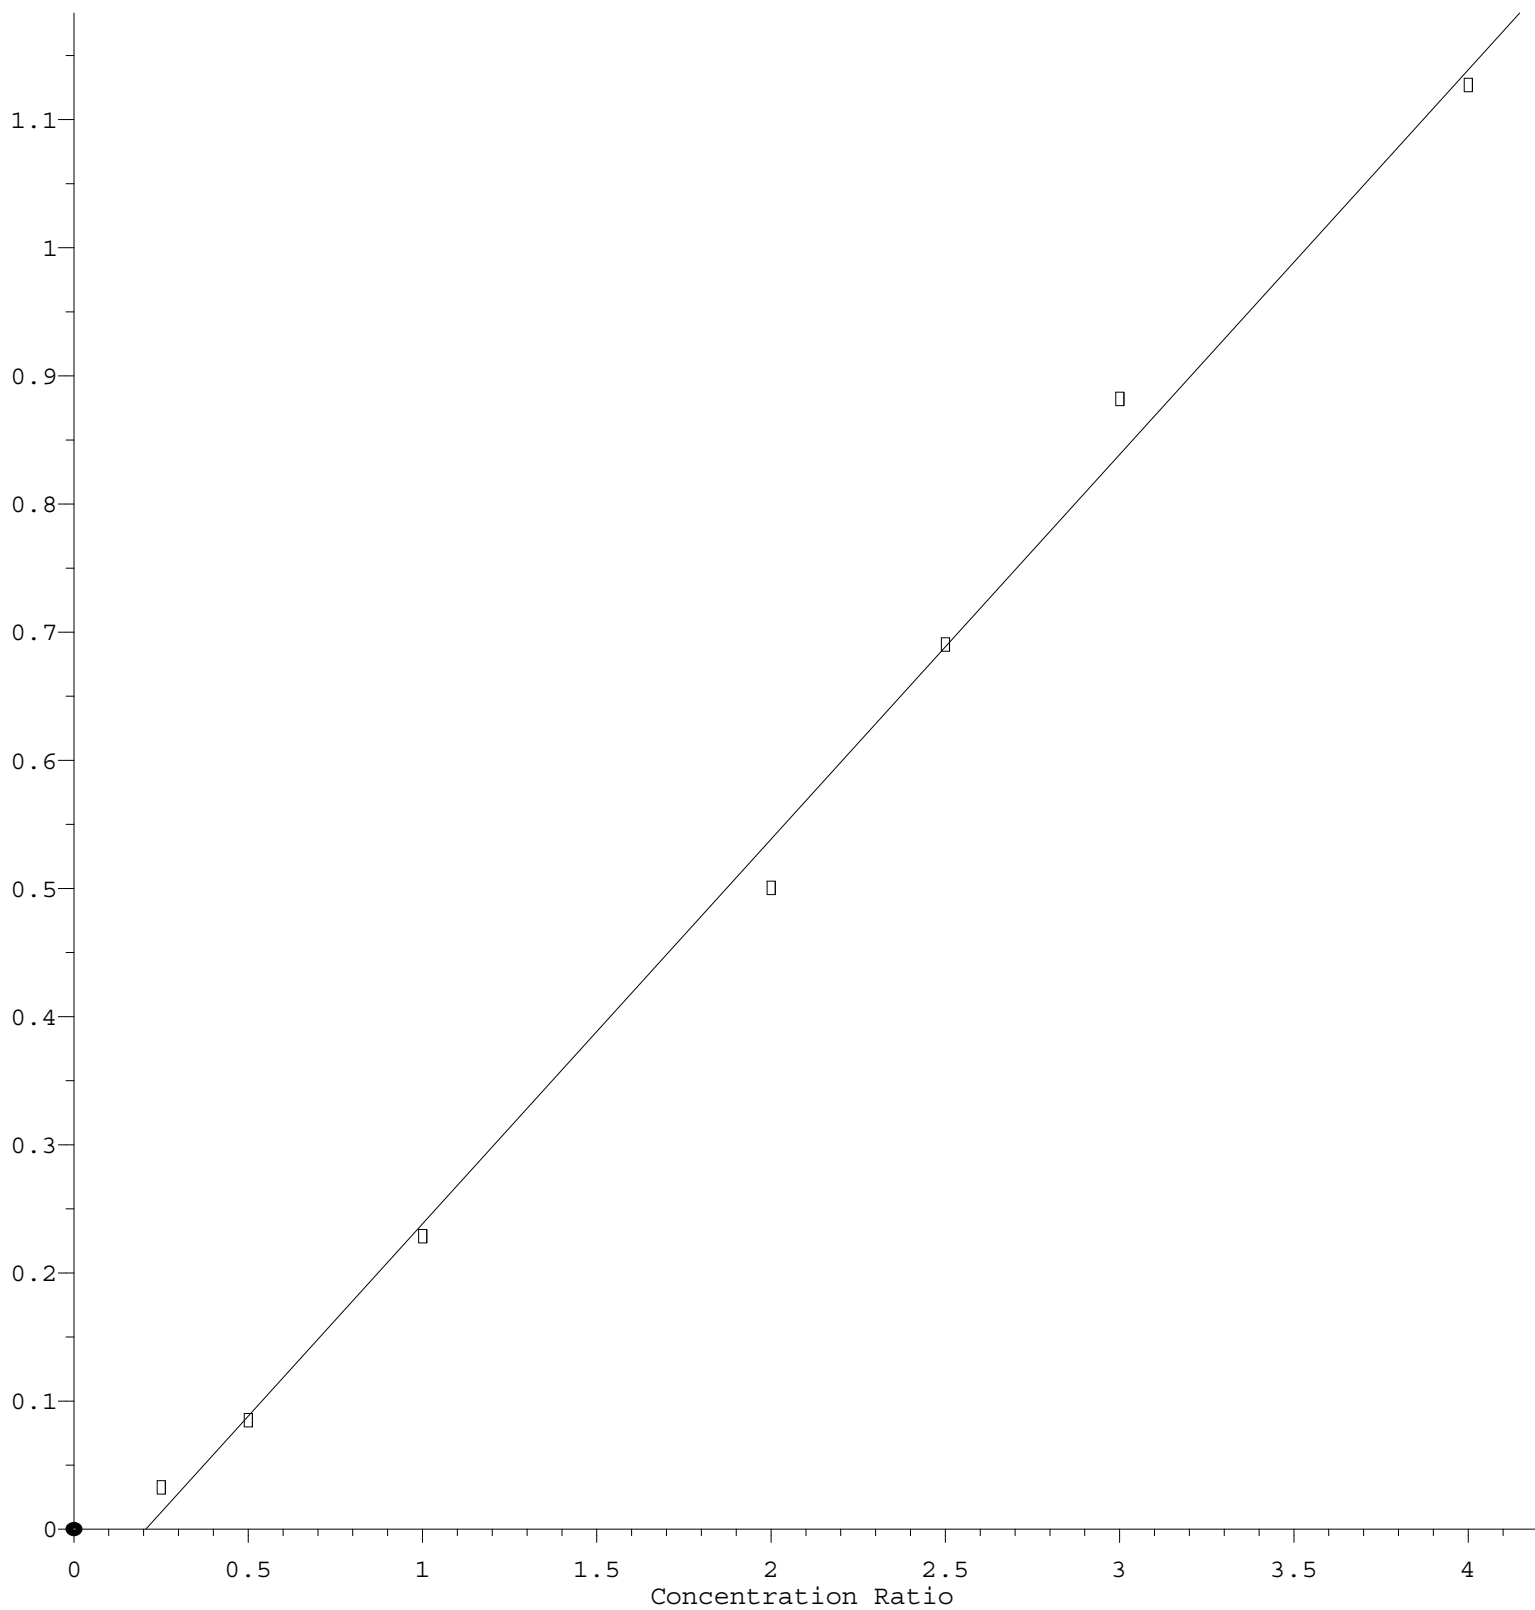

$$\text{Response} = 3.003\text{e-}001 * \text{Amt} - 6.182\text{e-}002$$


Coef of Det (r^2) = 0.996197 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M

Calibration Table Last Updated: Fri Sep 24 15:38:32 2021

3-Nitroaniline

Response Ratio

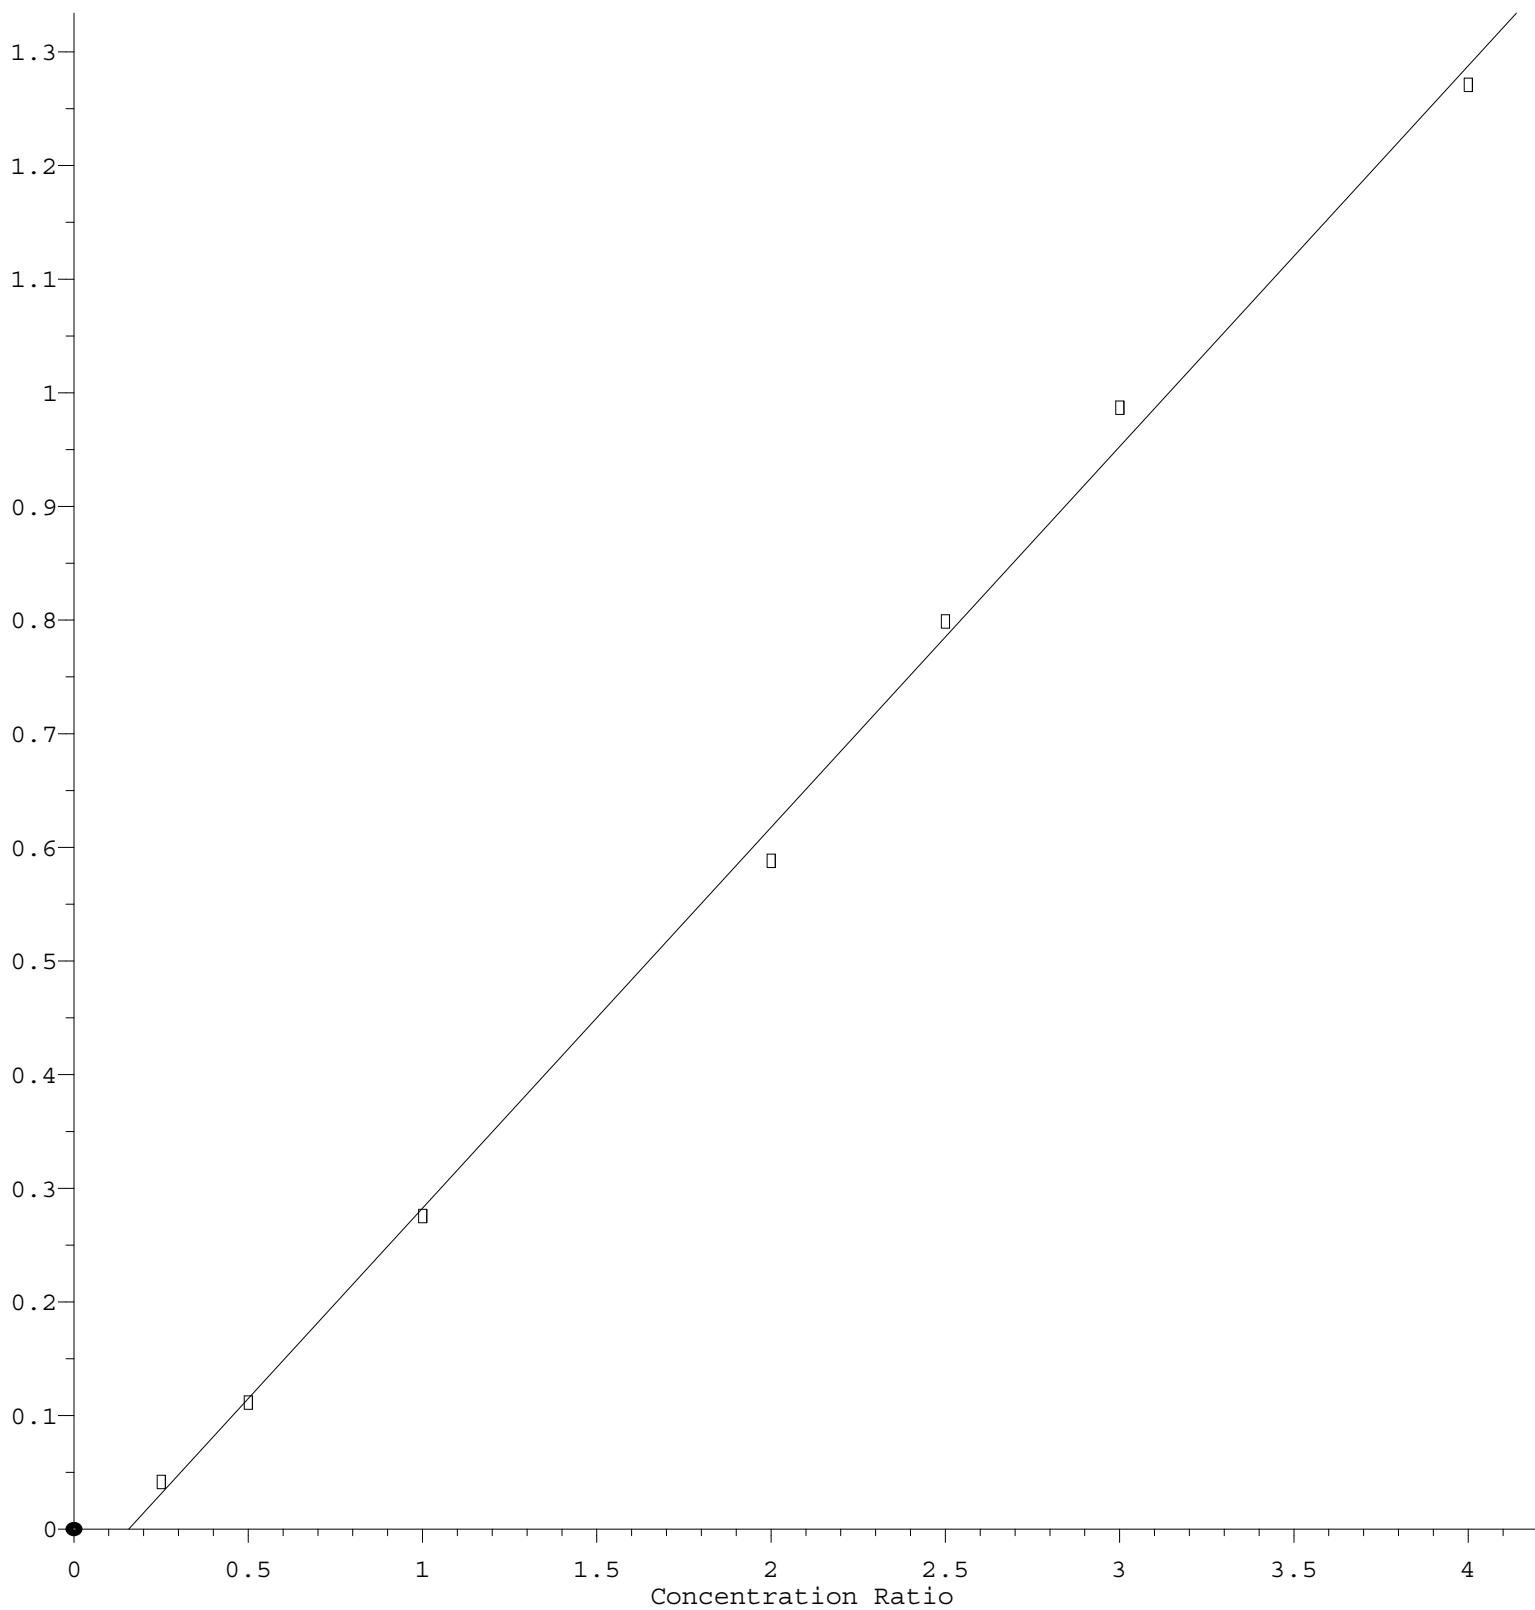


$$\text{Response} = 3.352\text{e-}001 * \text{Amt} - 5.268\text{e-}002$$

Coef of Det (r^2) = 0.997935 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M

Calibration Table Last Updated: Fri Sep 24 15:38:32 2021


2,4-Dinitrophenol

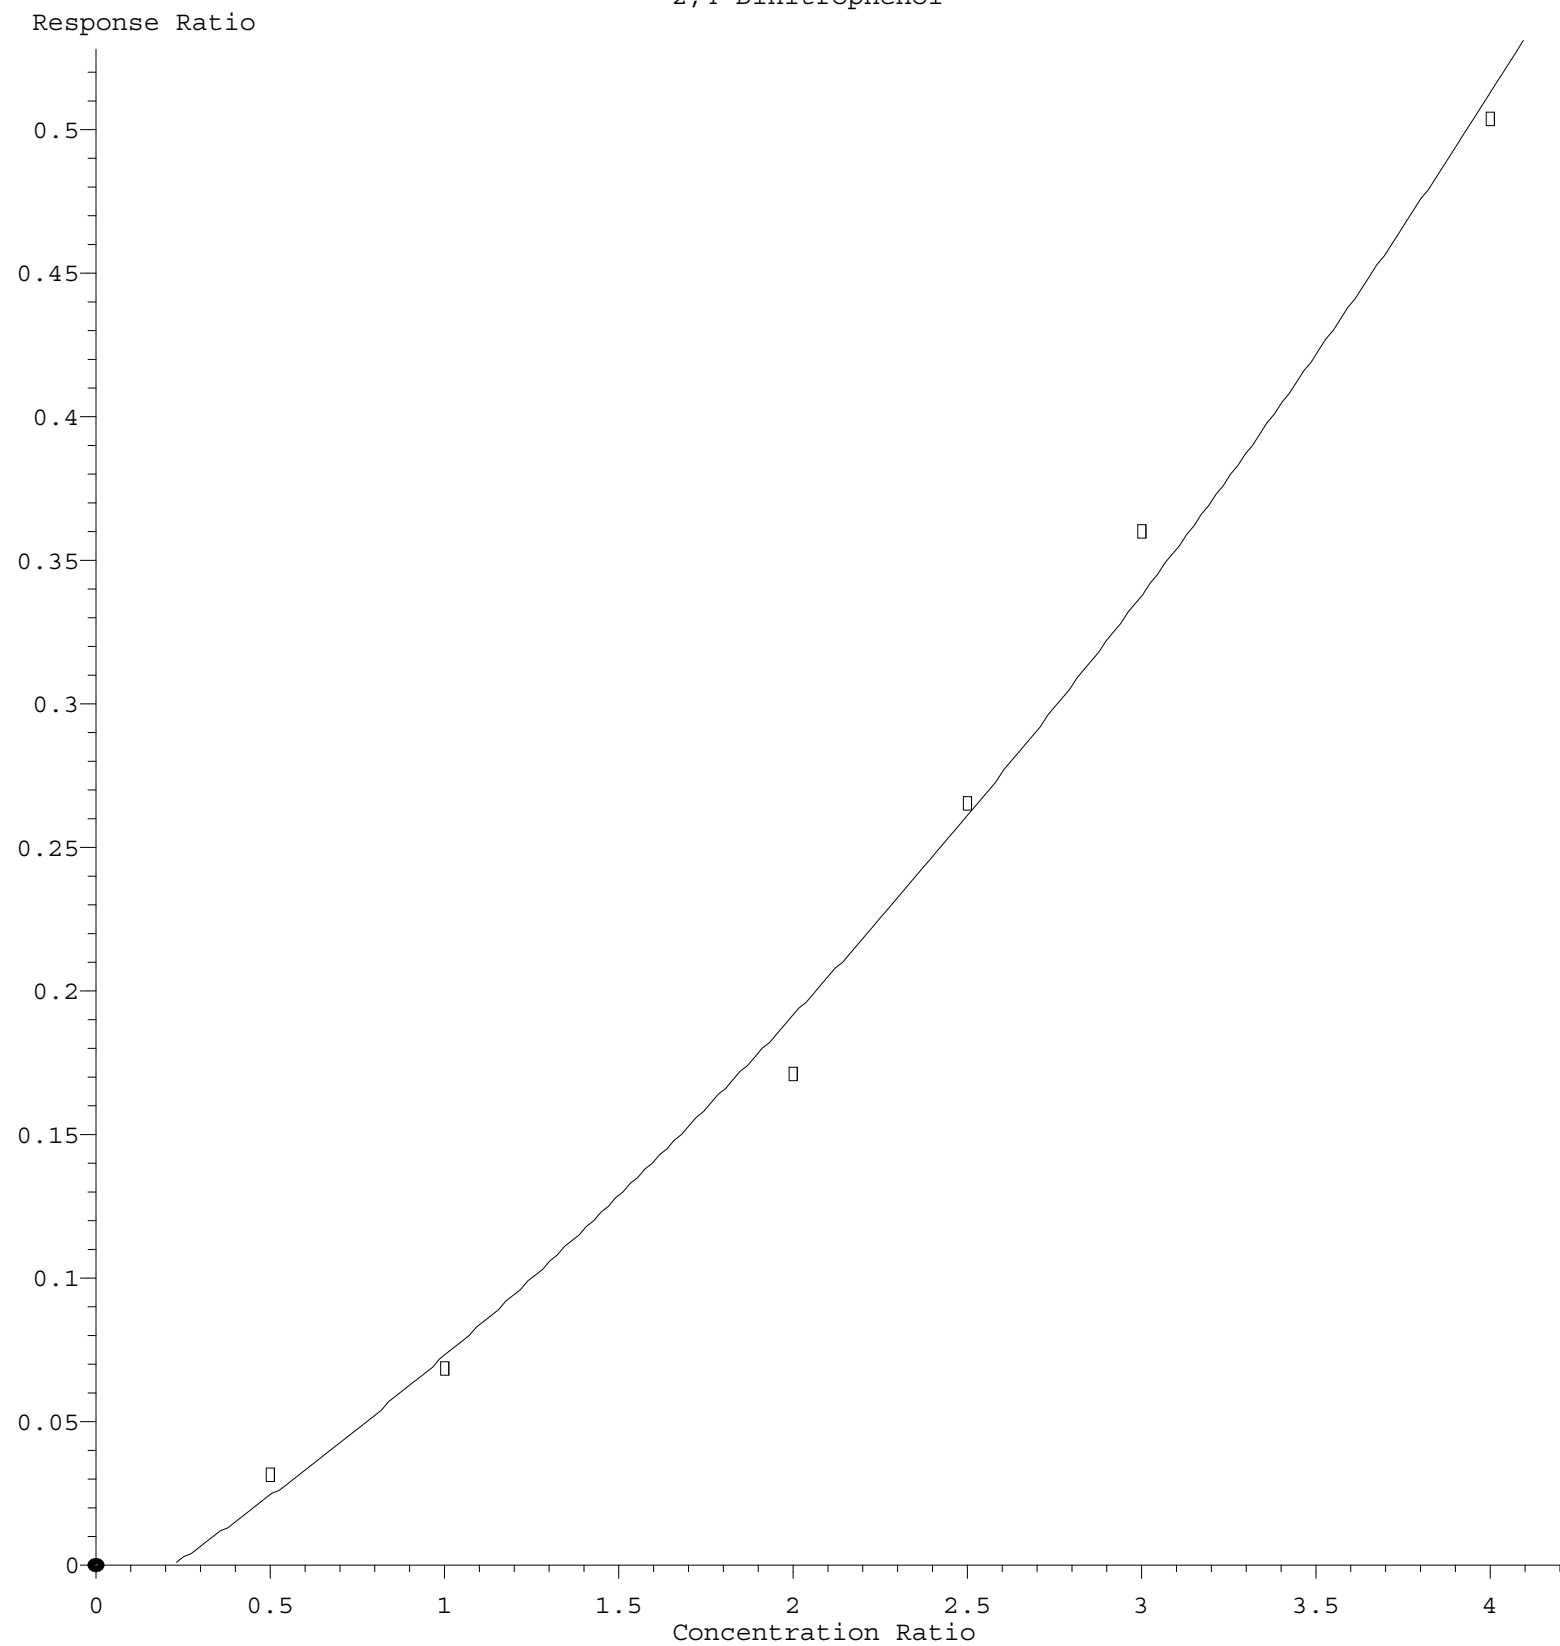

$R = 1.402e-002 A^2 + 7.642e-002 A - 1.753e-002$
 Coef of Det (r^2) = 0.993399 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M
 Calibration Table Last Updated: Fri Sep 24 15:38:32 2021

2,4-Dinitrotoluene

Response Ratio

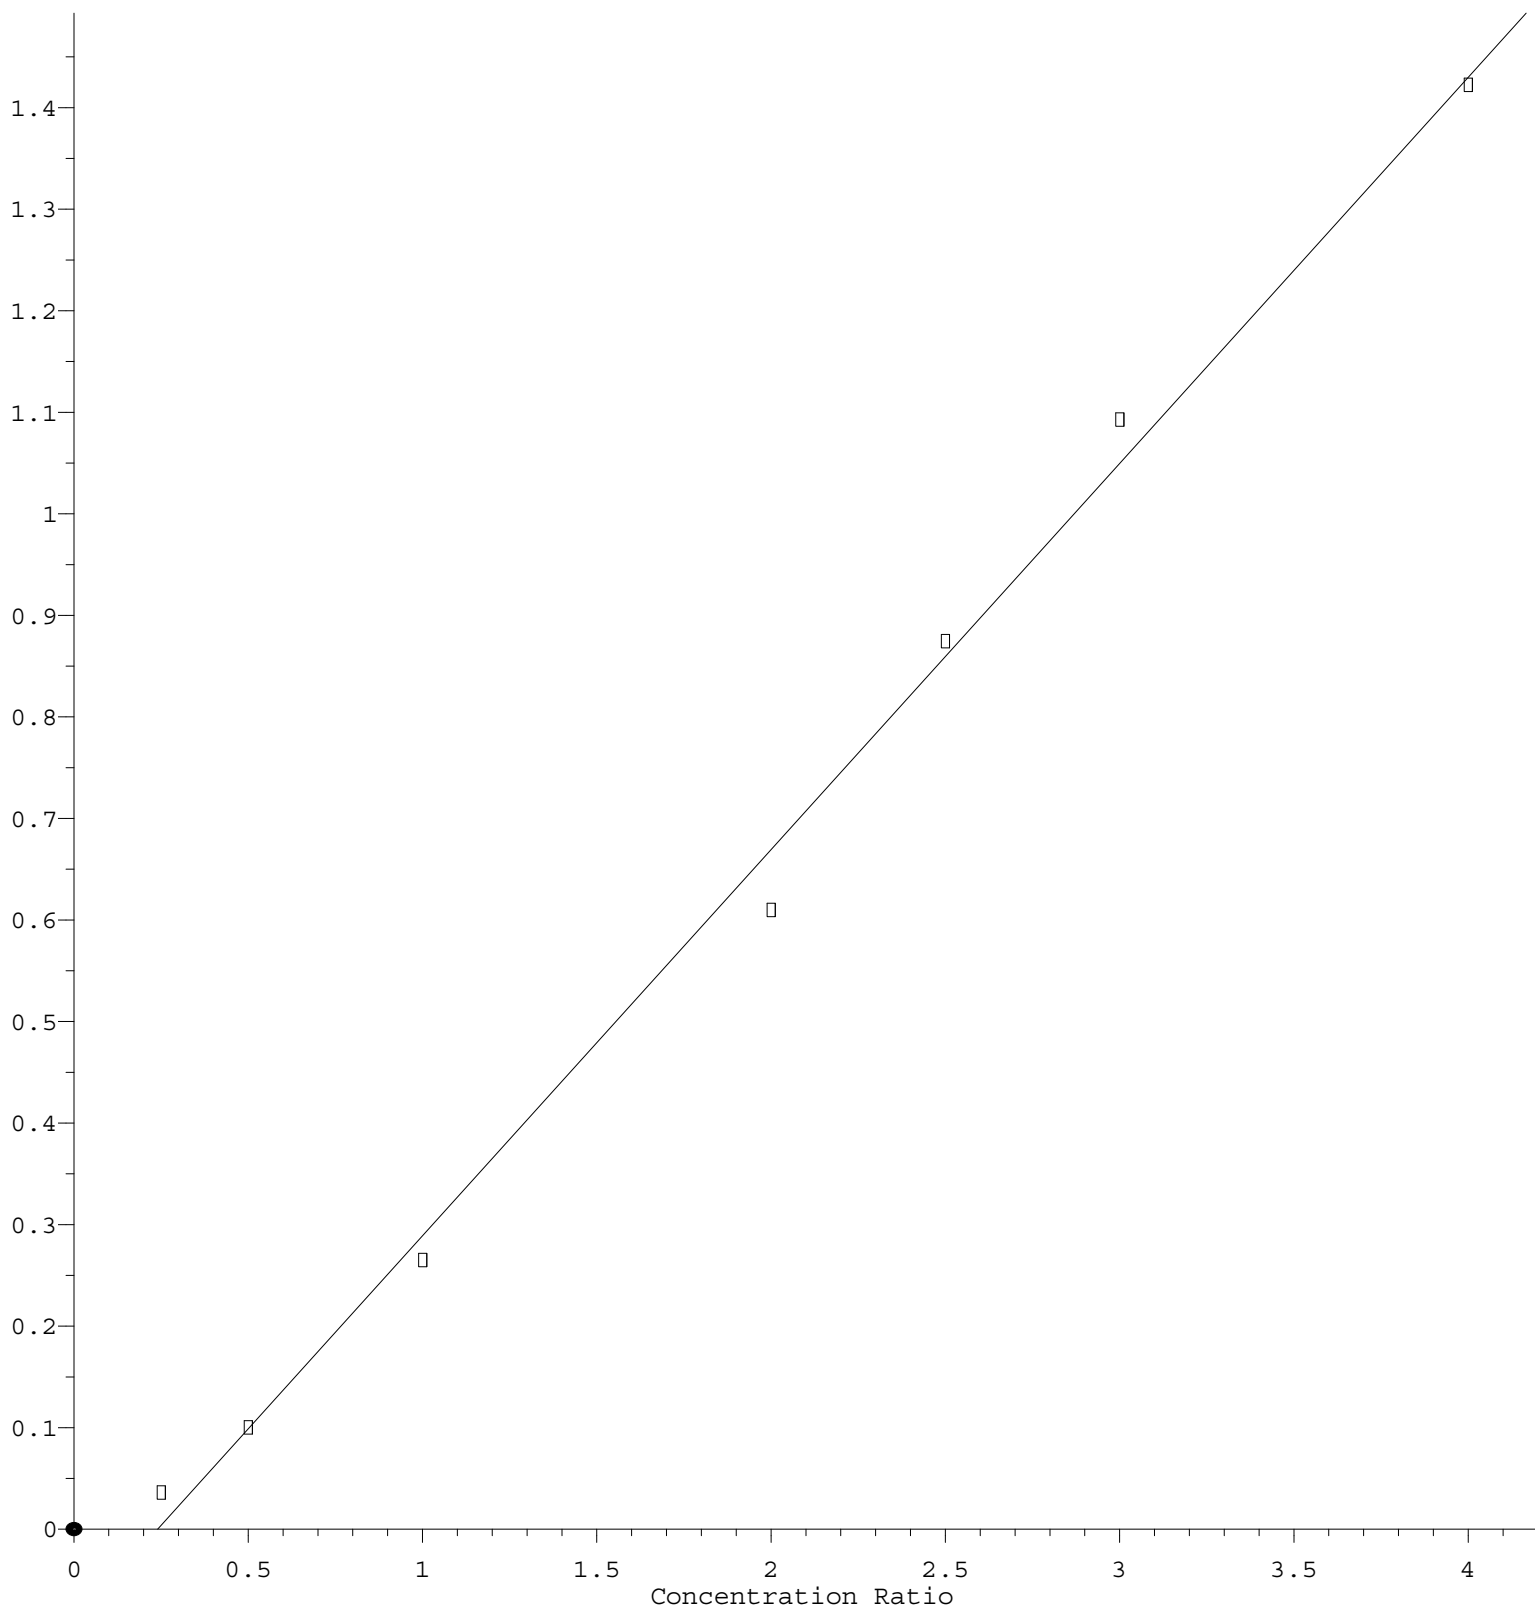

$$\text{Response} = 3.804\text{e-}001 * \text{Amt} - 9.134\text{e-}002$$


Coef of Det (r^2) = 0.995616 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M

Calibration Table Last Updated: Fri Sep 24 15:38:32 2021

4-Nitroaniline

Response Ratio

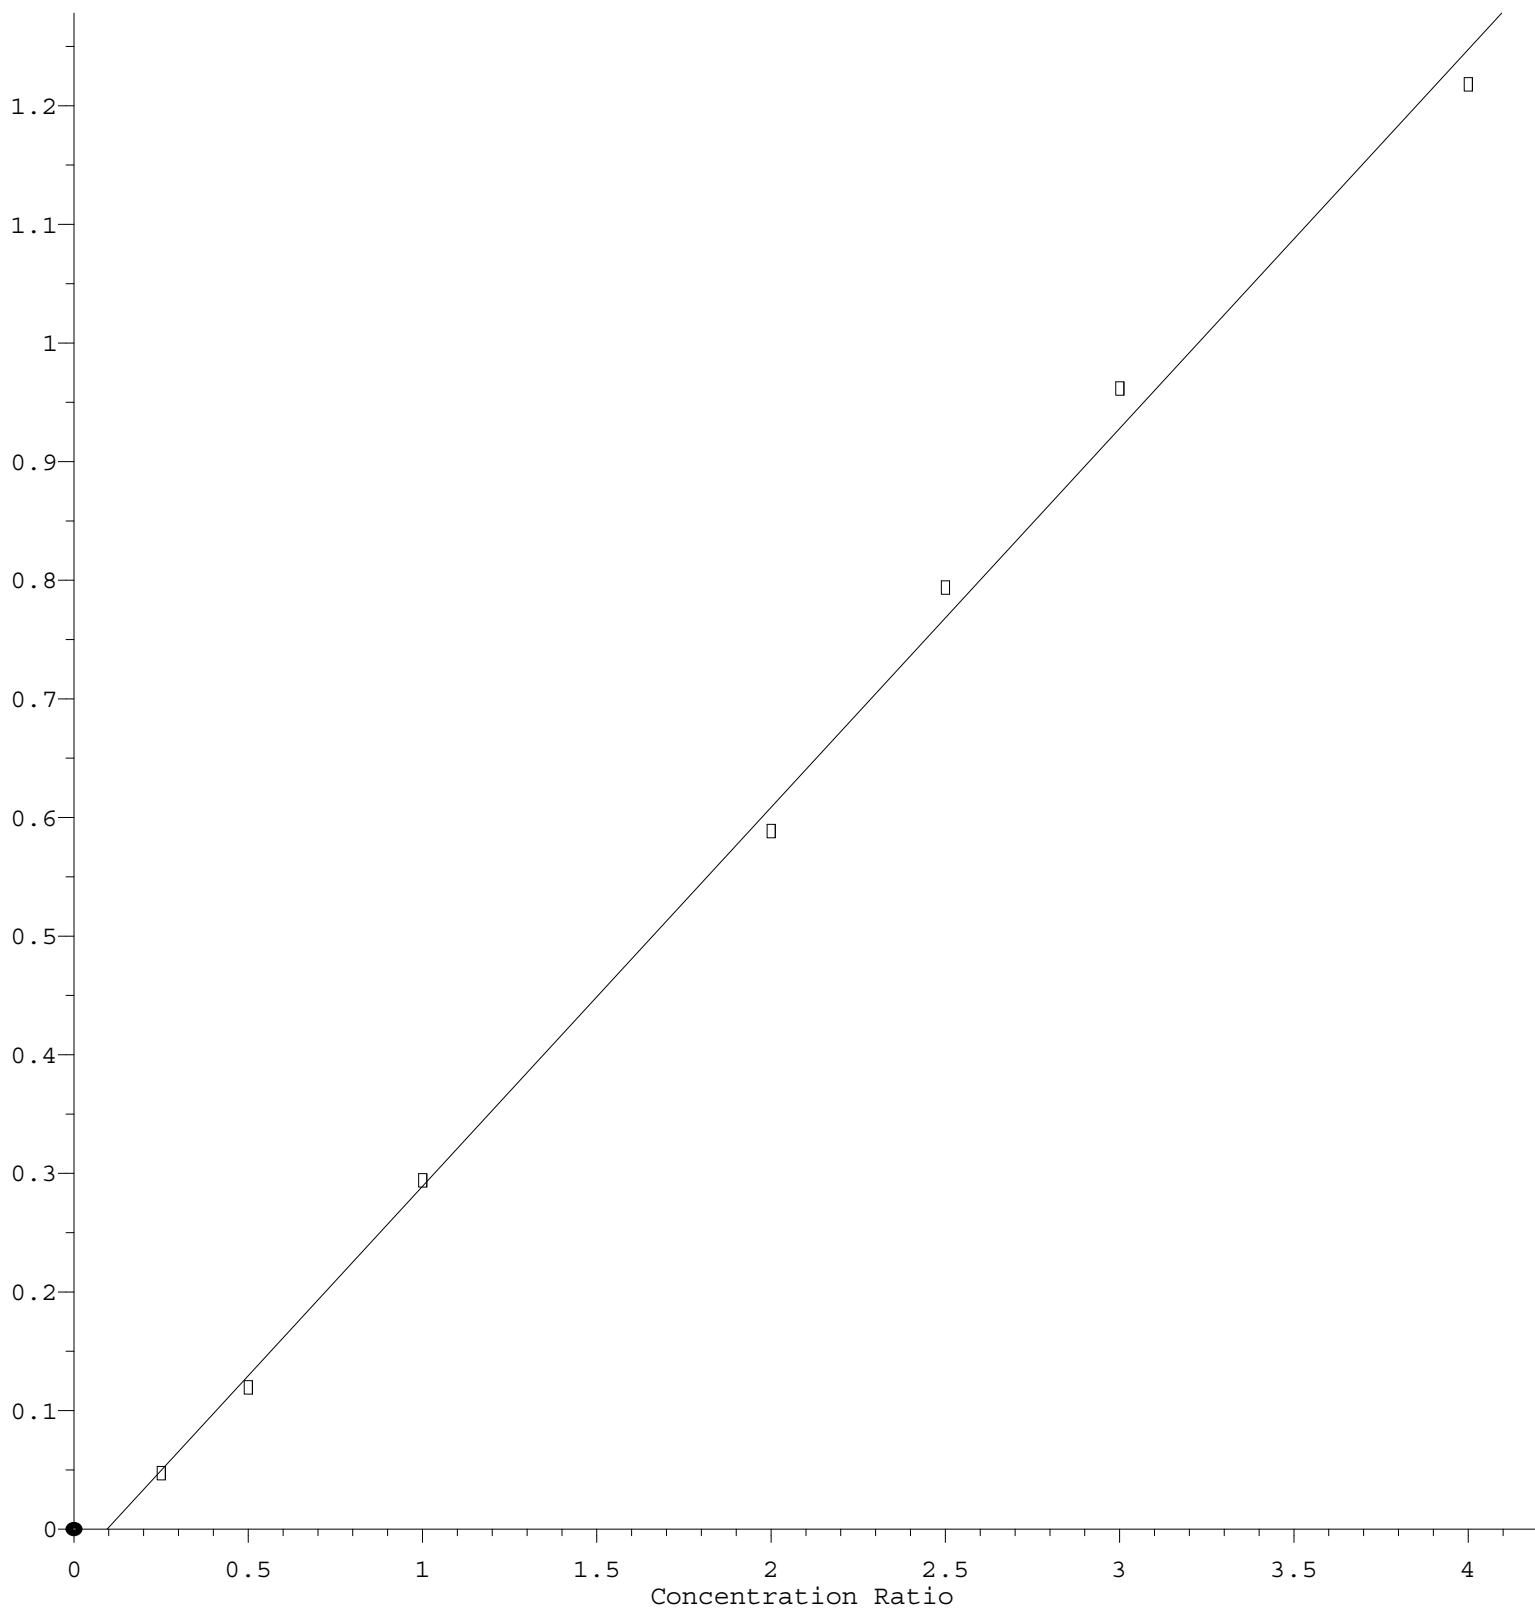


$$\text{Response} = 3.196\text{e-}001 * \text{Amt} - 3.029\text{e-}002$$

Coef of Det (r^2) = 0.997302 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M

Calibration Table Last Updated: Fri Sep 24 15:38:32 2021

4,6-Dinitro-2-methylphenol

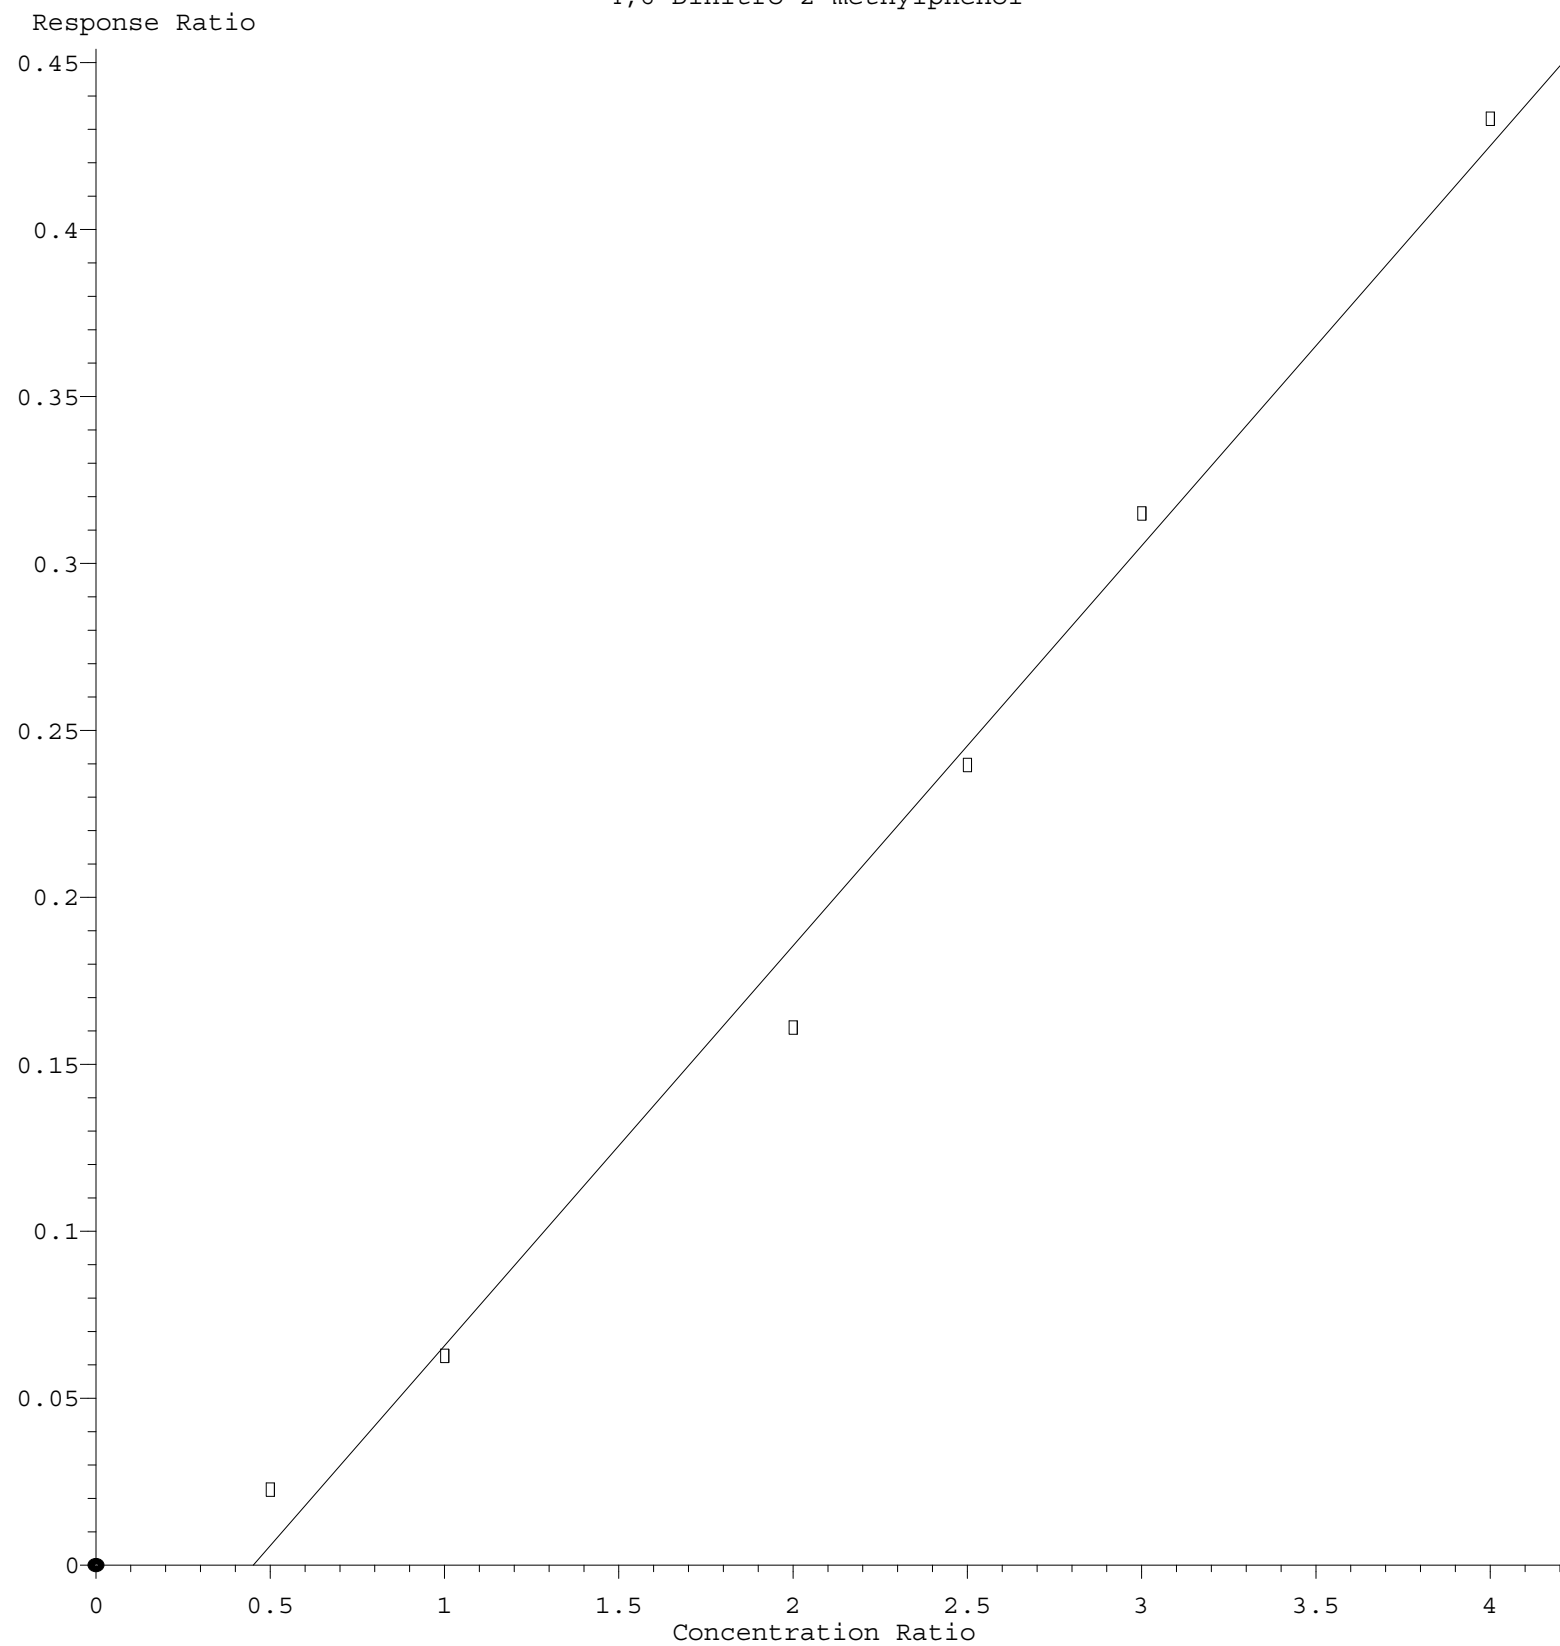

Response = 1.199e-001 * Amt - 5.401e-002
 Coef of Det (r^2) = 0.991028 Curve Fit: Linear
 Method Name: Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092421.M
 Calibration Table Last Updated: Fri Sep 24 15:38:32 2021