
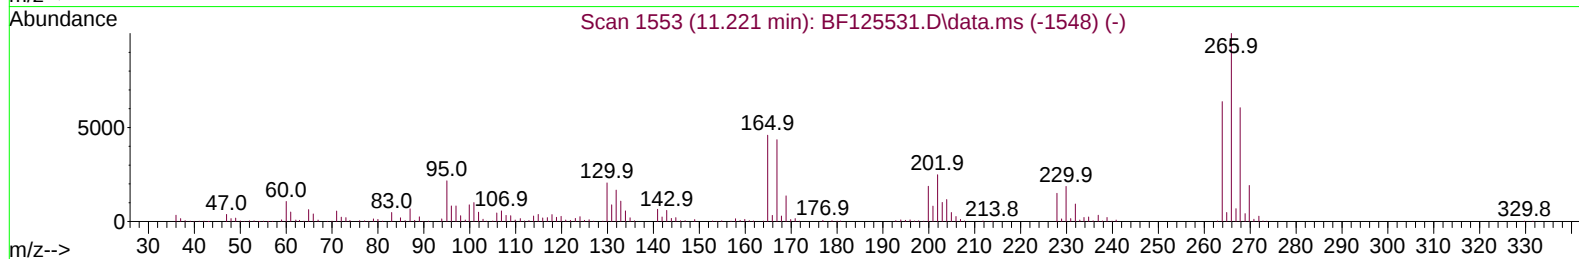
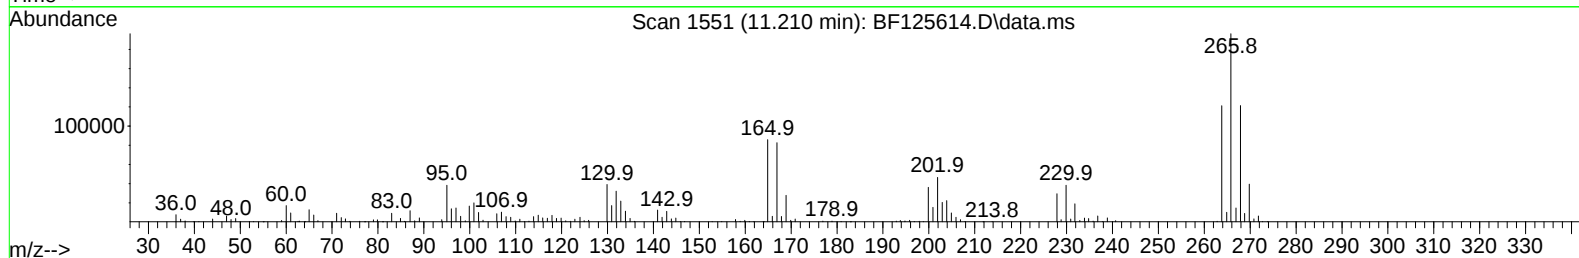


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
Data File : BF125614.D
Acq On : 24 Sep 2021 10:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 11:39:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 11:34:12 2021
Response via : Initial Calibration

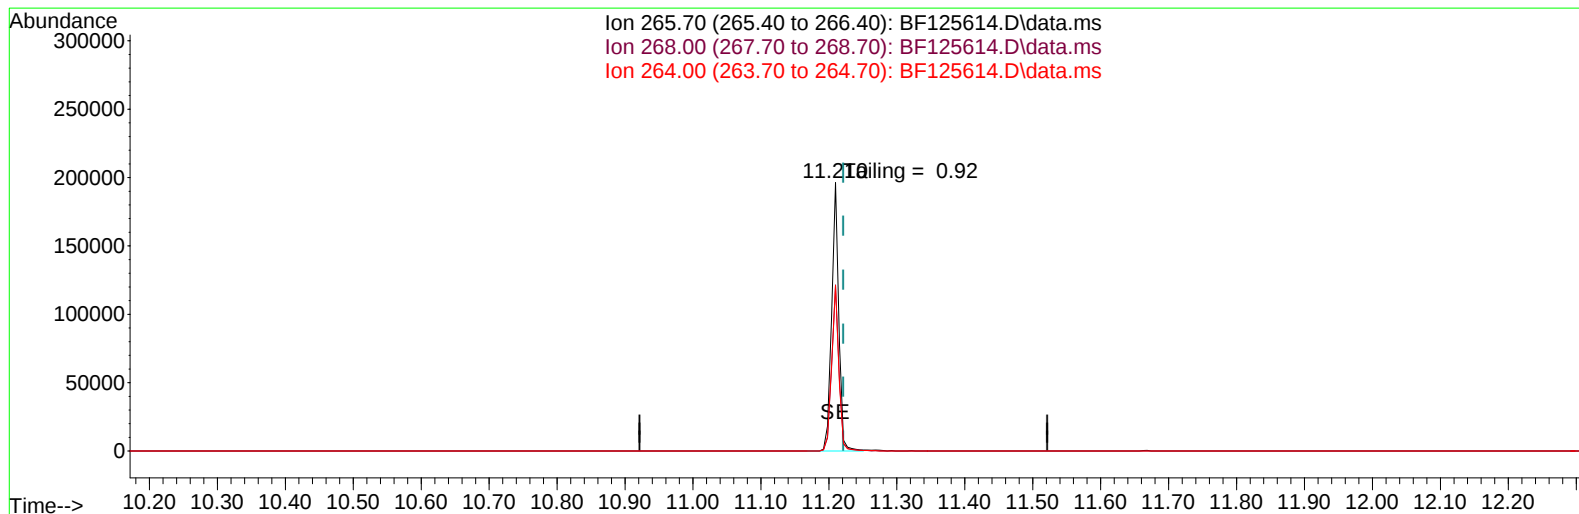

TIC: BF125614.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.012) 24038.11 ng

response 144383

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.89
264.00	69.90	61.75
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\  
Data File : BF125614.D  
Acq On    : 24 Sep 2021  10:33  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Sep 24 11:39:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 11:34:12 2021
Response via : Initial Calibration

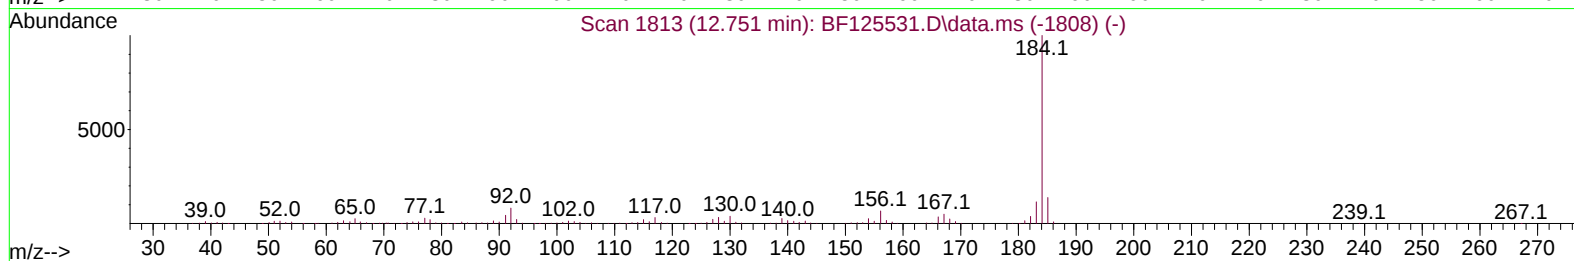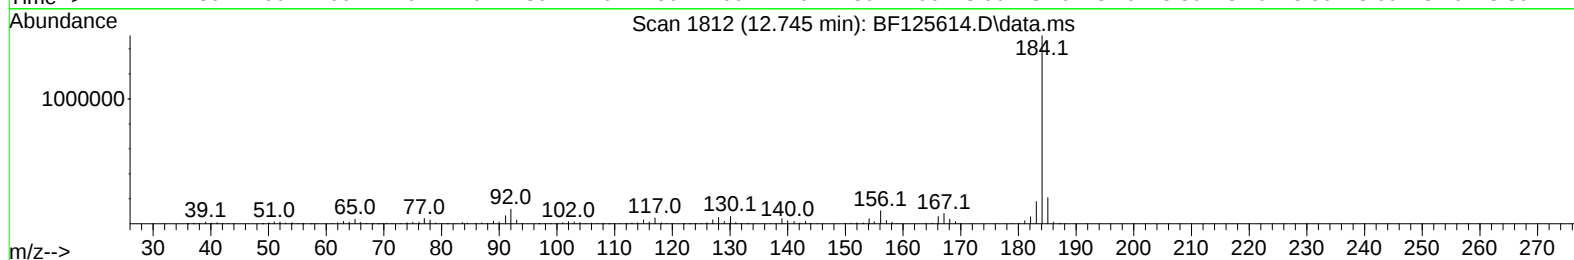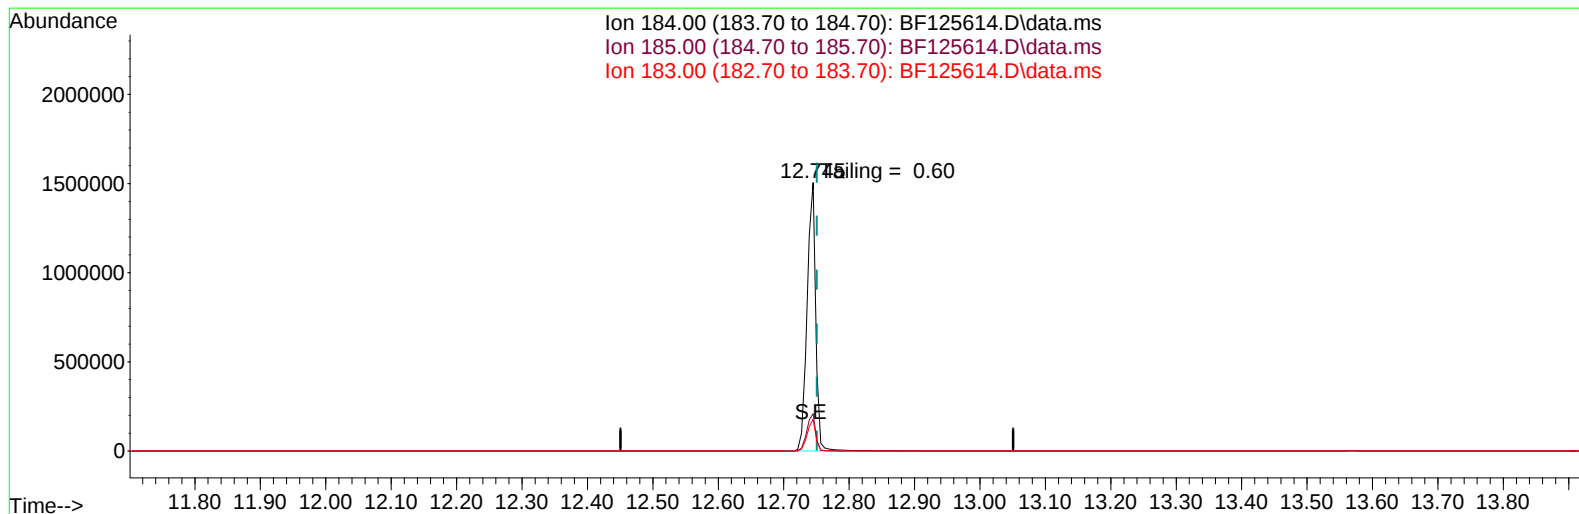

TIC: BF125614.D\data.ms

(77) Benzidine

12.745min (-0.006) 0.00 ng

```
response      1380448
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.92
183.00	10.10	11.82
0.00	0.00	0.00