

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
 Data File : BF125629.D
 Acq On : 24 Sep 2021 19:45
 Operator : JU/CG
 Sample : M3911-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-CB-02-(0.2)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125629.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.199	12	19	25	rVB	3695032	5092984	75.84%	13.682%
2	5.498	576	580	584	rBV	2627728	2583313	38.47%	6.940%
3	6.498	745	750	753	rBV	1961156	1628450	24.25%	4.375%
4	6.886	812	816	819	rBV	1406978	1098413	16.36%	2.951%
5	7.445	905	911	914	rBV	3405111	3511890	52.30%	9.435%
6	8.063	1013	1016	1029	rBV	137959	124548	1.85%	0.335%
7	8.169	1029	1034	1037	rBV	1682858	1540439	22.94%	4.138%
8	9.245	1211	1217	1220	rBV	7083486	6715159	100.00%	18.040%
9	9.922	1327	1332	1335	rBV	2198251	1771897	26.39%	4.760%
10	10.710	1461	1466	1469	rBV	4117933	3714454	55.31%	9.979%
11	11.404	1580	1584	1588	rBV	2087130	1715171	25.54%	4.608%
12	11.927	1665	1673	1678	rBV	105080	125607	1.87%	0.337%
13	12.992	1849	1854	1857	rBV	5757028	5452698	81.20%	14.649%
14	13.892	2001	2007	2008	rBV3	43676	68038	1.01%	0.183%
15	14.039	2028	2032	2036	rBV	1199450	987244	14.70%	2.652%
16	15.515	2277	2283	2287	rBV	918977	1093232	16.28%	2.937%




Sum of corrected areas: 37223537

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
Data File : BF125629.D
Acq On : 24 Sep 2021 19:45
Operator : JU/CG
Sample : M3911-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-CB-02-(0.2)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

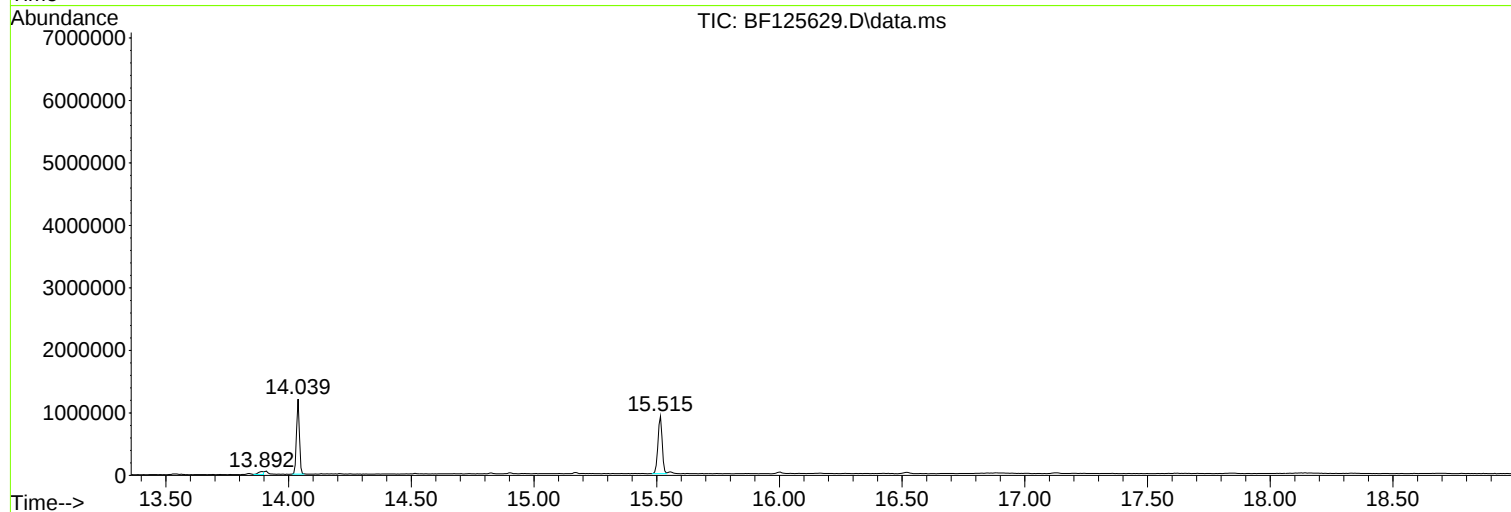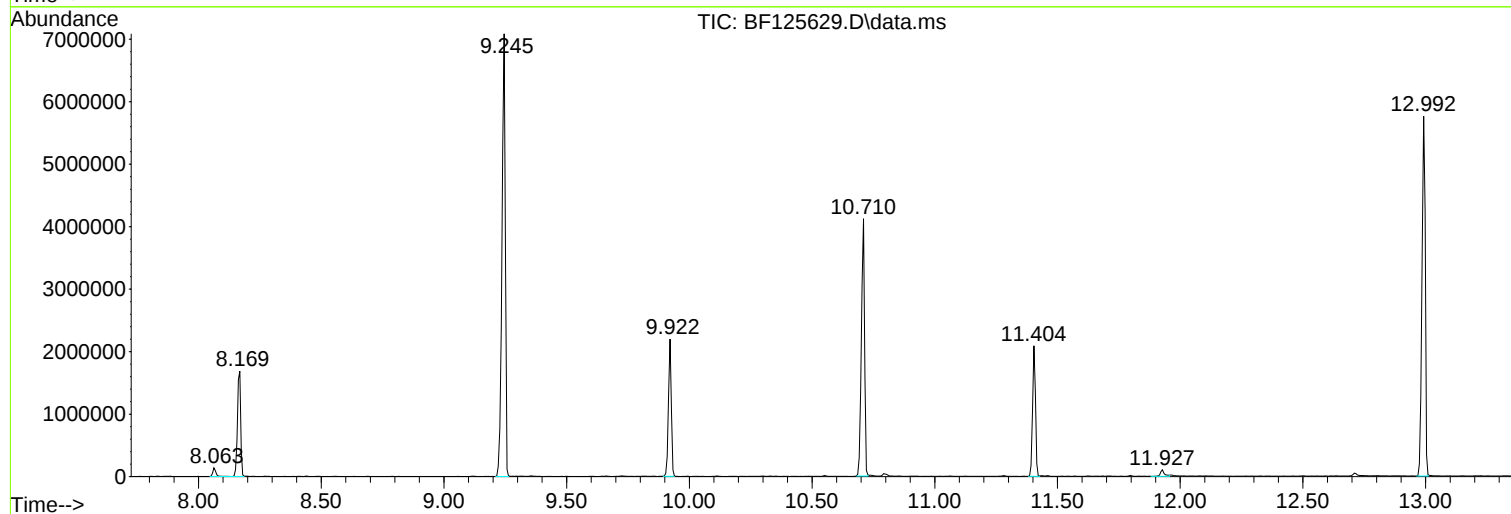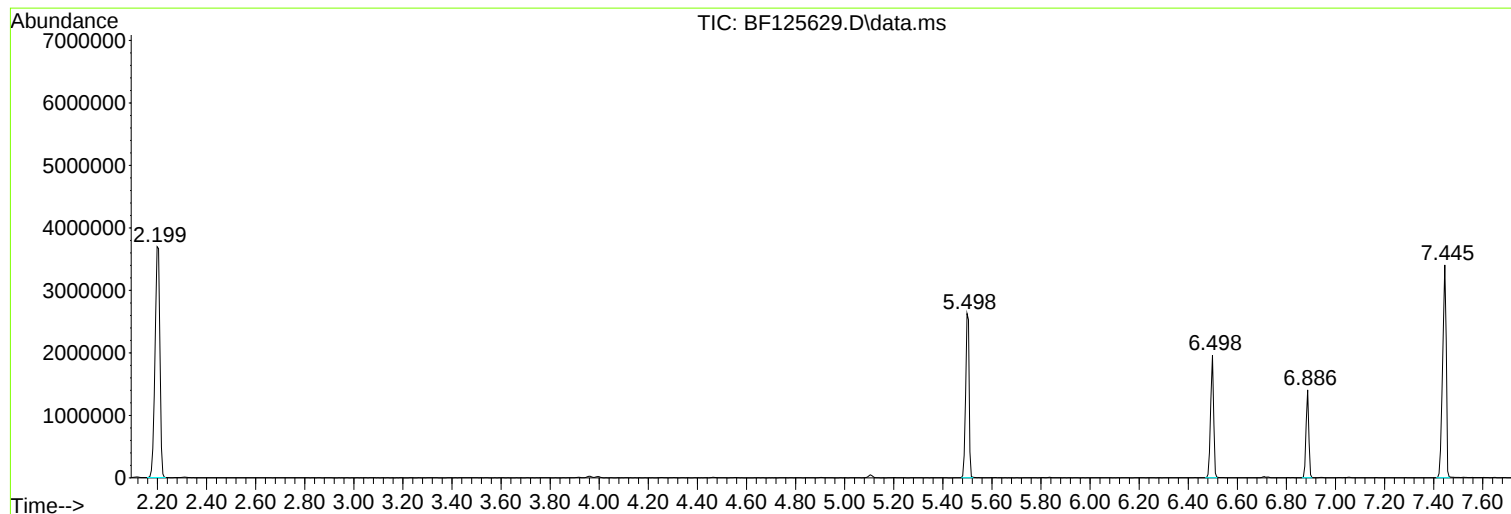

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
Data File : BF125629.D
Acq On : 24 Sep 2021 19:45
Operator : JU/CG
Sample : M3911-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-CB-02-(0.2)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.199	92.73 ng	5092980	1,4-Dichlorobenzene-d4	6.886

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17

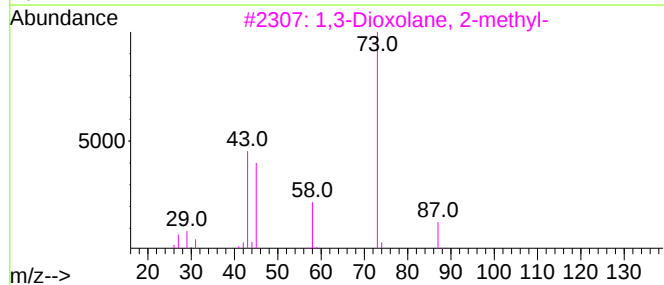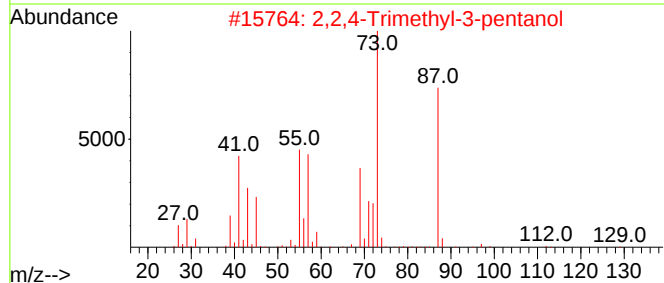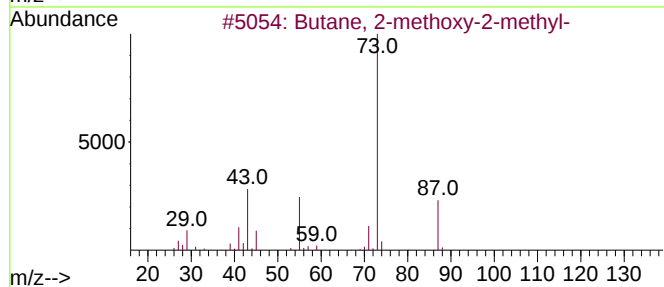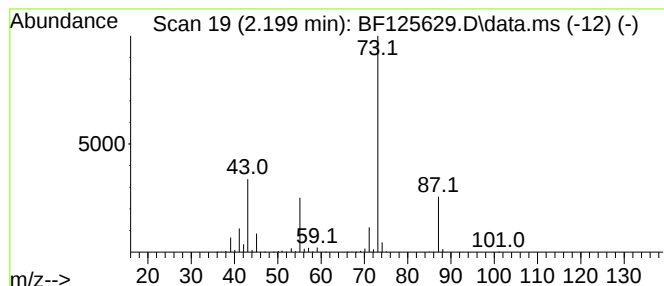

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
Data File : BF125629.D
Acq On : 24 Sep 2021 19:45
Operator : JU/CG
Sample : M3911-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-CB-02-(0.2)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.199	92.7	ng	5092980	1	6.886	1098410	20.0