


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
 Data File : BF125614.D
 Acq On : 24 Sep 2021 10:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 15:38:32 2021

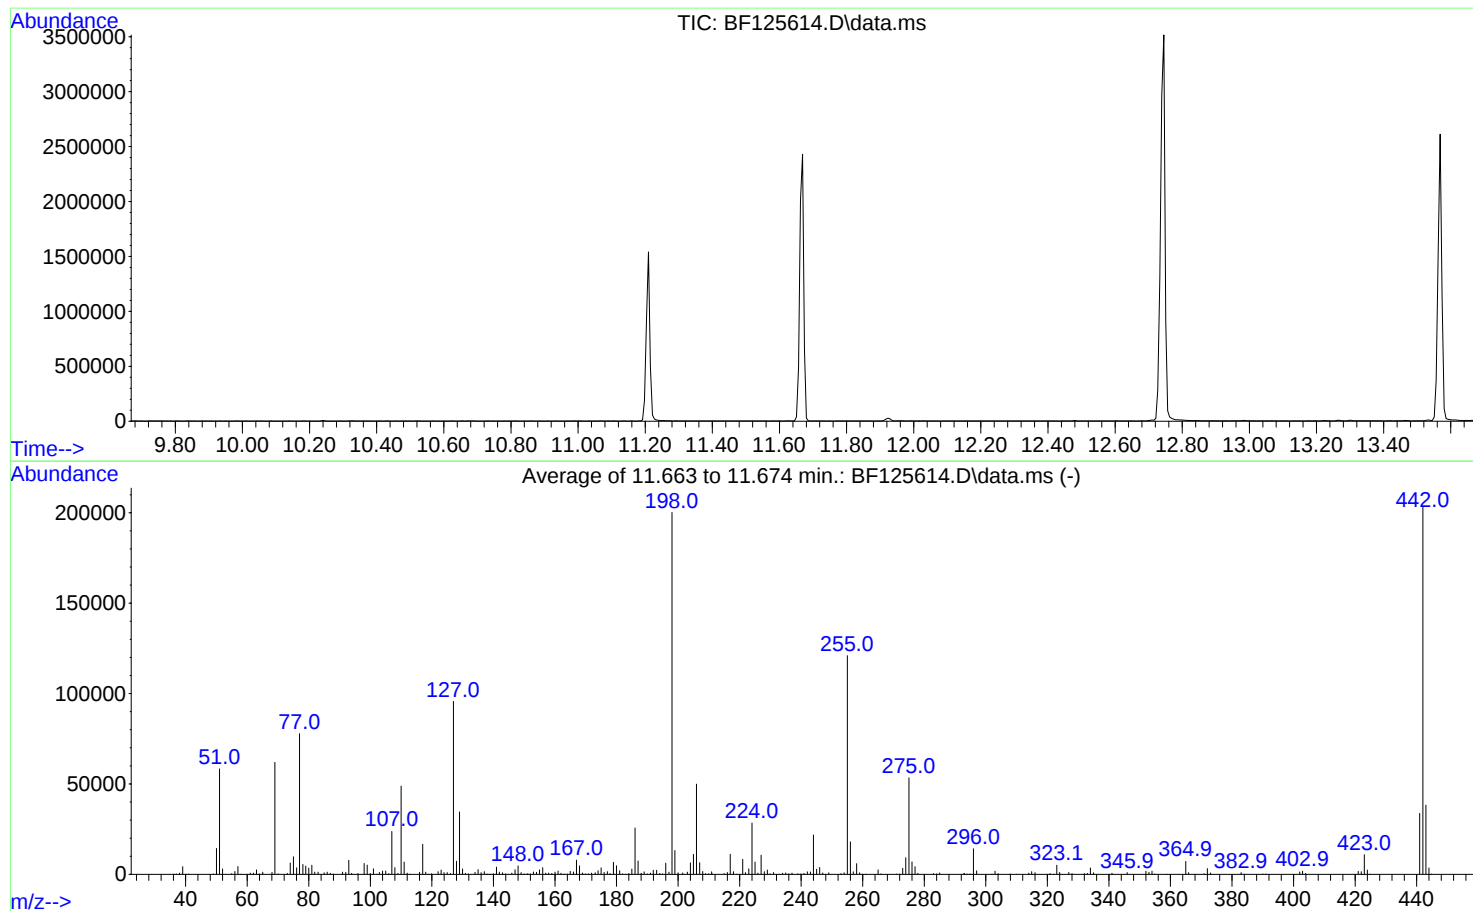




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	58335	PASS
68	69	0.00	2	1.7	1055	PASS
69	198	0.00	100	30.9	61948	PASS
70	69	0.00	2	0.5	316	PASS
127	198	10	80	47.8	95685	PASS
197	198	0.00	2	0.6	1228	PASS
198	198	100	100	100.0	200200	PASS
199	198	5	9	6.6	13180	PASS
275	198	10	60	26.7	53419	PASS
365	198	1	100	3.6	7217	PASS
441	198	0.01	100	16.9	33760	PASS
442	442	50	100	100.0	203499	PASS
443	442	15	24	18.8	38291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
Data File : BF125614.D
Acq On : 24 Sep 2021 10:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 24 11:39:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 11:34:12 2021
Response via : Initial Calibration

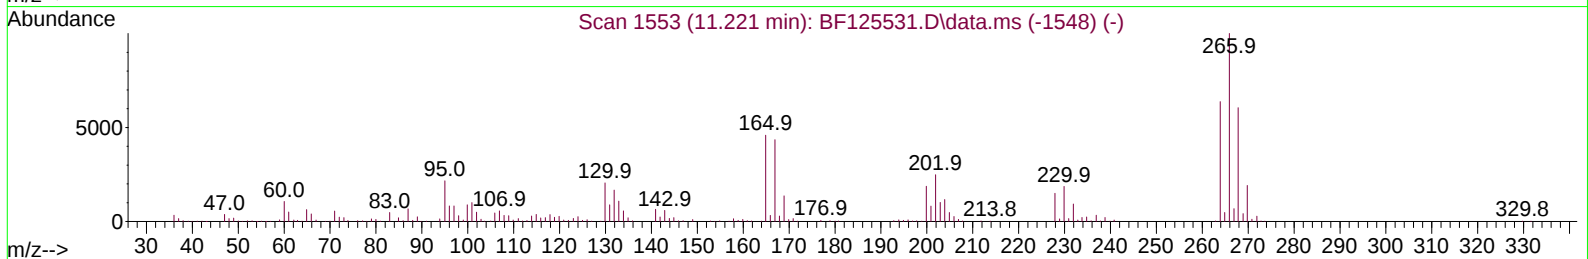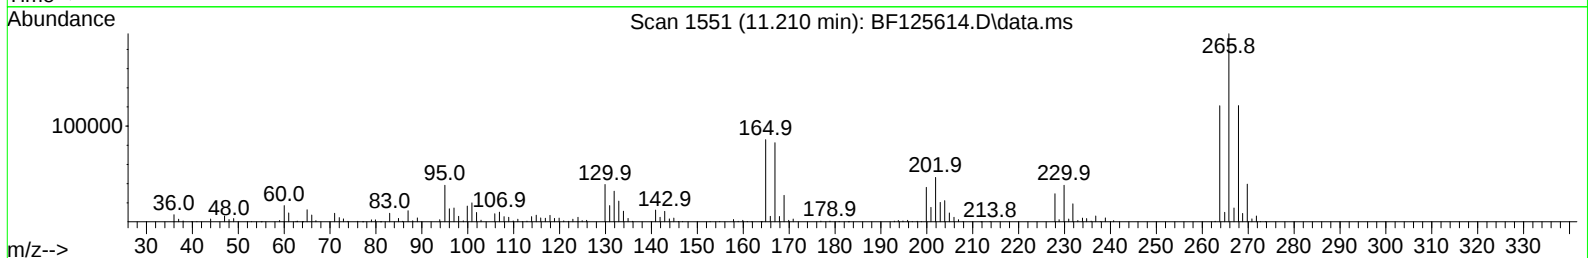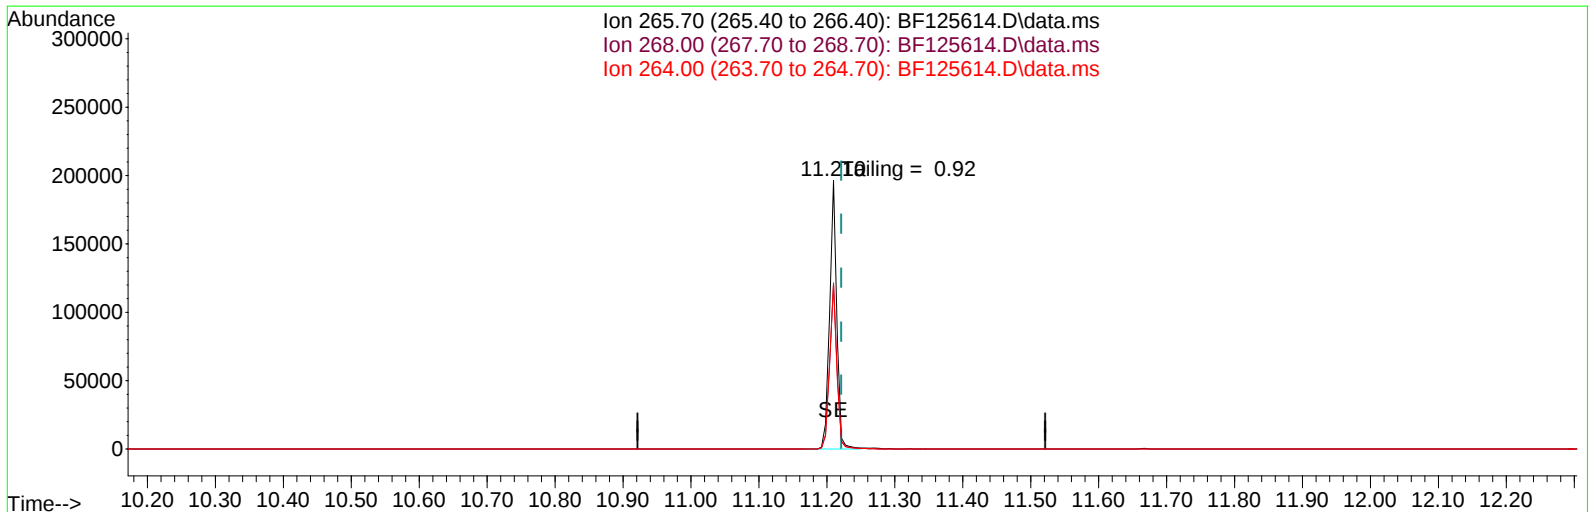

TIC: BF125614.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.012) 24038.11 ng




response 144383

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.89
264.00	69.90	61.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
 Data File : BF125614.D
 Acq On : 24 Sep 2021 10:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 24 11:39:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 11:34:12 2021
 Response via : Initial Calibration

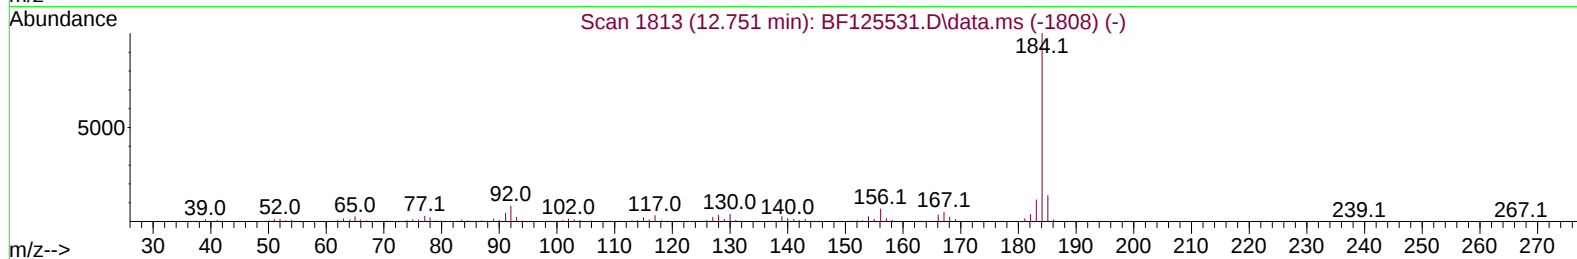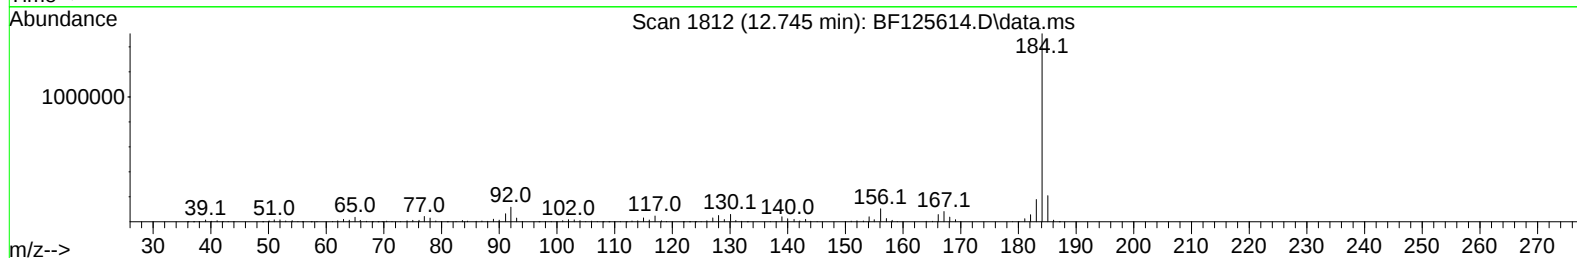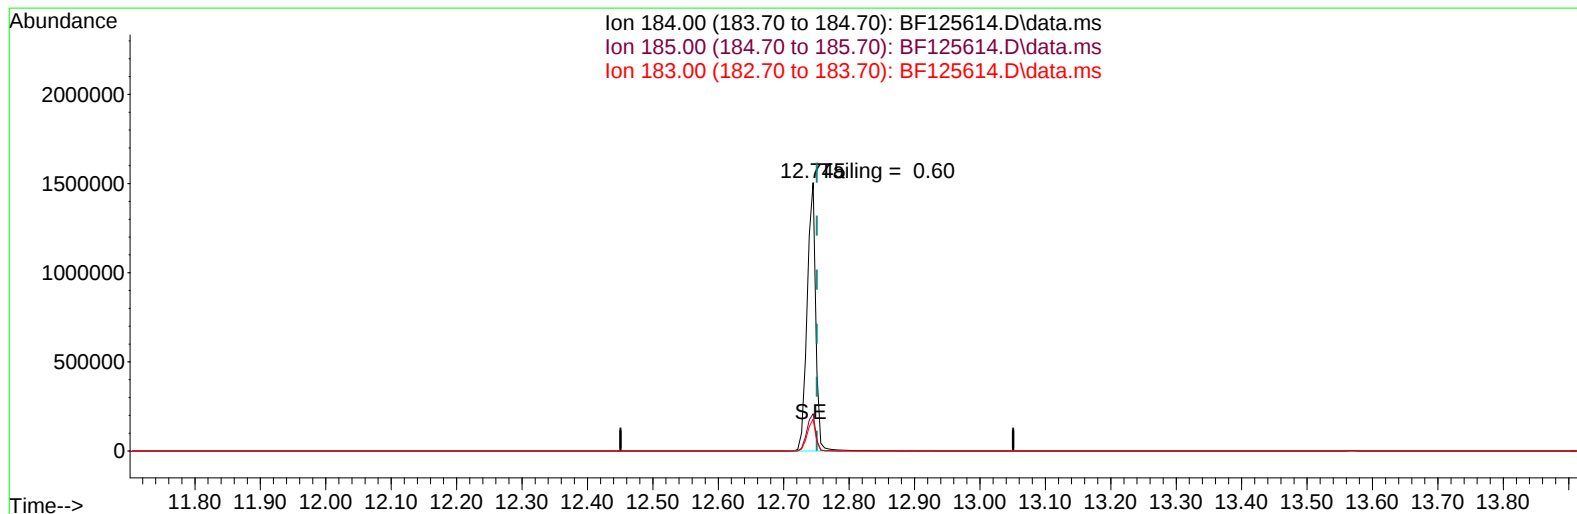

TIC: BF125614.D\data.ms

(77) Benzidine

12.745min (-0.006) 0.00 ng

response 1380448

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.92
183.00	10.10	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/24/2021	BNA_F	<u>BF125614.D</u>
Compound Name	Response	Retention Time
DDT	348699	13.56
DDD	1545	13.26
DDE	0	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1545	350244	0.44