
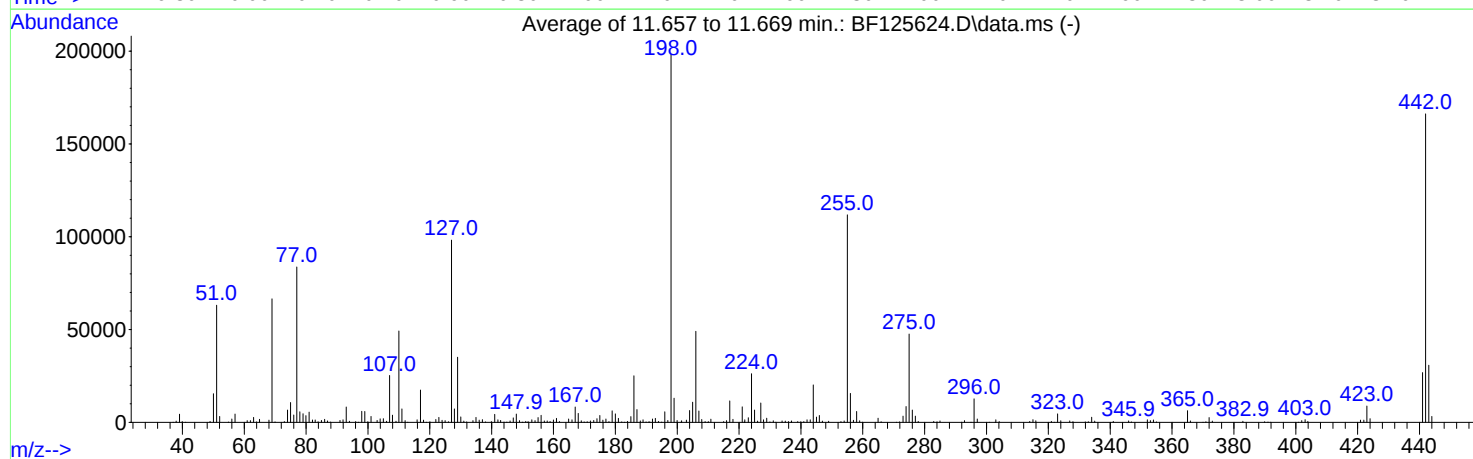


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
 Data File : BF125624.D
 Acq On : 24 Sep 2021 16:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 15:38:32 2021

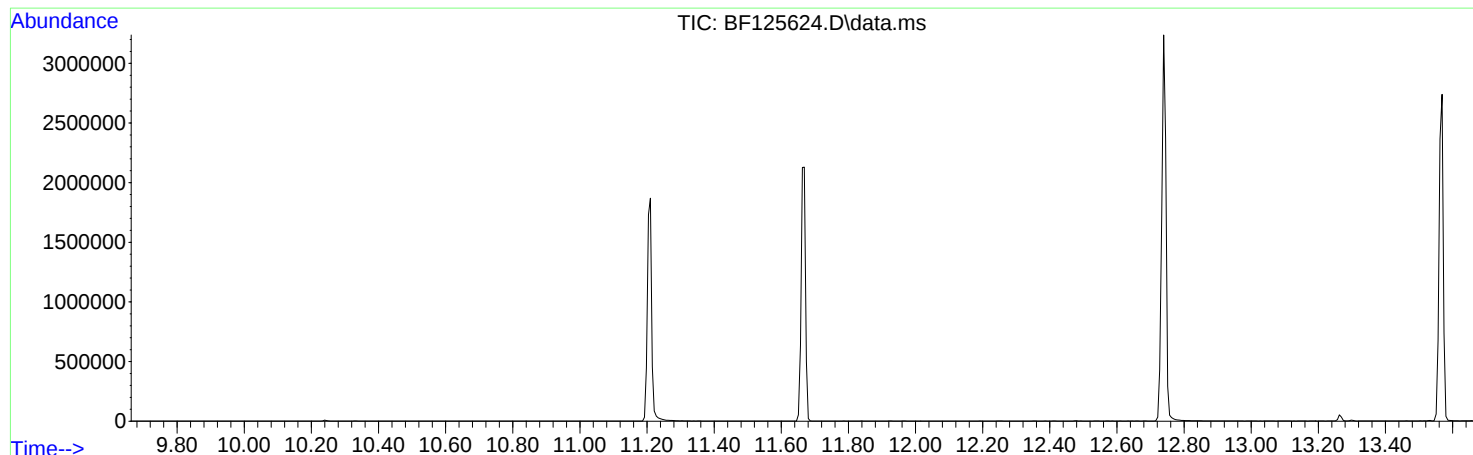


AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	63125	PASS
68	69	0.00	2	1.8	1183	PASS
69	198	0.00	100	33.6	66544	PASS
70	69	0.00	2	0.4	289	PASS
127	198	10	80	49.6	98224	PASS
197	198	0.00	2	0.5	1085	PASS
198	198	100	100	100.0	198173	PASS
199	198	5	9	6.6	12985	PASS
275	198	10	60	24.0	47631	PASS
365	198	1	100	3.2	6261	PASS
441	198	0.01	100	13.5	26796	PASS
442	442	50	100	100.0	166189	PASS
443	442	15	24	18.5	30818	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
 Data File : BF125624.D
 Acq On : 24 Sep 2021 16:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 24 17:45:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

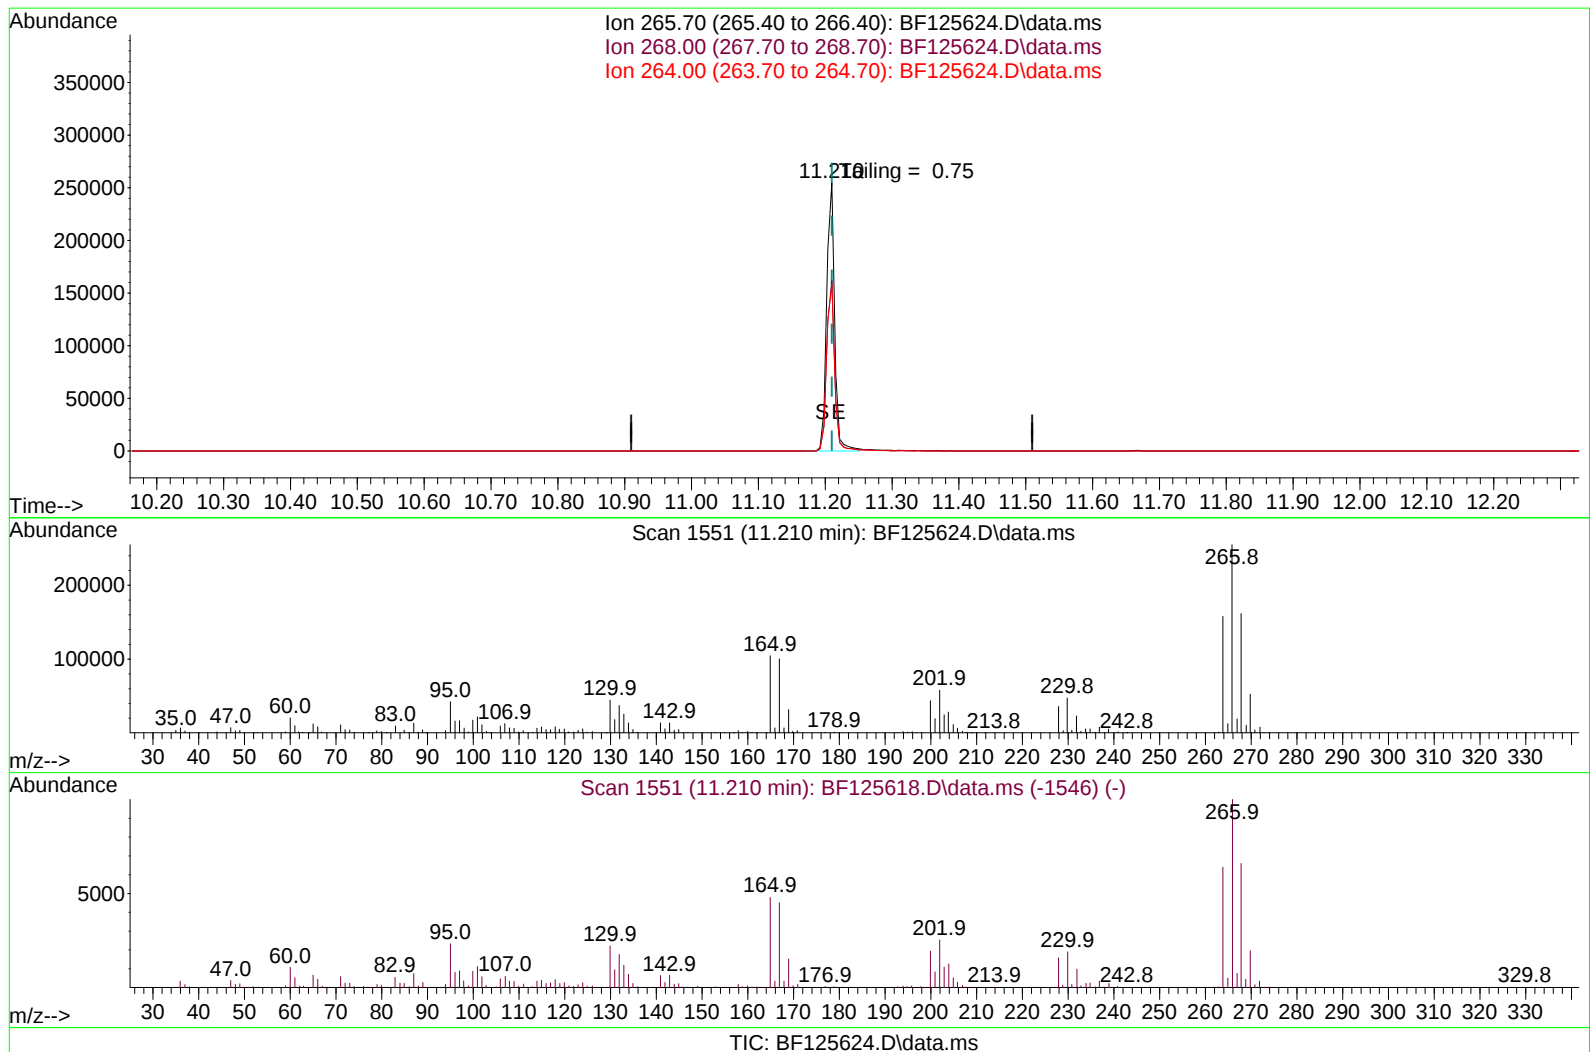

TIC: BF125624.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 38544.51 ng




response 212277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.47
264.00	69.90	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092421\
 Data File : BF125624.D
 Acq On : 24 Sep 2021 16:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 24 17:45:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

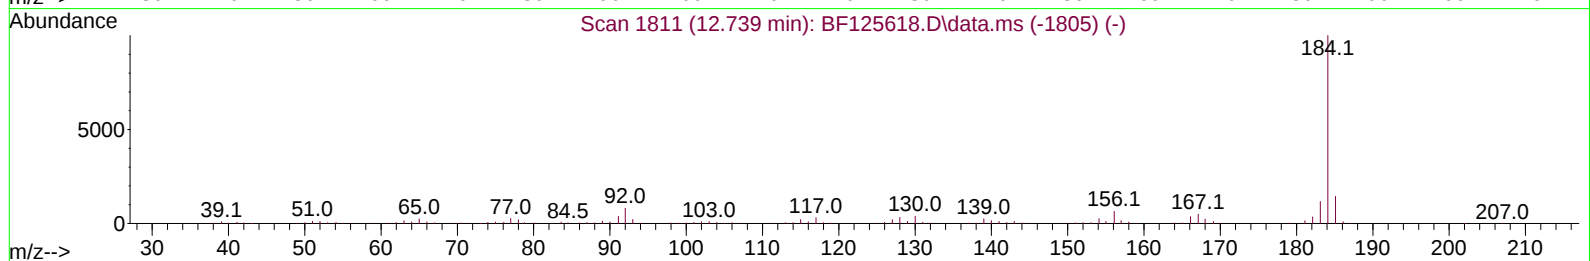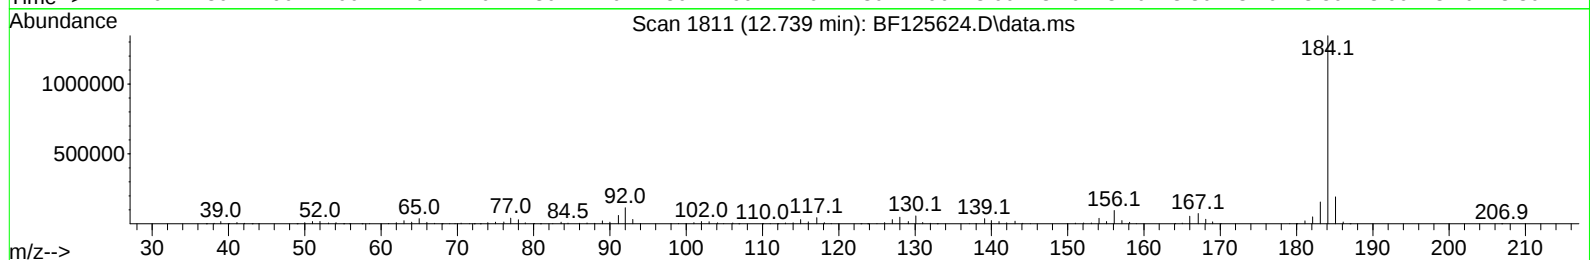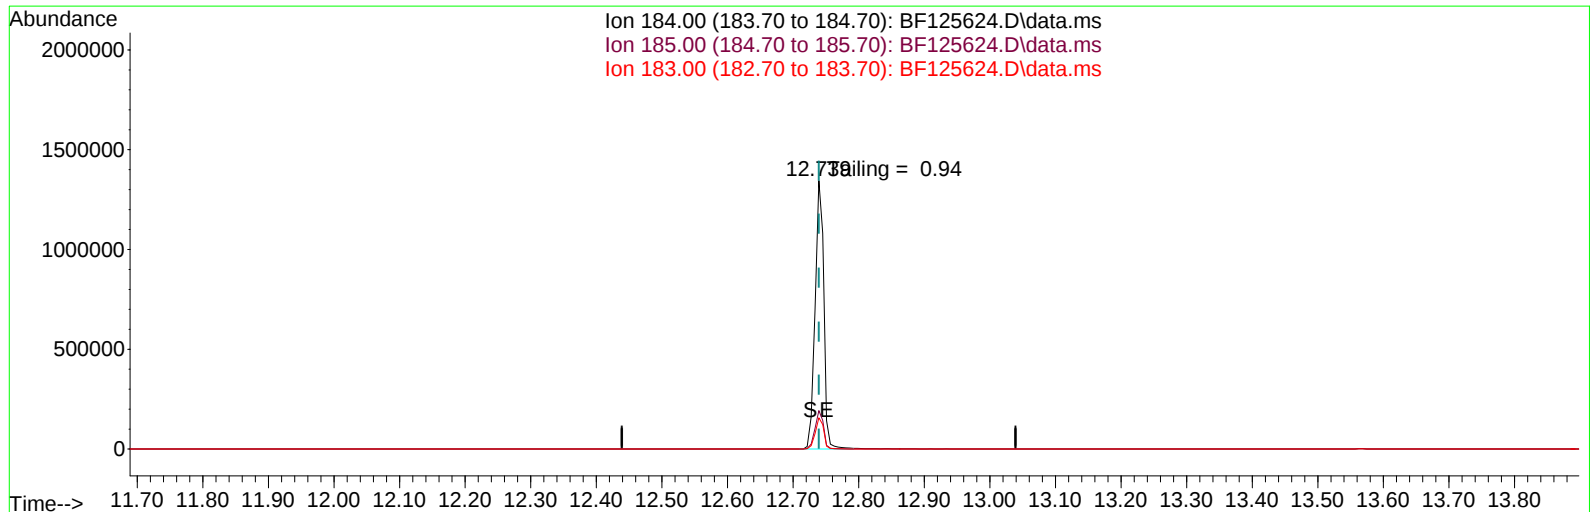

TIC: BF125624.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 0.00 ng

response 1249427

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.32
183.00	10.10	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/24/2021	BNA_F	<u>BF125624.D</u>
Compound Name	Response	Retention Time
DDT	468871	13.56
DDD	8628	13.26
DDE	0	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8628	477499	1.81

Instrument :
BNA_F
ClientSampleId :
DFTPP