

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092515\
 Data File : BF081801.D
 Acq On : 25 Sep 2015 14:11
 Operator : UM/IZ
 Sample : G3708-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MGP201-36-38

Quant Time: Sep 26 00:01:02 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 25 06:02:49 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	141784	20.00	ng	0.00
21) Naphthalene-d8	8.23	136	522400	20.00	ng	-0.01
38) Acenaphthene-d10	9.99	164	291174	20.00	ng	-0.01
63) Phenanthrene-d10	11.48	188	548253	20.00	ng	0.00
75) Chrysene-d12	14.12	240	513541	20.00	ng	0.00
86) Perylene-d12	15.58	264	376884	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.55	112	1054024	125.76	ng	0.01
7) Phenol-d6	6.57	99	1311499	123.72	ng	0.00
23) Nitrobenzene-d5	7.51	82	704307	88.95	ng	-0.01
41) 2,4,6-Tribromophenol	10.78	330	294443	116.48	ng	-0.01
44) 2-Fluorobiphenyl	9.31	172	1421169	80.12	ng	0.00
78) Terphenyl-d14	13.06	244	1380585	61.41	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.70	163	483059	21.80	ng	Qvalue # 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092515\
Data File : BF081801.D
Acq On : 25 Sep 2015 14:11
Operator : UM/IZ
Sample : G3708-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MGP201-36-38

Quant Time: Sep 26 00:01:02 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 06:02:49 2015
Response via : Initial Calibration

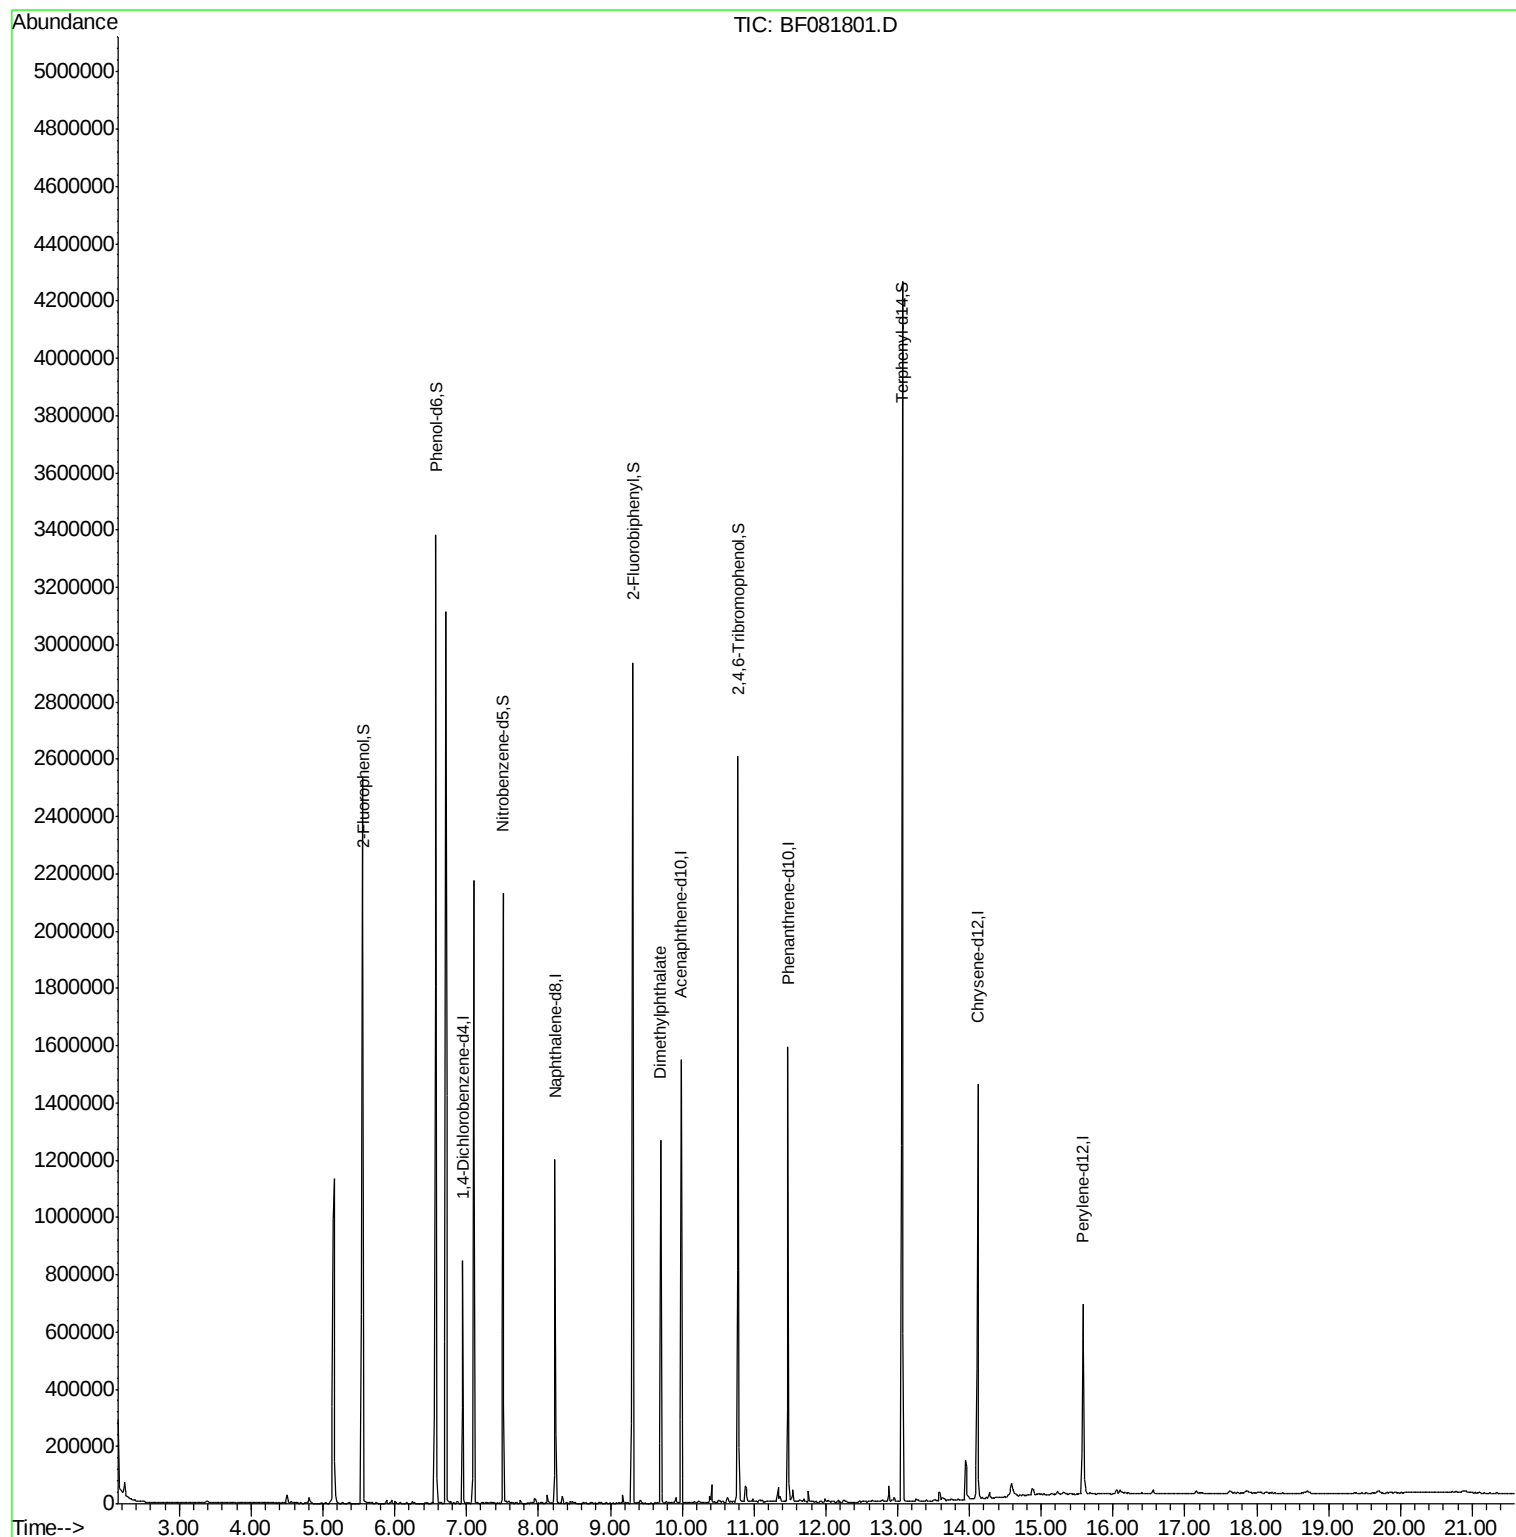

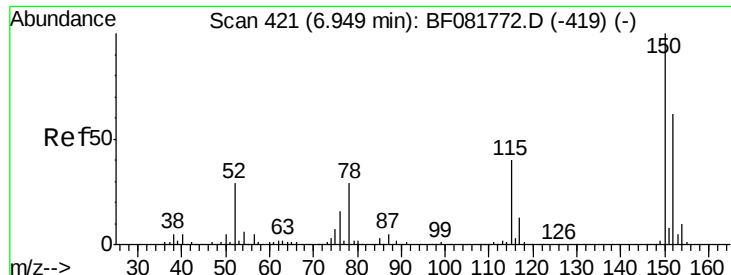

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.95 min Scan# 421

Delta R.T. 0.00 min

Lab File: BF081801.D

Acq: 25 Sep 2015 14:11

Instrument :

BNA_F

ClientSampleId :

MGP201-36-38


Tgt Ion:152 Resp: 141784

Ion Ratio Lower Upper

152 100

150 154.5 124.7 187.1




115 52.3 39.0 58.4

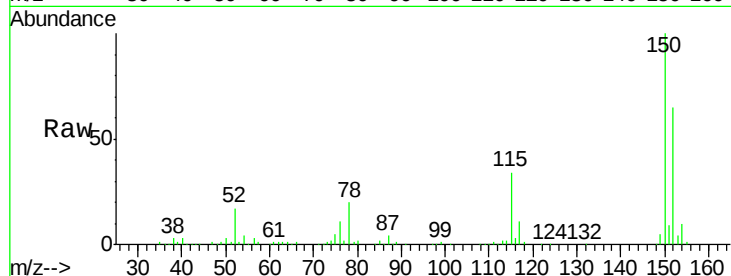

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

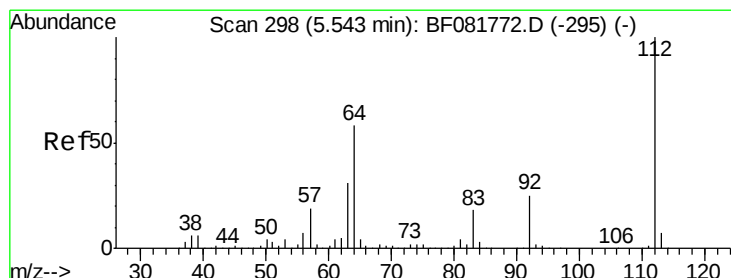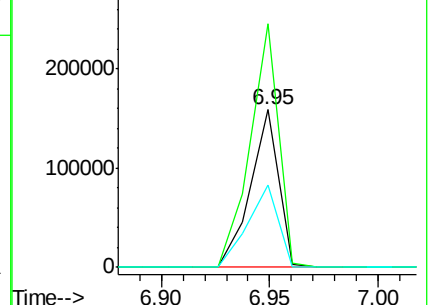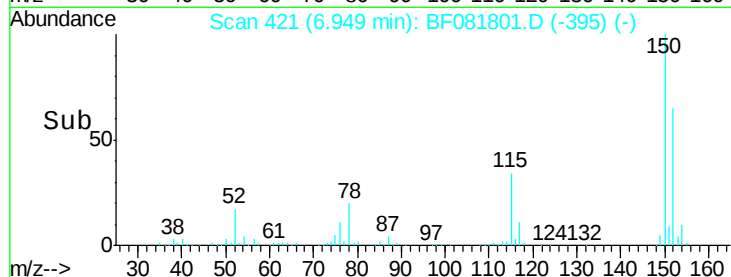

#5

2-Fluorophenol

Concen: 125.76 ng

RT: 5.55 min Scan# 299

Delta R.T. 0.01 min

Lab File: BF081801.D

Acq: 25 Sep 2015 14:11


Tgt Ion:112 Resp: 1054024

Ion Ratio Lower Upper

112 100

64 48.5 39.7 59.5



63 24.8 17.4 26.0

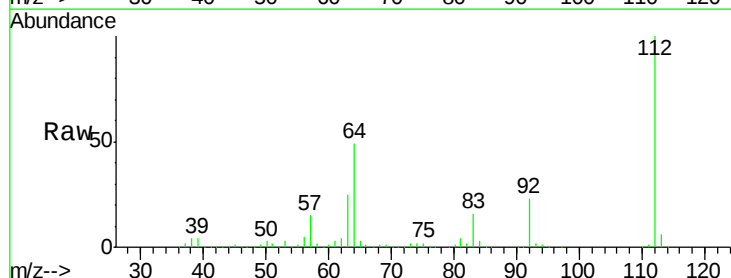


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

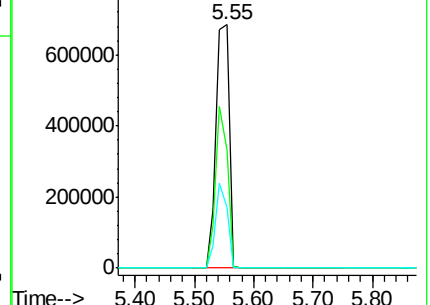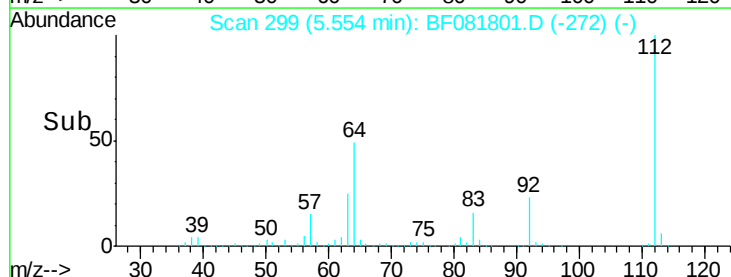

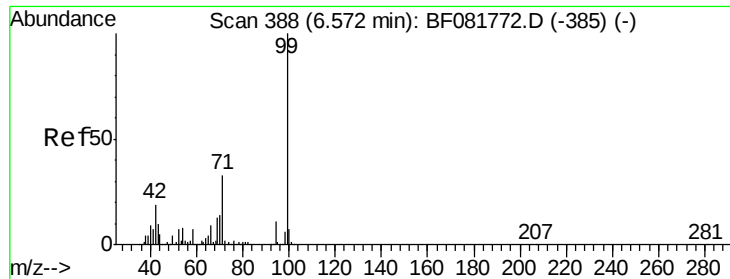

#7

Phenol-d6

Concen: 123.72 ng

RT: 6.57 min Scan# 388

Delta R.T. 0.00 min

Lab File: BF081801.D

Acq: 25 Sep 2015 14:11

Instrument :

BNA_F

ClientSampleId :

MGP201-36-38





Tgt Ion: 99 Resp: 1311499

Ion Ratio Lower Upper

99 100

42 19.7 13.7 20.5

71 35.1 14.2 21.2#

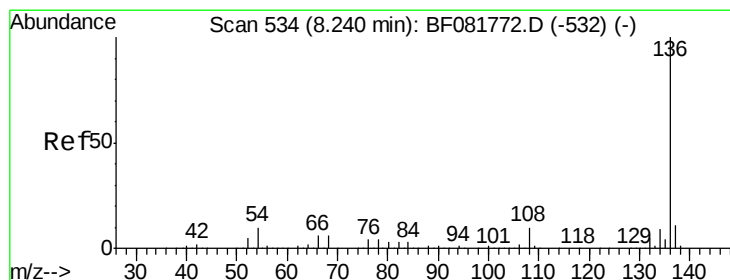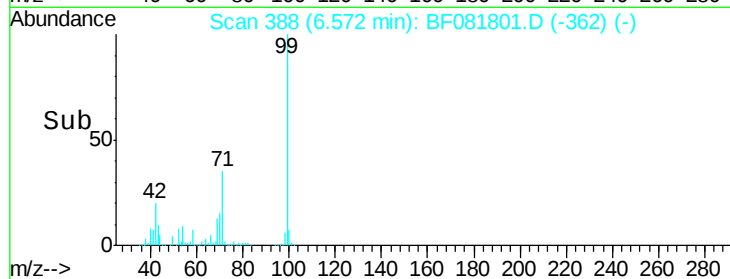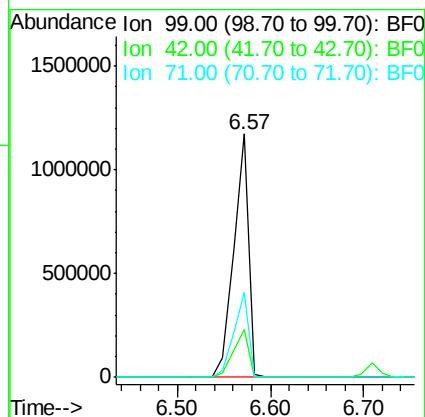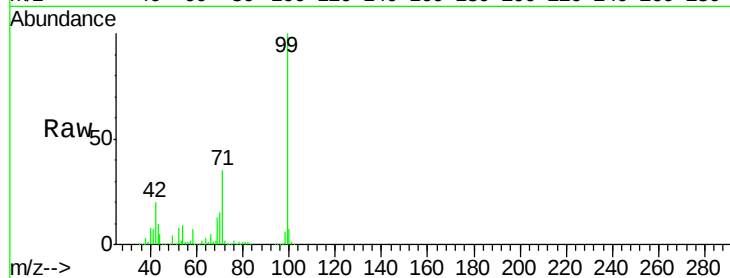

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.23 min Scan# 533

Delta R.T. -0.01 min

Lab File: BF081801.D

Acq: 25 Sep 2015 14:11

Tgt Ion: 136 Resp: 522400




Ion Ratio Lower Upper


136 100

137 11.3 9.0 13.6

54 9.7 8.2 12.2

68 6.5 5.8 8.6

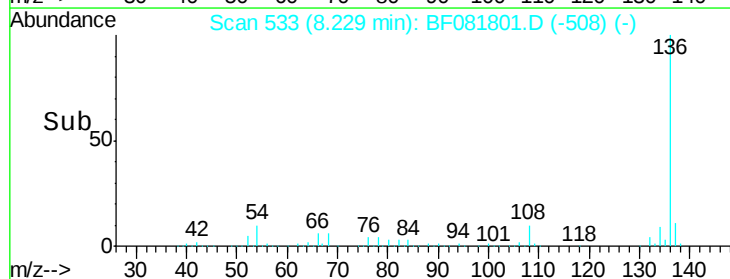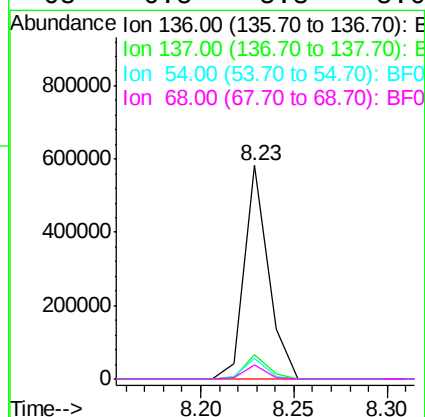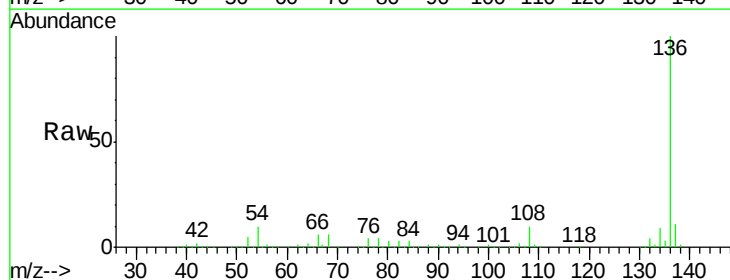

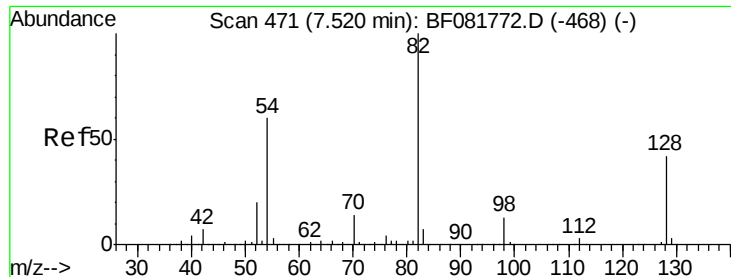

#23

Nitrobenzene-d5

Concen: 88.95 ng

RT: 7.51 min Scan# 470

Delta R.T. -0.01 min

Lab File: BF081801.D

Acq: 25 Sep 2015 14:11

Instrument :

BNA_F

ClientSampleId :

MGP201-36-38


Tgt Ion: 82 Resp: 704307

Ion Ratio Lower Upper

82 100

128 41.0 51.0 76.6#




54 58.6 47.5 71.3

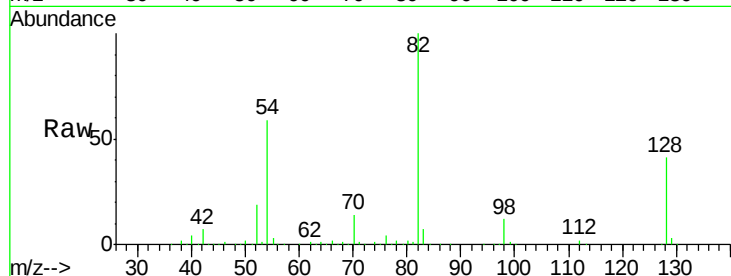

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

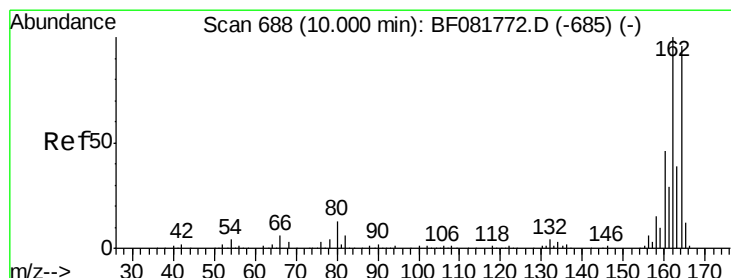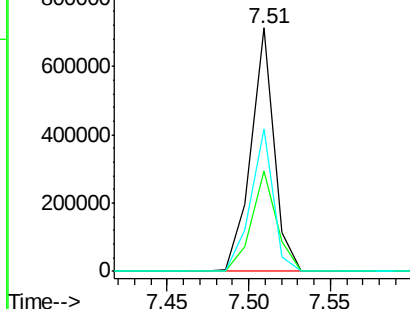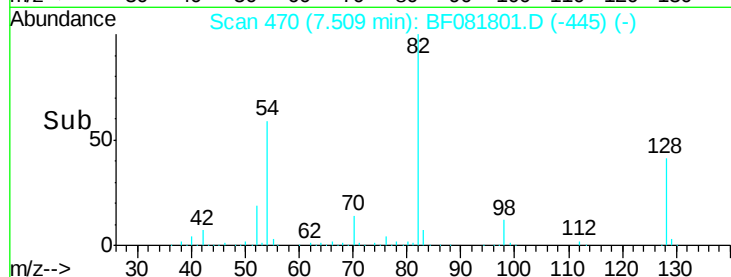

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.99 min Scan# 687

Delta R.T. -0.01 min

Lab File: BF081801.D

Acq: 25 Sep 2015 14:11


Tgt Ion: 164 Resp: 291174

Ion Ratio Lower Upper

164 100

162 103.5 75.2 112.8



160 45.4 31.5 47.3

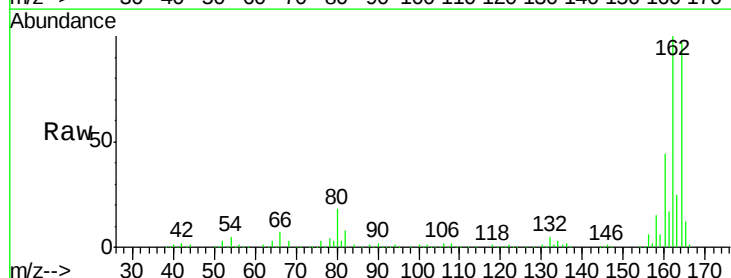


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

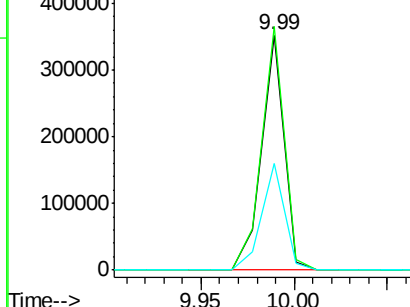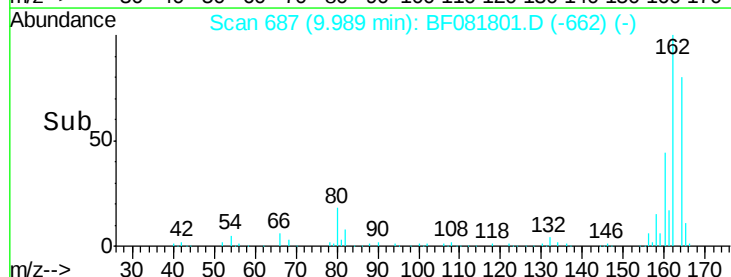


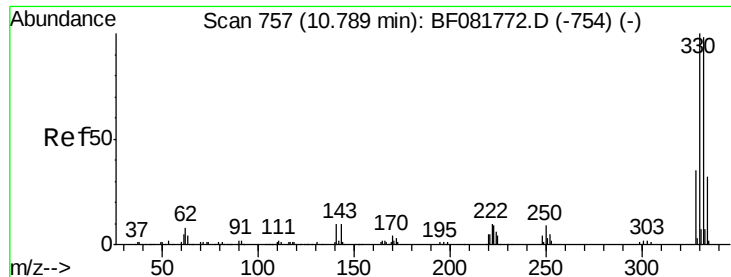




#41
 2,4,6-Tribromophenol
 Concen: 116.48 ng
 RT: 10.78 min Scan# 756
 Delta R.T. -0.01 min
 Lab File: BF081801.D
 Acq: 25 Sep 2015 14:11

Instrument :
 BNA_F
 ClientSampleId :
 MGP201-36-38

Tgt Ion:330 Resp: 294443
 Ion Ratio Lower Upper
 330 100
 332 94.5 76.6 114.8
 141 38.9 29.7 44.5

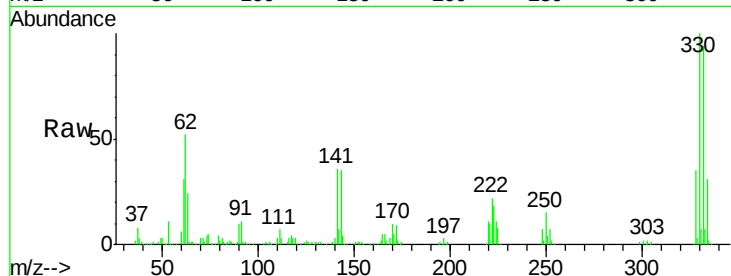


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

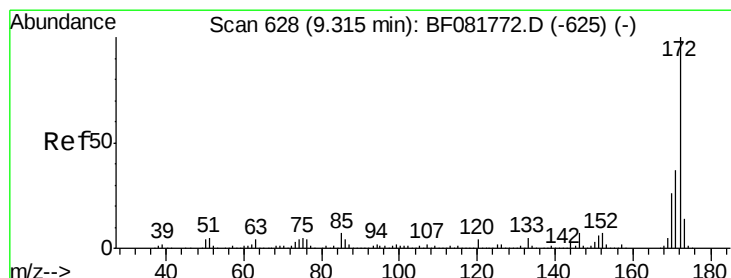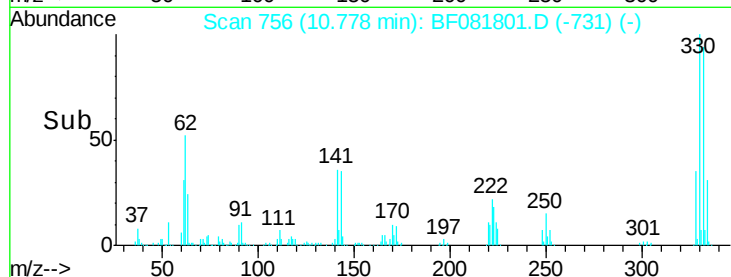
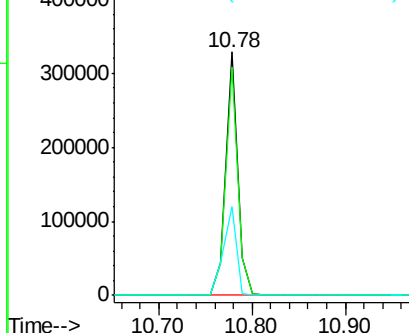



#44
 2-Fluorobiphenyl
 Concen: 80.12 ng
 RT: 9.31 min Scan# 628
 Delta R.T. 0.00 min
 Lab File: BF081801.D
 Acq: 25 Sep 2015 14:11

Tgt Ion:172 Resp: 1421169
 Ion Ratio Lower Upper
 172 100
 171 36.2 26.1 39.1
 170 24.9 17.4 26.2

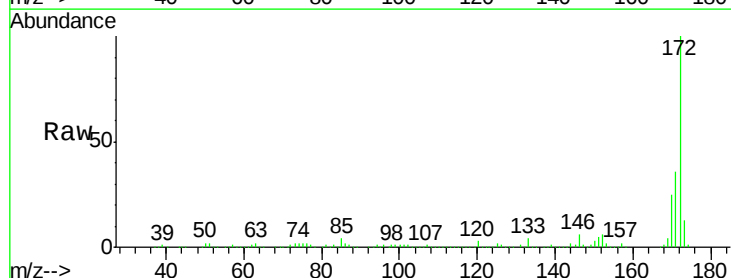

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

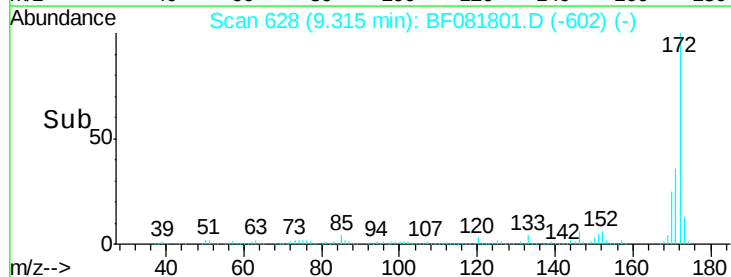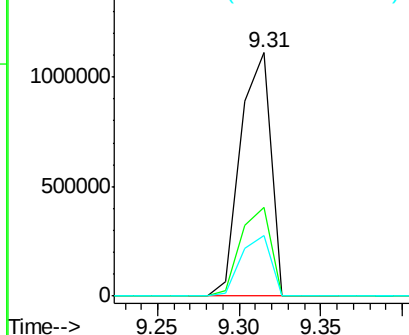


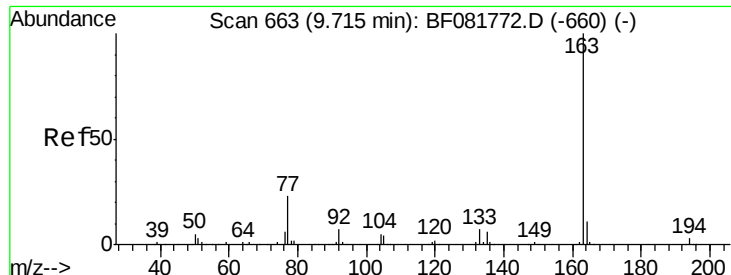




#49
Dimethylphthalate
Concen: 21.80 ng
RT: 9.70 min Scan# 662
Delta R.T. -0.01 min
Lab File: BF081801.D
Acq: 25 Sep 2015 14:11

Instrument :
BNA_F
ClientSampleId :
MGP201-36-38

Tgt Ion:163 Resp: 483059
Ion Ratio Lower Upper
163 100
194 3.6 4.4 6.6#
164 10.2 8.3 12.5

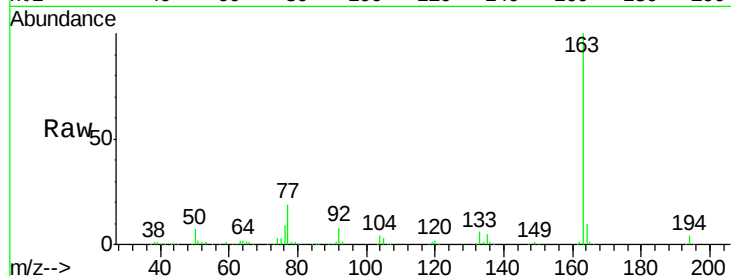


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

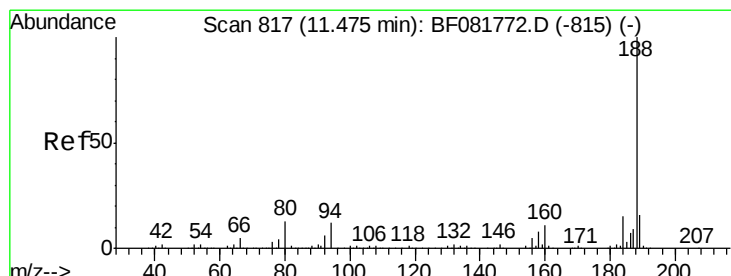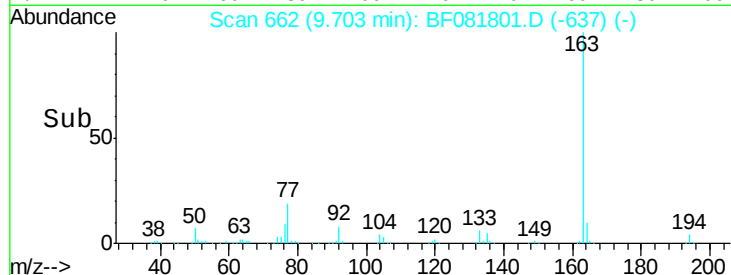
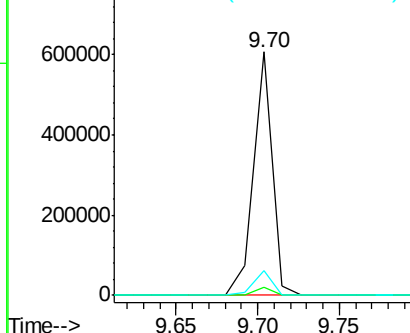



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.48 min Scan# 817
Delta R.T. 0.00 min
Lab File: BF081801.D
Acq: 25 Sep 2015 14:11

Tgt Ion:188 Resp: 548253
Ion Ratio Lower Upper
188 100
94 8.3 11.1 16.7#
80 8.5 11.0 16.4#

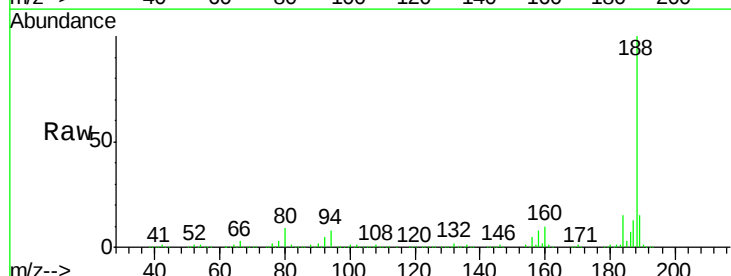

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

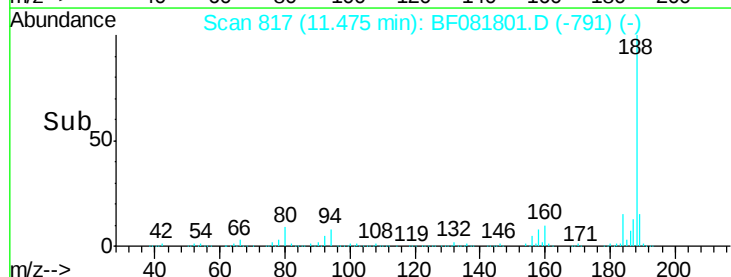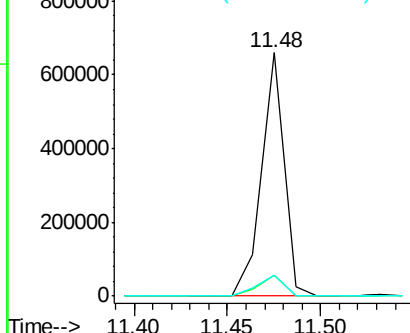

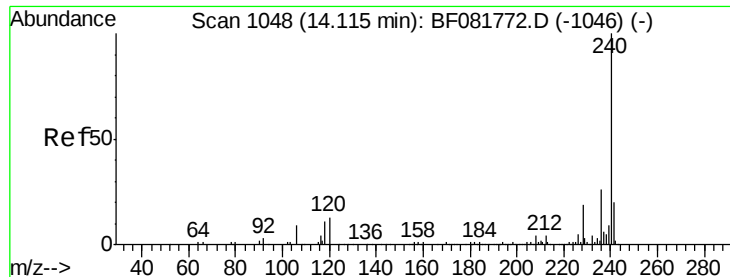

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.12 min Scan# 1048

Delta R.T. 0.00 min

Lab File: BF081801.D

Acq: 25 Sep 2015 14:11

Instrument :

BNA_F

ClientSampleId :

MGP201-36-38


Tgt Ion:240 Resp: 513541

Ion Ratio Lower Upper

240 100

120 8.7 16.2 24.2#




236 26.9 18.4 27.6

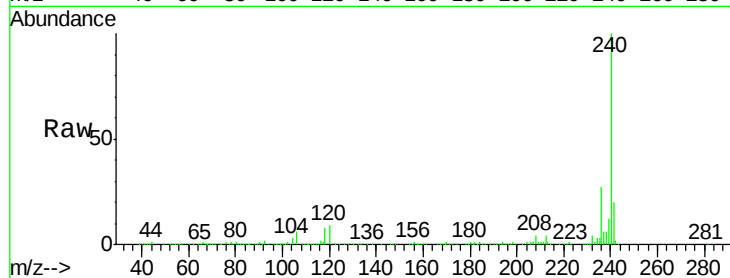

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

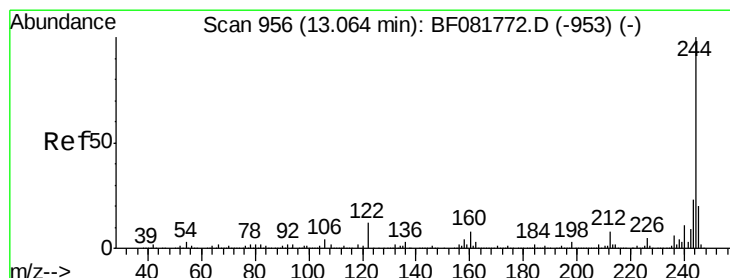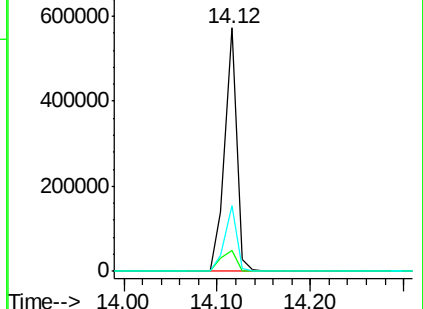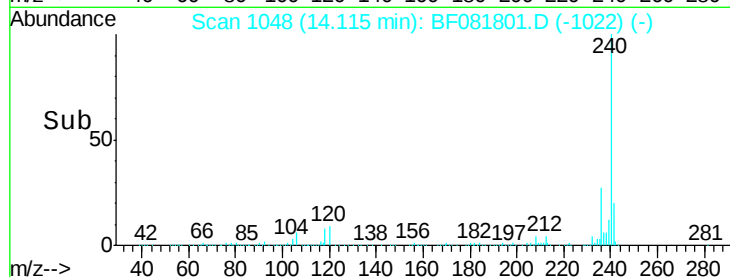

#78

Terphenyl-d14

Concen: 61.41 ng

RT: 13.06 min Scan# 956

Delta R.T. 0.00 min

Lab File: BF081801.D

Acq: 25 Sep 2015 14:11


Tgt Ion:244 Resp: 1380585

Ion Ratio Lower Upper

244 100

212 8.1 4.3 6.5#



122 11.6 17.4 26.2#

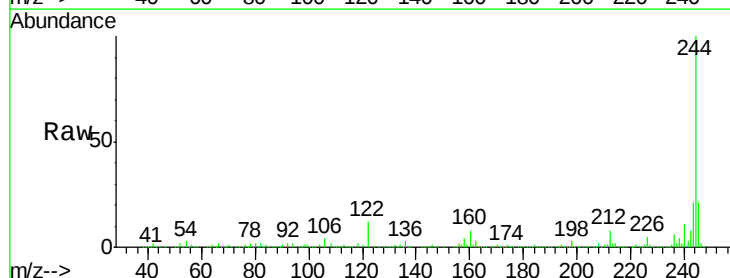


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

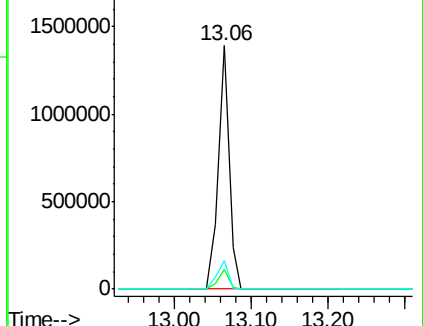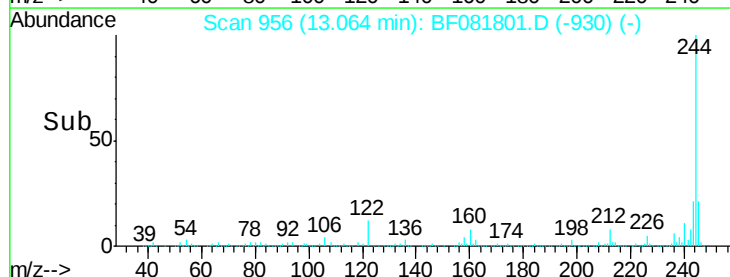

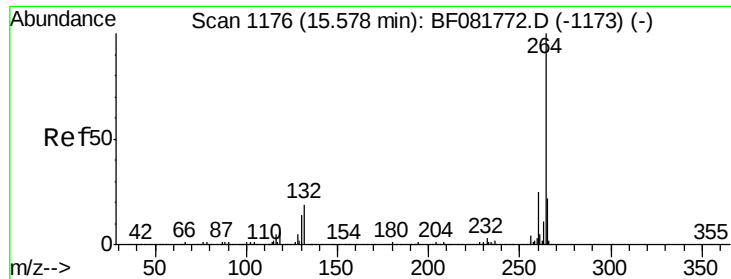

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.58 min Scan# 1176
Delta R.T. 0.00 min
Lab File: BF081801.D
Acq: 25 Sep 2015 14:11

Instrument :
BNA_F
ClientSampleId :
MGP201-36-38

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.7	16.7	25.1
265	21.6	17.2	25.8

