

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092515\
 Data File : BF081813.D
 Acq On : 25 Sep 2015 20:26
 Operator : UM/IZ
 Sample : G3676-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TEC-6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.131	260	262	265	rVB	238505	236022	5.11%	0.619%
2	5.543	295	298	300	rBV	1138177	1236604	26.76%	3.242%
3	6.560	385	387	389	rBV	1012649	828272	17.92%	2.171%
4	6.709	398	400	402	rBV	2322857	2019995	43.71%	5.296%
5	6.869	411	414	416	rBV	123355	113259	2.45%	0.297%
6	6.949	419	421	422	rBV	1067984	966256	20.91%	2.533%
7	6.983	422	424	425	rVB2	56461	67709	1.46%	0.178%
8	7.109	432	435	437	rBV	2733734	3267393	70.69%	8.566%
9	7.269	447	449	452	rBV2	36450	48348	1.05%	0.127%
10	7.349	452	456	461	rBV2	62103	90869	1.97%	0.238%
11	7.509	467	470	472	rBV	1751847	2628385	56.87%	6.891%
12	7.554	472	474	476	rVB2	40017	63107	1.37%	0.165%
13	7.932	506	507	510	rBV2	55558	57428	1.24%	0.151%
14	7.977	510	511	513	rVB	79171	59082	1.28%	0.155%
15	8.137	523	525	527	rBV2	40141	60397	1.31%	0.158%
16	8.229	531	533	536	rVV	1027439	1159101	25.08%	3.039%
17	8.355	542	544	546	rBV	495209	446693	9.66%	1.171%
18	8.412	546	549	551	rVB3	27672	49167	1.06%	0.129%
19	8.457	551	553	556	rBV2	40043	84720	1.83%	0.222%
20	8.515	556	558	559	rVV	201737	224214	4.85%	0.588%
21	8.549	559	561	564	rVV	2832578	3879819	83.94%	10.172%
22	8.652	567	570	573	rVB4	45518	94639	2.05%	0.248%
23	8.800	581	583	586	rBV2	27846	51298	1.11%	0.134%
24	8.995	597	600	604	rBV3	32595	85411	1.85%	0.224%
25	9.155	612	614	615	rBV2	48042	52467	1.14%	0.138%
26	9.177	615	616	618	rVB2	62645	63482	1.37%	0.166%
27	9.223	618	620	625	rVB2	155674	210958	4.56%	0.553%
28	9.315	625	628	629	rBV	4726859	4621865	100.00%	12.117%
29	9.338	629	630	632	rVB	300666	242503	5.25%	0.636%
30	9.383	632	634	636	rBV	305183	263817	5.71%	0.692%
31	9.418	636	637	642	rVB2	175619	250520	5.42%	0.657%
32	9.532	646	647	650	rBV2	42427	78956	1.71%	0.207%
33	9.635	654	656	658	rBV2	103431	121608	2.63%	0.319%
34	9.703	660	662	663	rBV	275609	297141	6.43%	0.779%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092515\
 Data File : BF081813.D
 Acq On : 25 Sep 2015 20:26
 Operator : UM/IZ
 Sample : G3676-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TEC-6

Integration Parameters: rteint.p

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	9.795	668	670	674	rVB3	46889	89960	1.95%	0.236%
36	9.852	674	675	676	rBV	63371	57372	1.24%	0.150%
37	9.886	676	678	679	rBV2	36045	61234	1.32%	0.161%
38	9.909	679	680	683	rVB	292024	310794	6.72%	0.815%
39	9.989	685	687	689	rVB	1497007	1281013	27.72%	3.358%
40	10.058	689	693	694	rVB3	35053	58881	1.27%	0.154%
41	10.149	698	701	702	rBV	45376	78955	1.71%	0.207%
42	10.195	704	705	707	rBV	60942	72797	1.58%	0.191%
43	10.252	707	710	711	rBV	300310	316959	6.86%	0.831%
44	10.366	718	720	721	rBV	69232	60688	1.31%	0.159%
45	10.412	722	724	726	rVV2	250839	229670	4.97%	0.602%
46	10.469	728	729	733	rVB4	31754	49025	1.06%	0.129%
47	10.629	741	743	746	rBV2	112618	174786	3.78%	0.458%
48	10.675	746	747	749	rVV2	48429	65877	1.43%	0.173%
49	10.778	753	756	759	rVV	1752296	1600610	34.63%	4.196%
50	10.835	759	761	762	rVV	274756	260239	5.63%	0.682%
51	10.881	764	765	768	rVB2	155080	197057	4.26%	0.517%
52	11.018	776	777	779	rVB	89291	91324	1.98%	0.239%
53	11.075	779	782	784	rBV	114757	129208	2.80%	0.339%
54	11.132	785	787	789	rVB	68412	75349	1.63%	0.198%
55	11.246	793	797	798	rBV2	39283	80418	1.74%	0.211%
56	11.338	803	805	809	rBV3	299978	411553	8.90%	1.079%
57	11.395	809	810	813	rVB	48483	64832	1.40%	0.170%
58	11.475	815	817	820	rVB	1279709	1123628	24.31%	2.946%
59	11.658	830	833	834	rBV	502943	565751	12.24%	1.483%
60	11.863	848	851	852	rBV3	33560	53711	1.16%	0.141%
61	12.001	861	863	867	rBV	363359	393828	8.52%	1.032%
62	12.184	877	879	882	rVB3	51919	63011	1.36%	0.165%
63	12.789	930	932	935	rBV2	103252	139273	3.01%	0.365%
64	12.949	944	946	948	rVB	63089	72012	1.56%	0.189%
65	13.064	953	956	959	rBV	2987893	3214878	69.56%	8.428%
66	13.624	1003	1005	1009	rBV4	52146	87584	1.89%	0.230%
67	13.955	1032	1034	1036	rBV	121169	133430	2.89%	0.350%
68	14.115	1046	1048	1053	rVB	1009440	949131	20.54%	2.488%
69	15.590	1174	1177	1180	rVB	701344	883588	19.12%	2.316%
70	16.104	1219	1222	1226	rVB	36618	72237	1.56%	0.189%
71	17.235	1317	1321	1329	rBV2	181155	492243	10.65%	1.291%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092515\
Data File : BF081813.D
Acq On : 25 Sep 2015 20:26
Operator : UM/IZ
Sample : G3676-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEC-6

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	17.635	1354	1356	1359	rVB4	31329	59133	1.28%	0.155%
----	--------	------	------	------	------	-------	-------	-------	--------


Sum of corrected areas: 38143544

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092515\
Data File : BF081813.D
Acq On : 25 Sep 2015 20:26
Operator : UM/IZ
Sample : G3676-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEC-6

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

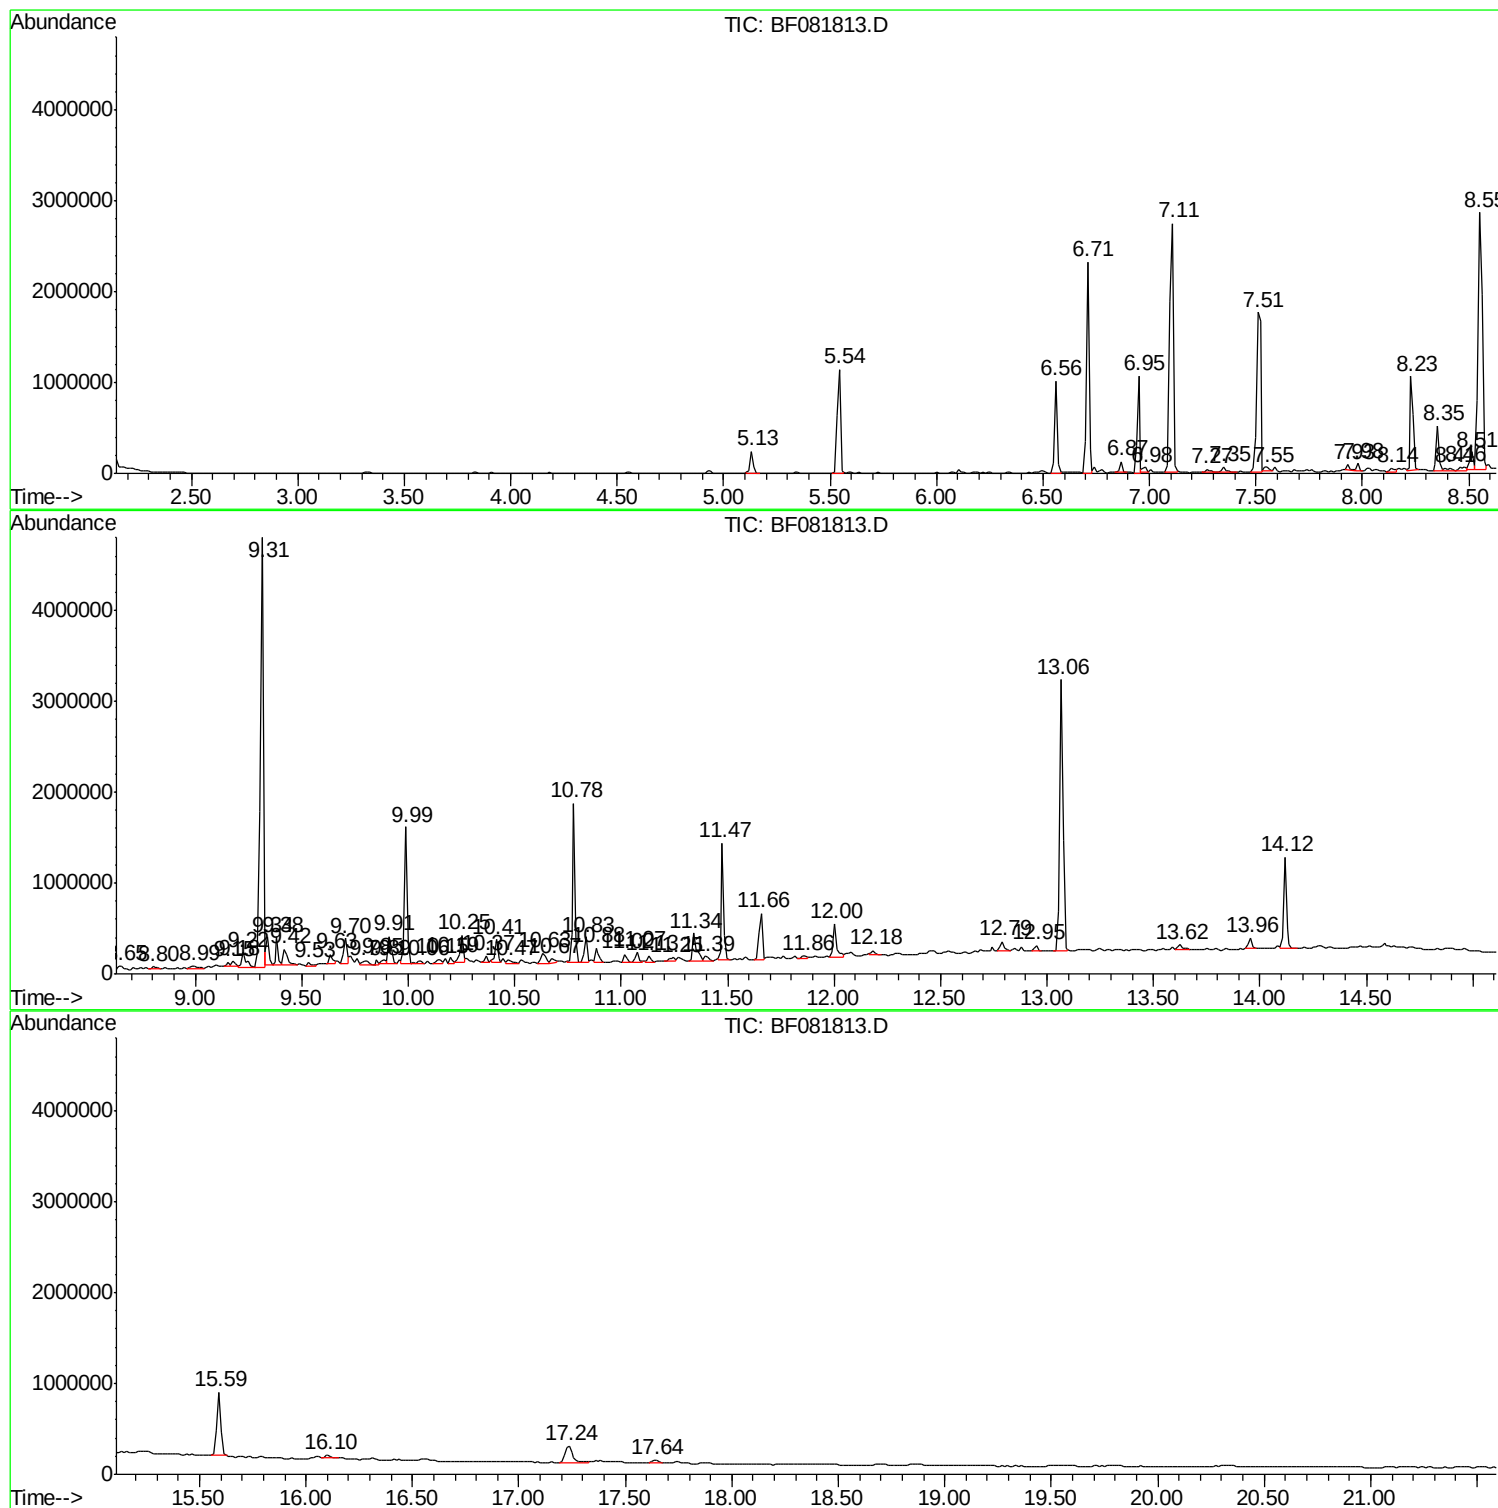

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092515\
Data File : BF081813.D
Acq On : 25 Sep 2015 20:26
Operator : UM/IZ
Sample : G3676-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEC-6

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092515\
Data File : BF081813.D
Acq On : 25 Sep 2015 20:26
Operator : UM/IZ
Sample : G3676-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TEC-6

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc