


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092515\
 Data File : BF081799.D
 Acq On : 25 Sep 2015 13:06
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 25 06:02:49 2015

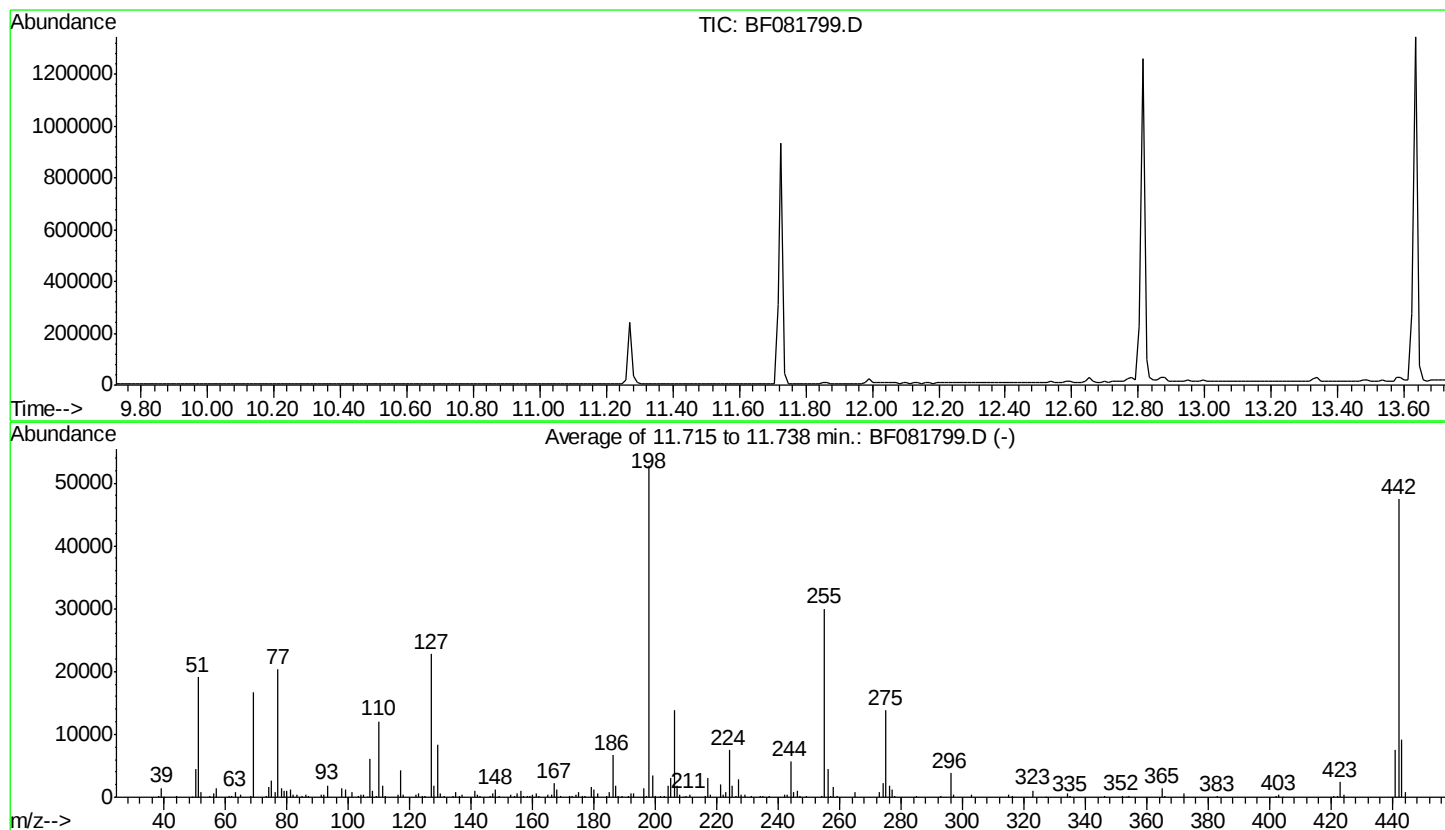

AutoFind: Scans 838, 839, 840; Background Corrected with Scan 835

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	19060	PASS
68	69	0.00	2	1.8	306	PASS
69	198	0.00	100	31.5	16643	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	22799	PASS
197	198	0.00	2	0.4	232	PASS
198	198	100	100	100.0	52756	PASS
199	198	5	9	6.5	3443	PASS
275	198	10	60	26.2	13847	PASS
365	198	1	100	2.5	1335	PASS
441	442	0.01	24	15.8	7491	PASS
442	198	50	100	89.8	47390	PASS
443	442	15	24	19.5	9254	PASS