
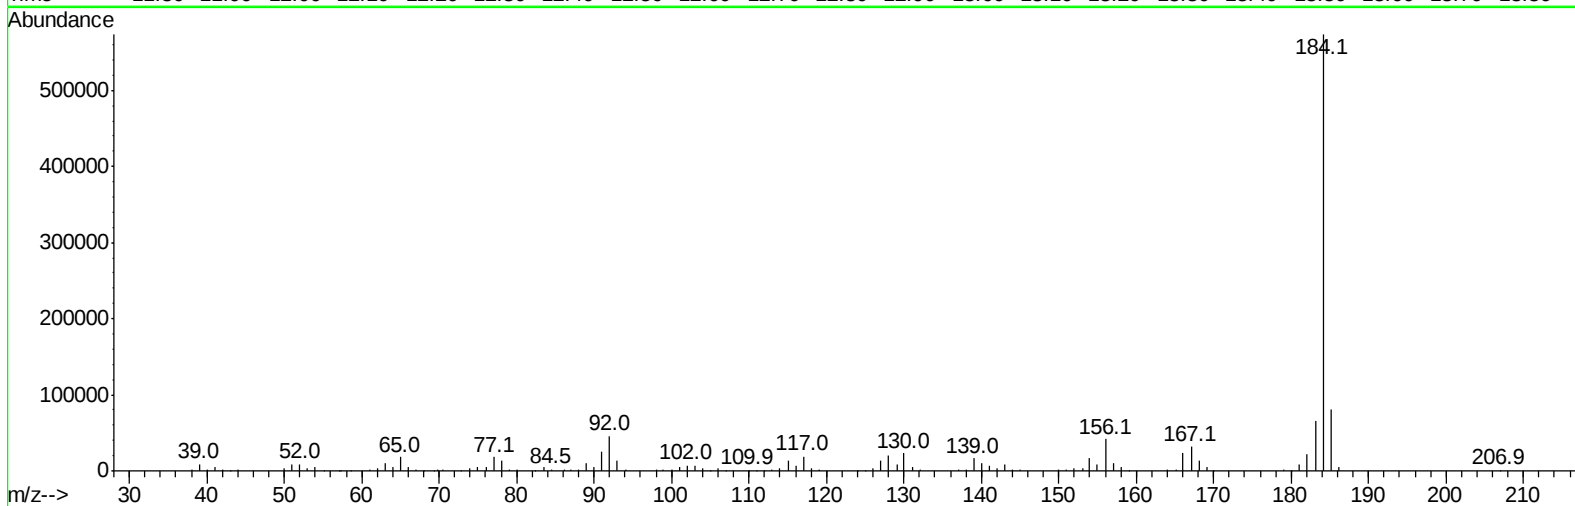


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092517\
Data File : BF098772.D
Acq On : 25 Sep 2017 9:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 09:21:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

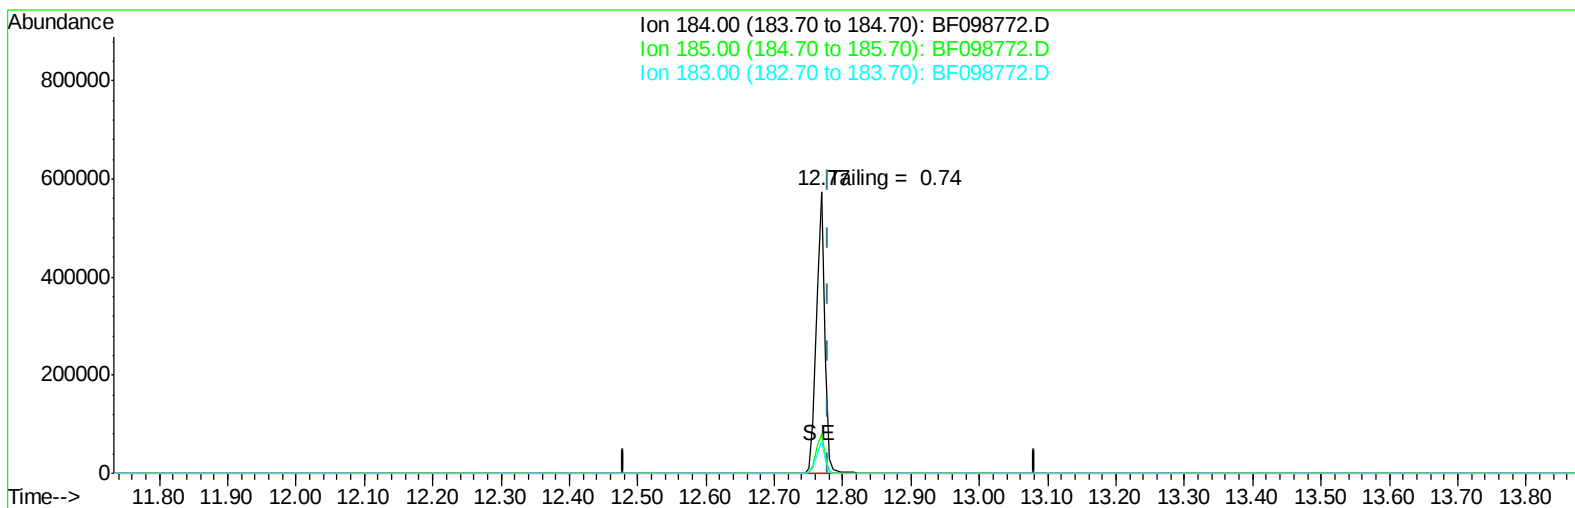

TIC: BF098772.D

(76) Benzidine



12.769min (-0.012) 0.00ng

response 480248

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.95
183.00	11.60	11.57
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092517\
Data File : BF098772.D
Acq On : 25 Sep 2017 9:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 09:21:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

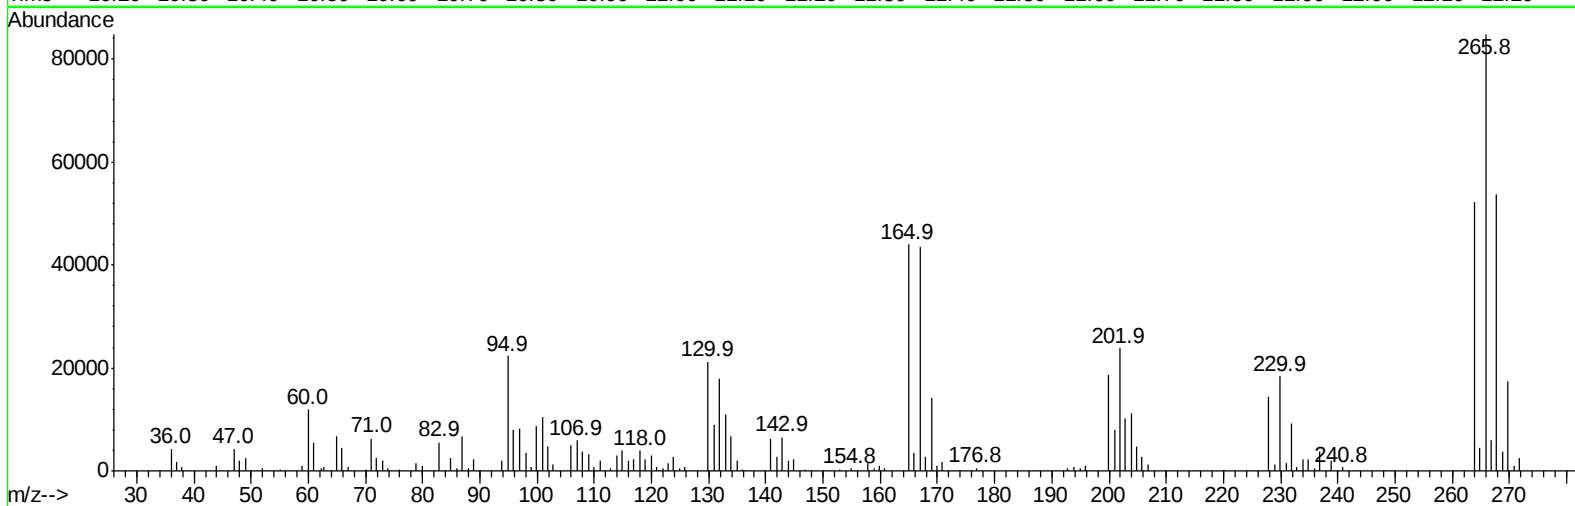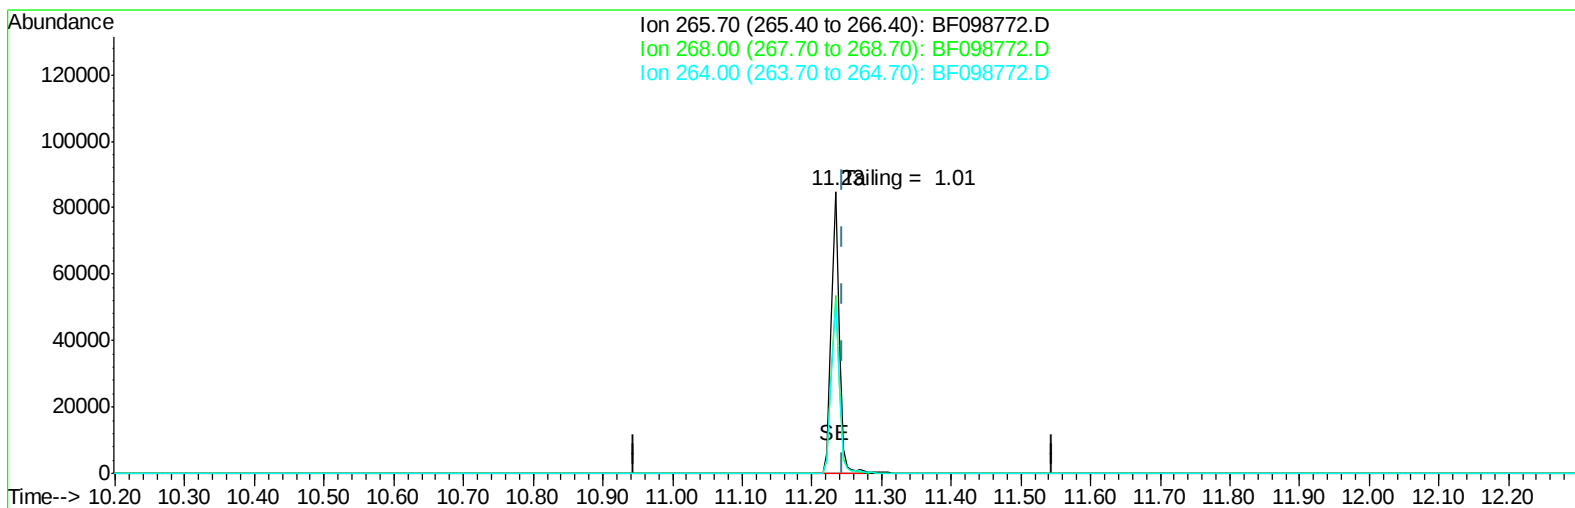

TIC: BF098772.D

(69) Pentachlorophenol (C)

11.233min (-0.012) 63106.28ng

response 65695

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.35
264.00	61.90	61.58
0.00	0.00	0.00