
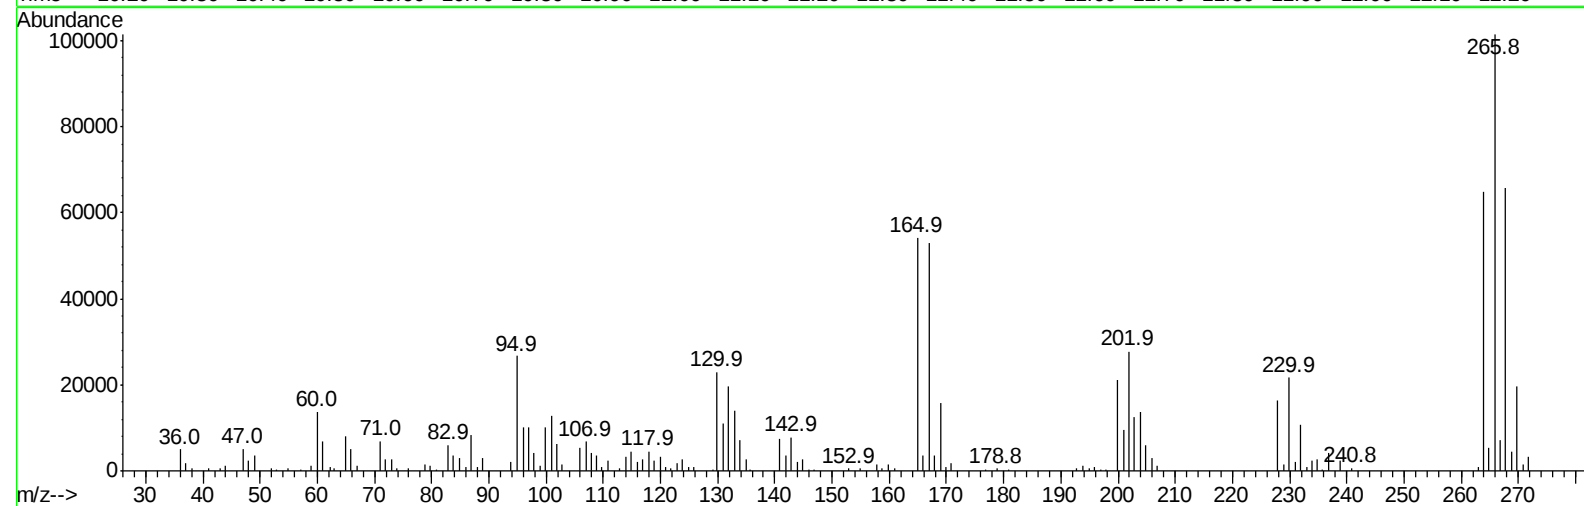


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092517\
Data File : BF098785.D
Acq On : 25 Sep 2017 16:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 09:22:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

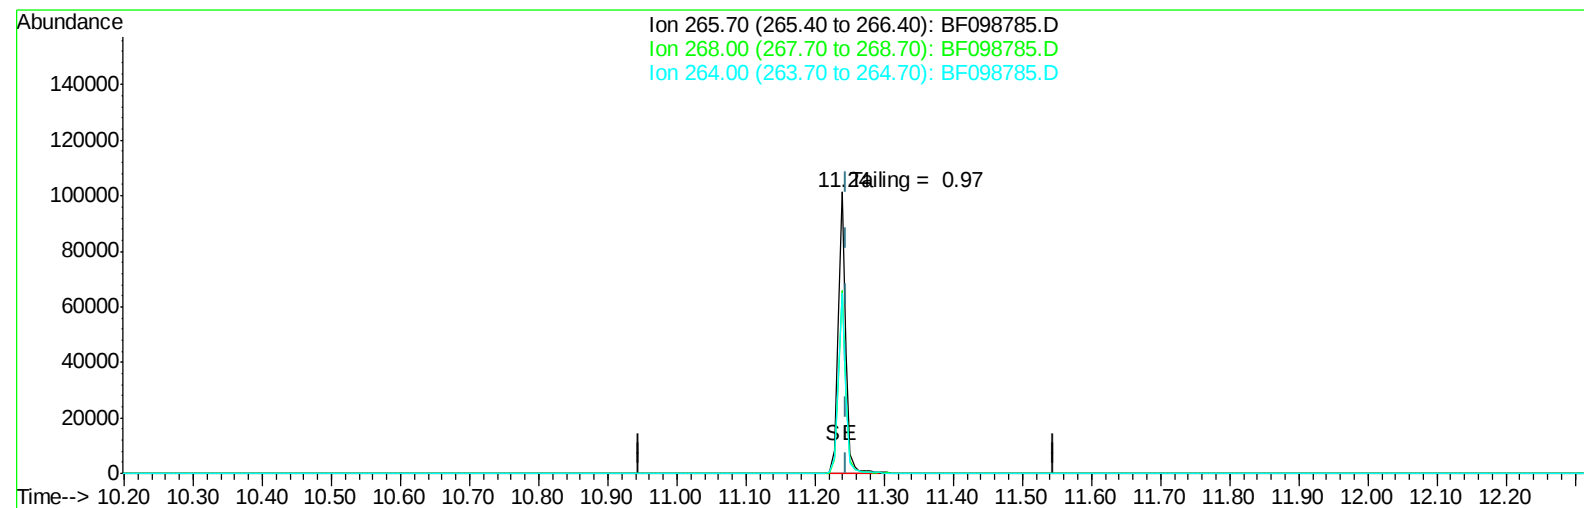

TIC: BF098785.D

(69) Pentachlorophenol (C)



11.239min (-0.006) 43180.20ng

response 79508

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.86
264.00	61.90	63.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092517\
Data File : BF098785.D
Acq On : 25 Sep 2017 16:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 09:22:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

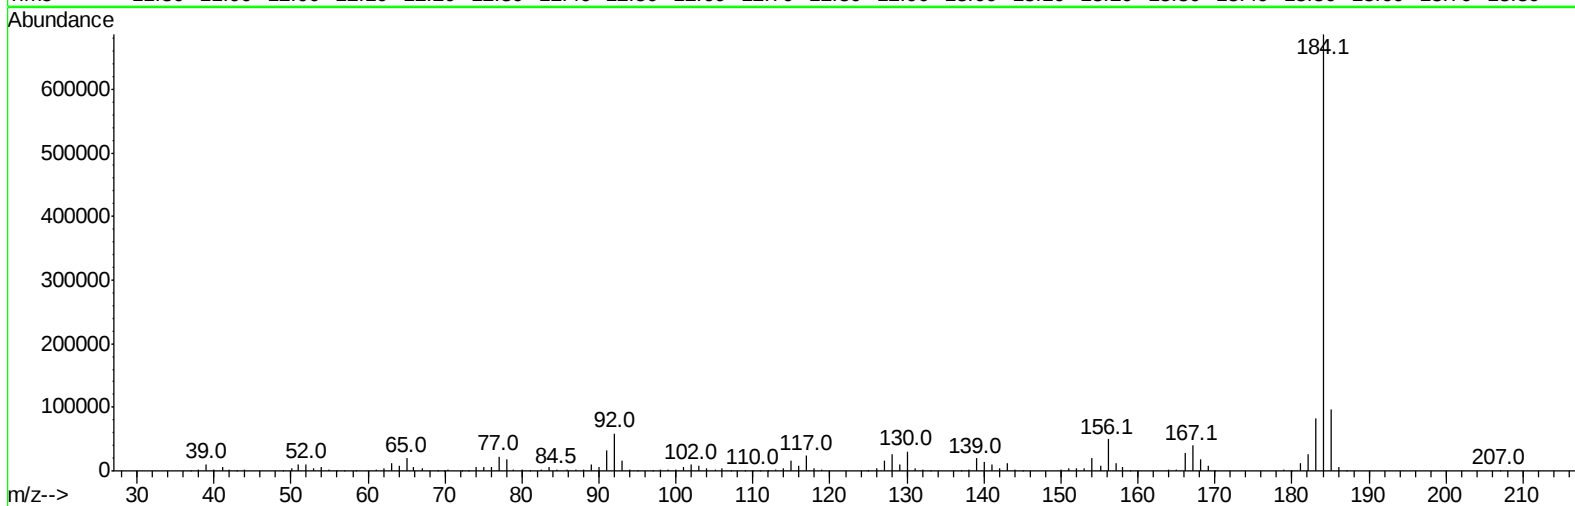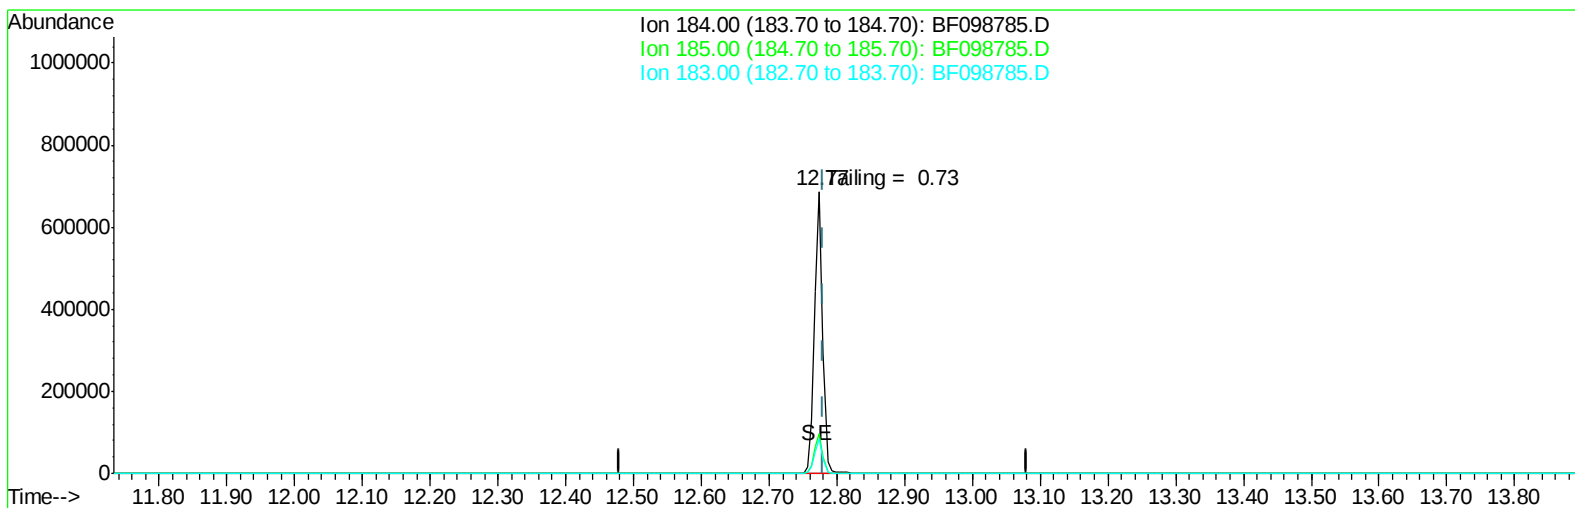

TIC: BF098785.D

(76) Benzidine

12.774min (-0.006) 0.00ng

response 571774

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.94
183.00	11.60	12.08
0.00	0.00	0.00