
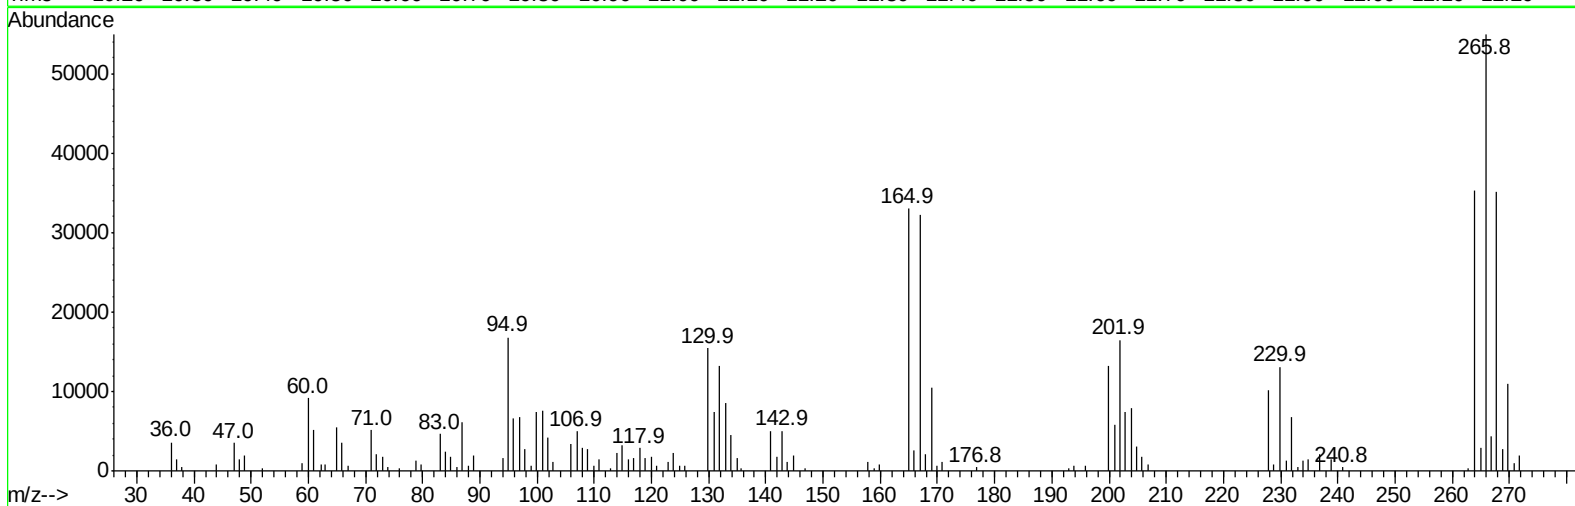


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092517\
Data File : BF098811.D
Acq On : 26 Sep 2017 5:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 09:23:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

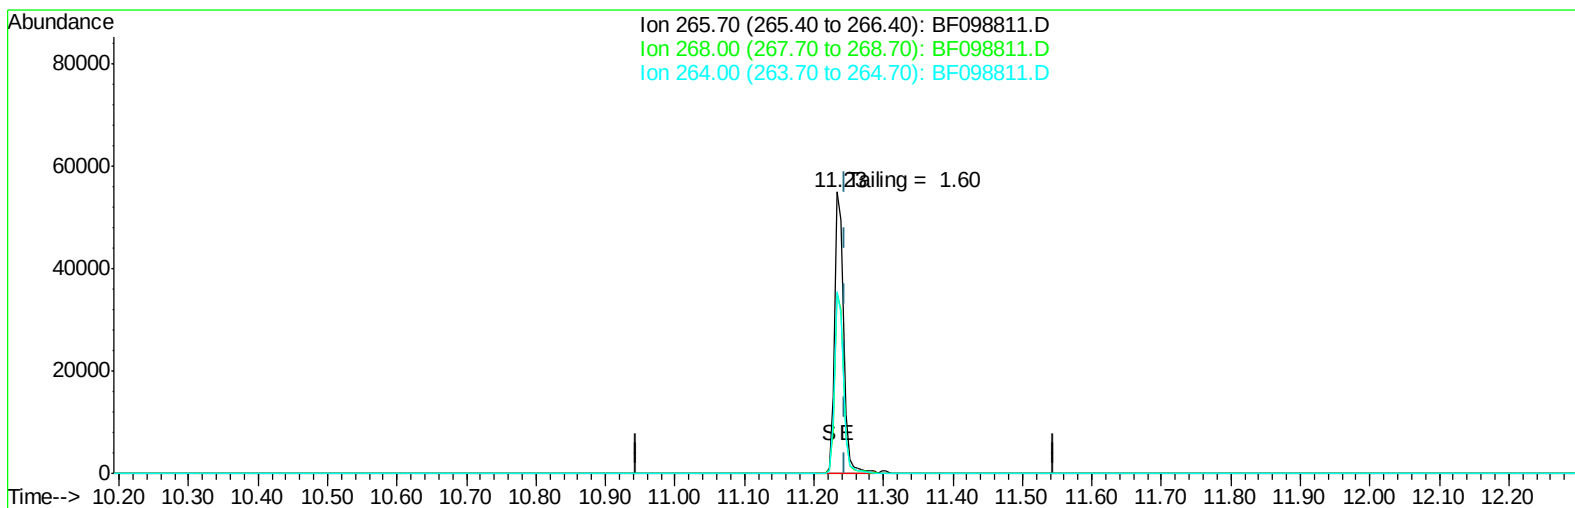

TIC: BF098811.D

(69) Pentachlorophenol (C)



11.233min (-0.012) 28357.92ng

response 49079

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.06
264.00	61.90	64.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092517\
Data File : BF098811.D
Acq On : 26 Sep 2017 5:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 09:23:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

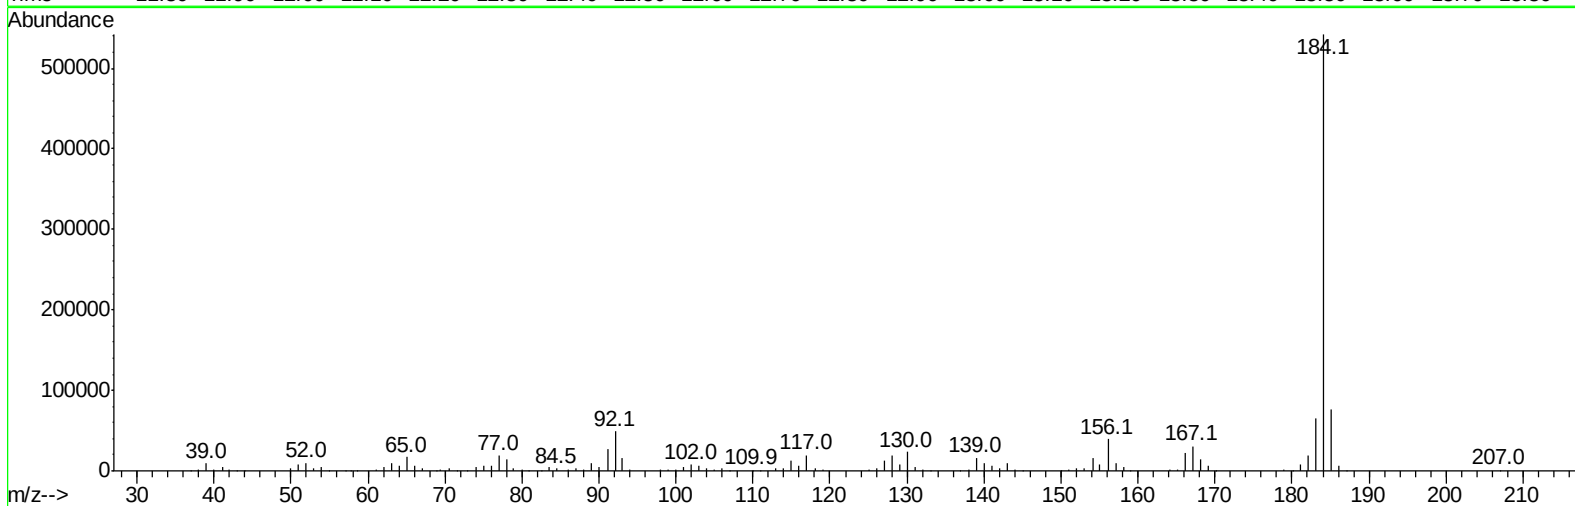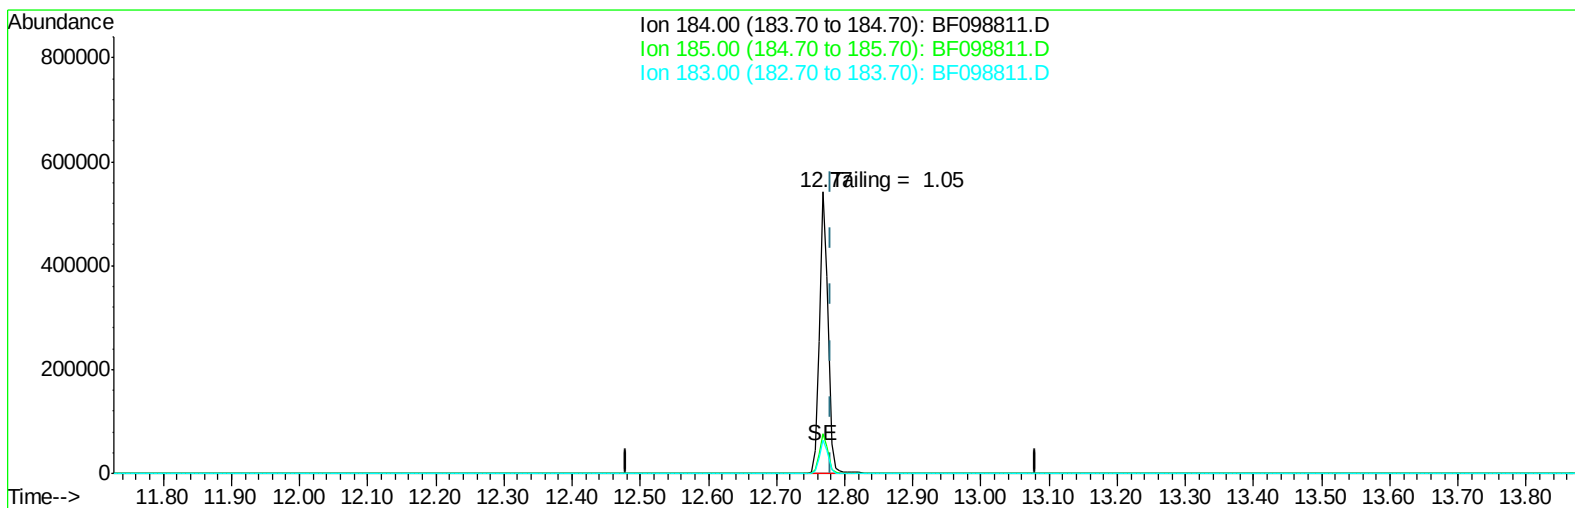

TIC: BF098811.D

(76) Benzidine

12.769min (-0.012) 0.00ng

response 462356

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.18
183.00	11.60	11.92
0.00	0.00	0.00