


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092517\
 Data File : BF098772.D
 Acq On : 25 Sep 2017 9:45
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

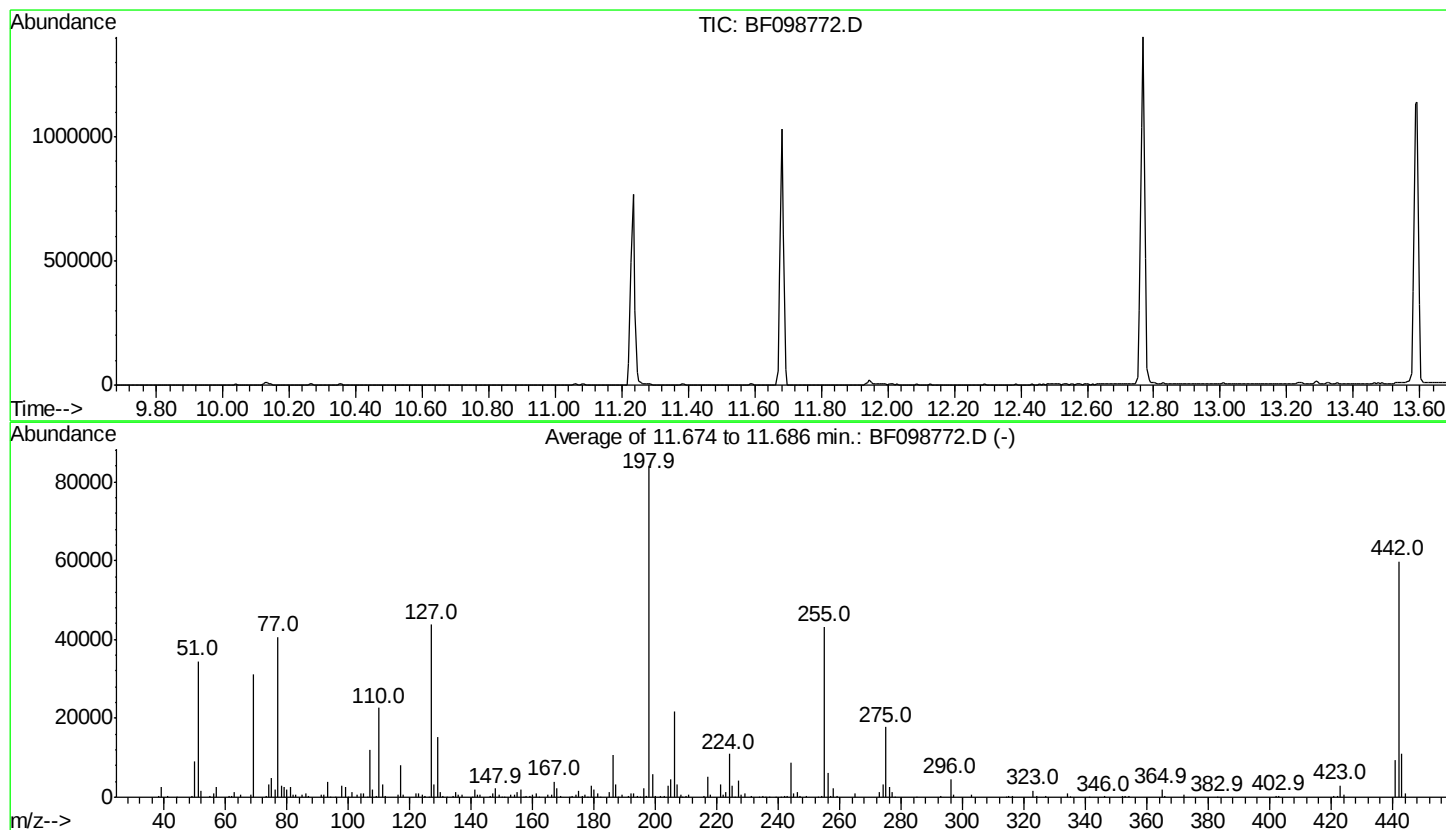

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	34480	PASS
68	69	0.00	2	1.8	570	PASS
69	198	0.00	100	36.9	31072	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.0	43760	PASS
197	198	0.00	2	0.5	445	PASS
198	198	100	100	100.0	84098	PASS
199	198	5	9	7.0	5873	PASS
275	198	10	60	21.1	17775	PASS
365	198	1	100	2.4	2045	PASS
441	442	0.01	24	15.6	9322	PASS
442	198	50	100	71.2	59842	PASS
443	442	15	24	18.5	11085	PASS