


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092517\
 Data File : BF098785.D
 Acq On : 25 Sep 2017 16:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

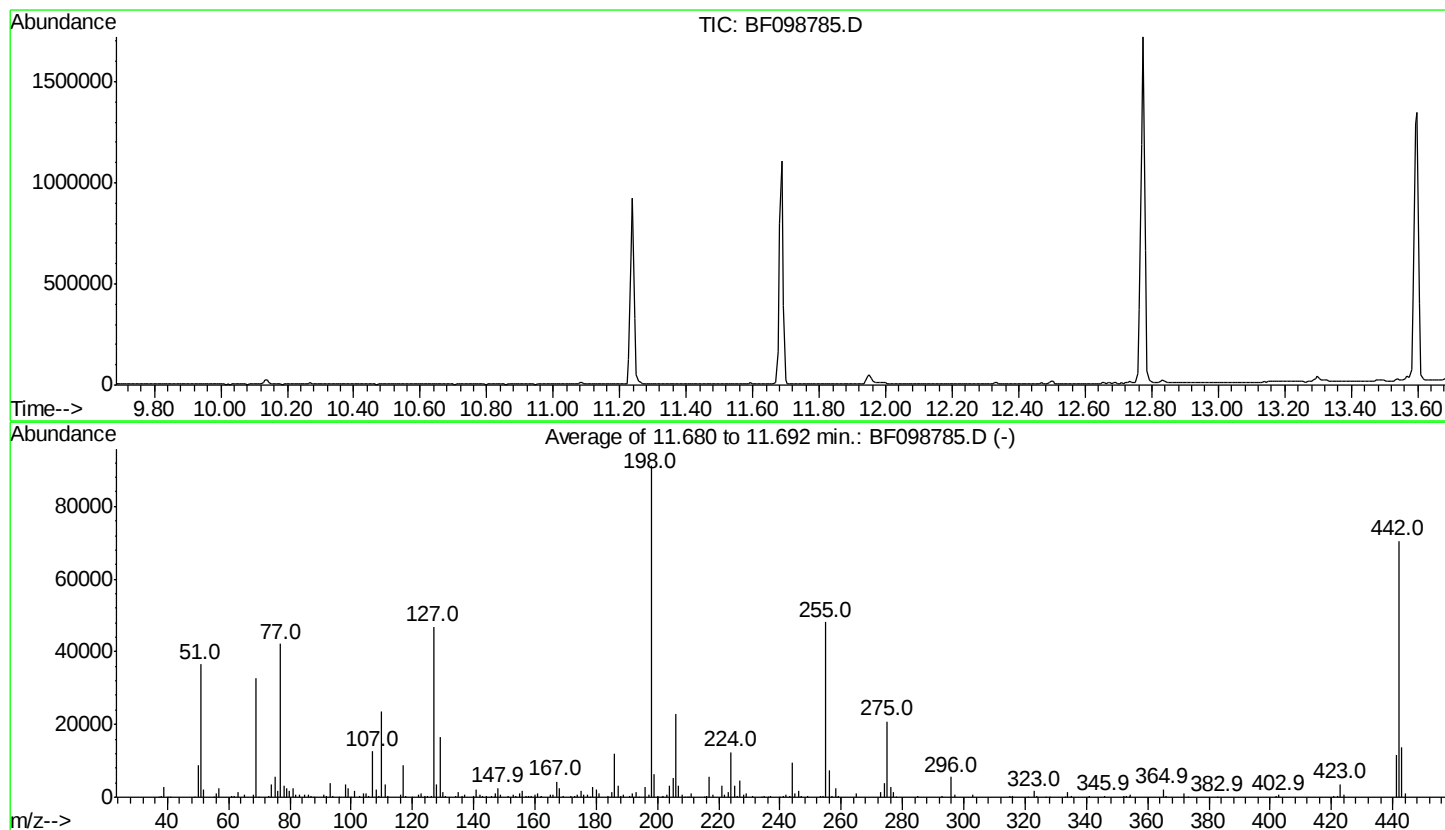

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	36476	PASS
68	69	0.00	2	1.9	622	PASS
69	198	0.00	100	36.1	32917	PASS
70	69	0.00	2	0.4	143	PASS
127	198	10	80	51.5	46933	PASS
197	198	0.00	2	0.9	823	PASS
198	198	100	100	100.0	91200	PASS
199	198	5	9	7.1	6468	PASS
275	198	10	60	22.9	20879	PASS
365	198	1	100	2.5	2294	PASS
441	442	0.01	24	16.4	11569	PASS
442	198	50	100	77.4	70597	PASS
443	442	15	24	19.6	13835	PASS