


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092518\
 Data File : BF109281.D
 Acq On : 25 Sep 2018 12:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 22 13:32:18 2018

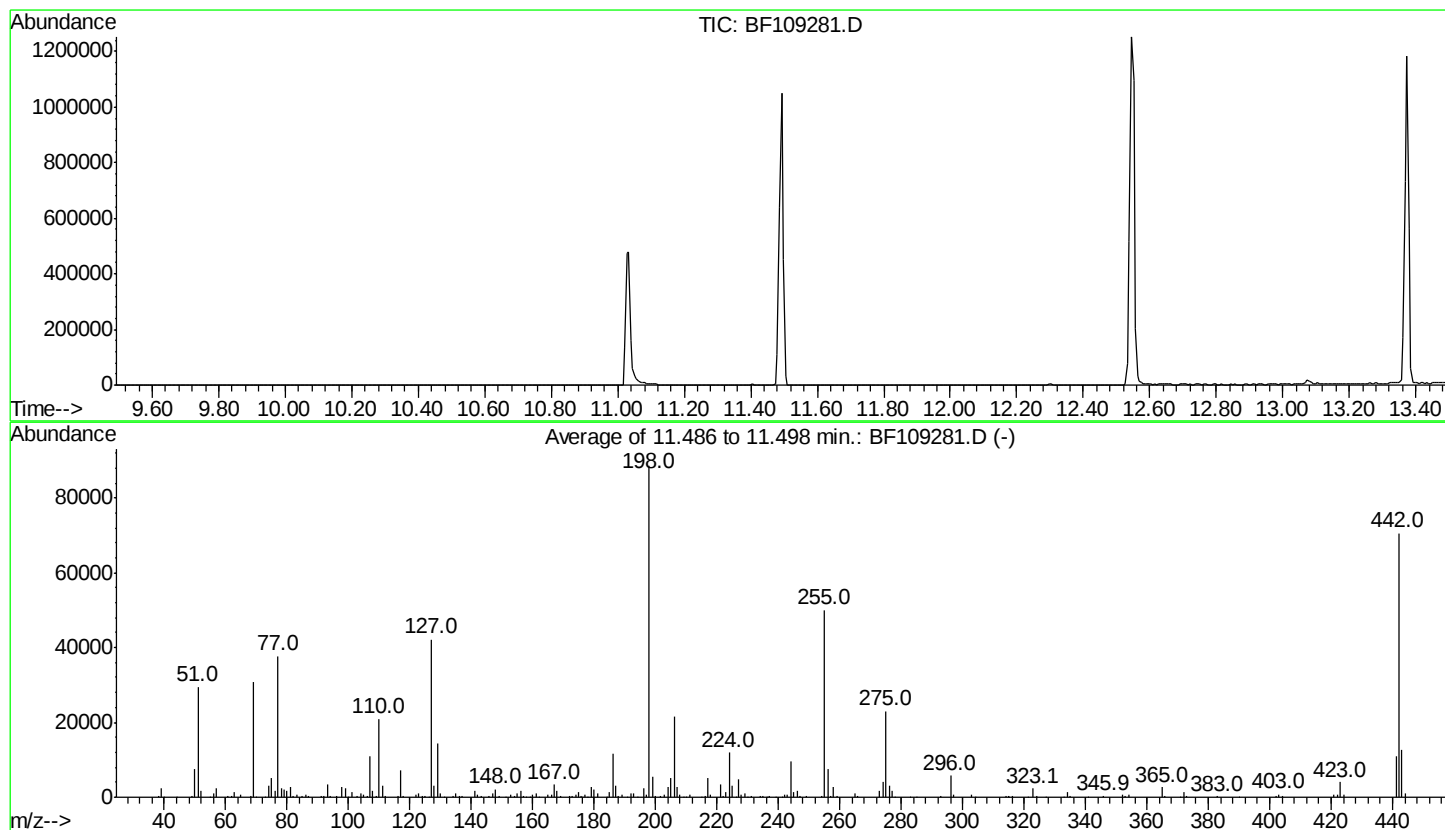

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	29595	PASS
68	69	0.00	2	1.4	417	PASS
69	198	0.00	100	34.7	30779	PASS
70	69	0.00	2	0.4	111	PASS
127	198	10	80	47.5	42117	PASS
197	198	0.00	2	0.7	636	PASS
198	198	100	100	100.0	88626	PASS
199	198	5	9	6.4	5638	PASS
275	198	10	60	26.1	23093	PASS
365	198	1	100	3.1	2739	PASS
441	198	0.01	100	12.4	10978	PASS
442	198	50	100	79.6	70570	PASS
443	442	15	24	18.1	12790	PASS