
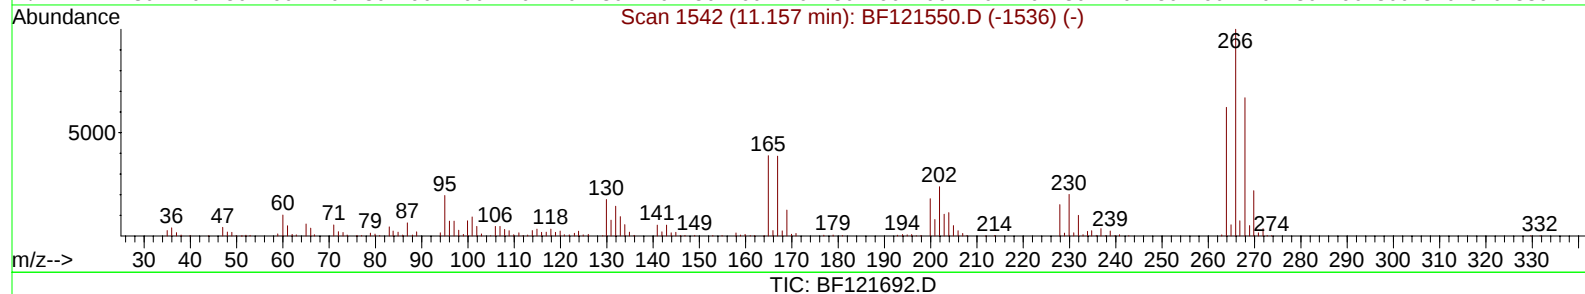
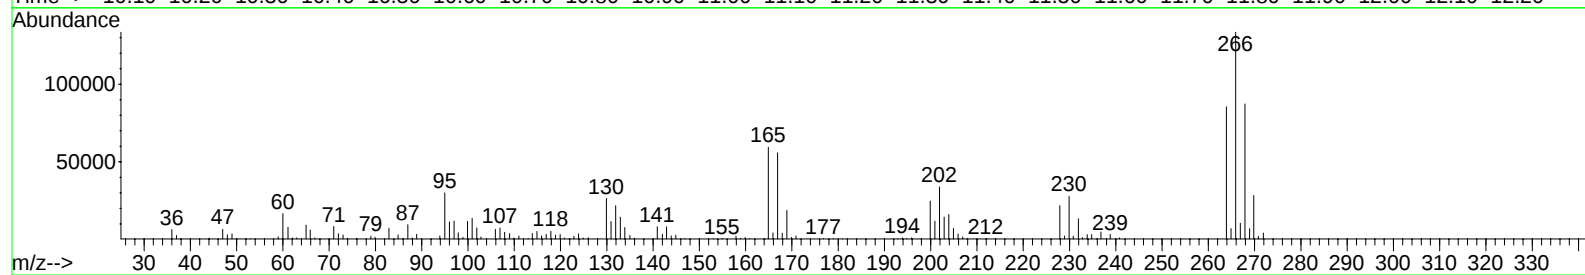


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092520\
 Data File : BF121692.D
 Acq On : 25 Sep 2020 13:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 18:19:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 25 14:15:19 2020
 Response via : Initial Calibration

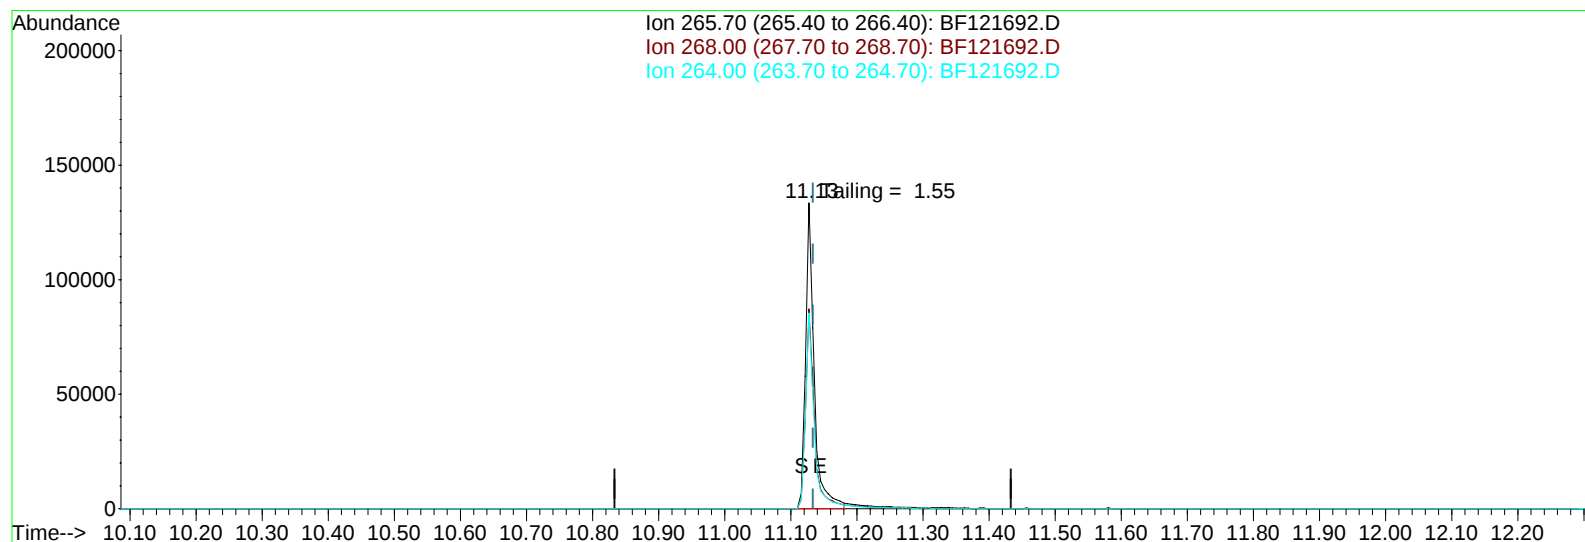

(70) Pentachlorophenol (C)




11.127min (-0.006) 38920.96ng

response 128807

Ion	Exp%	Act%
265.70	100	100
268.00	66.80	65.37
264.00	60.90	64.02
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092520\
 Data File : BF121692.D
 Acq On : 25 Sep 2020 13:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 18:19:54 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 25 14:15:19 2020
 Response via : Initial Calibration

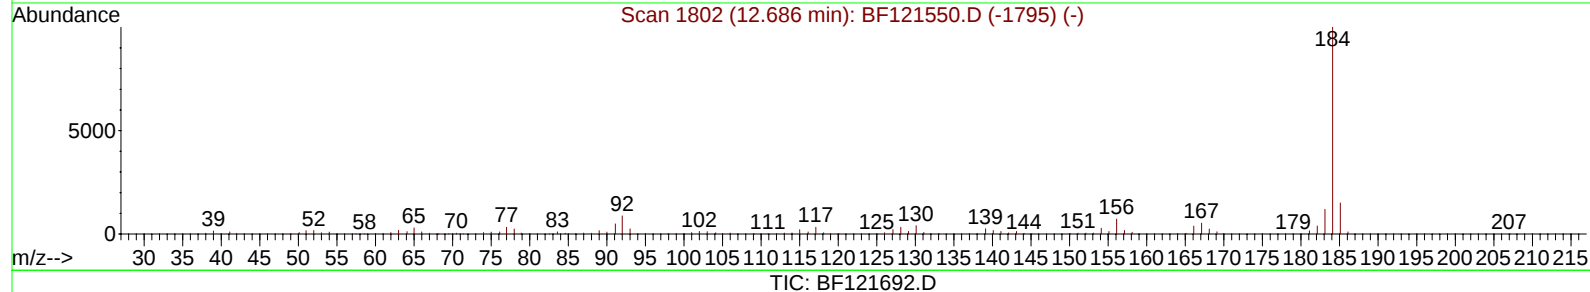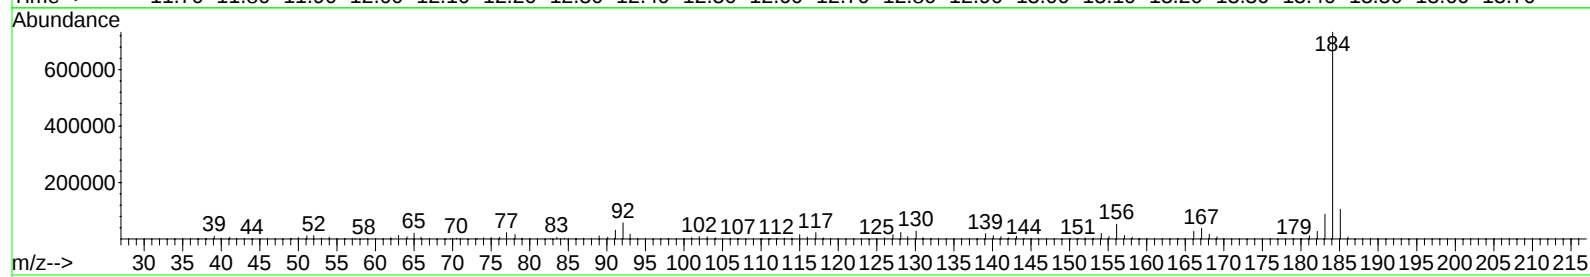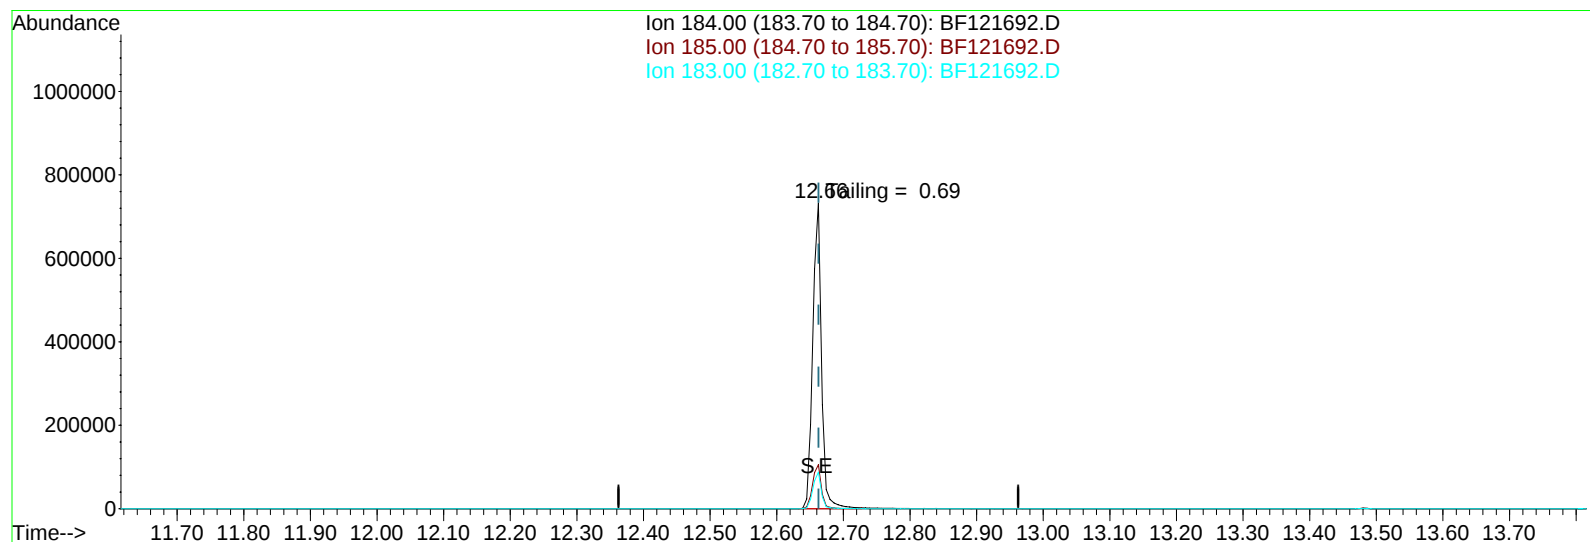

(77) Benzidine

12.663min (-0.000) 0.00ng

response 675337

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.40
183.00	11.90	12.01
0.00	0.00	0.00