


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092520\
 Data File : BF121692.D
 Acq On : 25 Sep 2020 13:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 28 11:40:42 2020

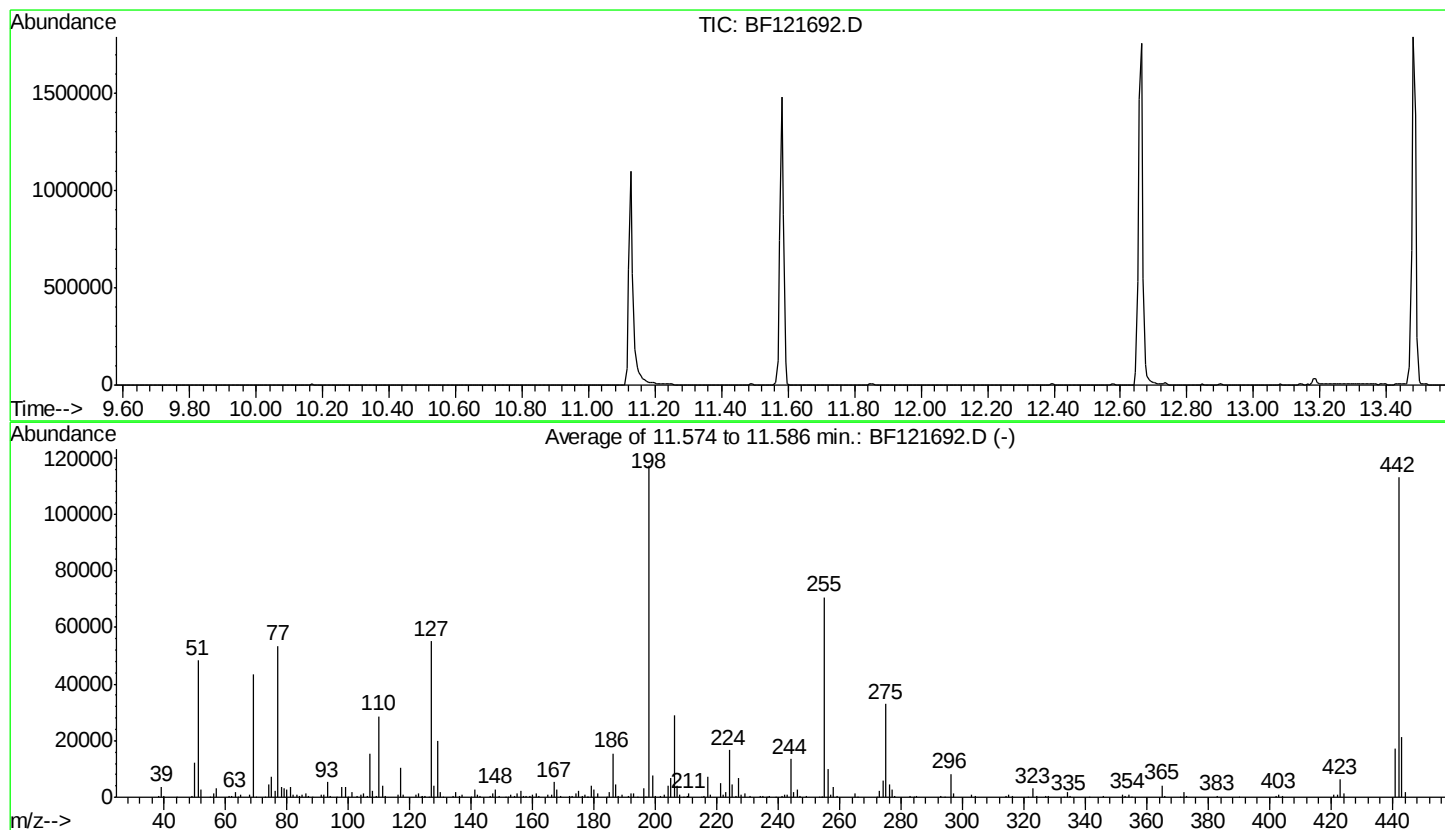

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	48261	PASS
68	69	0.00	2	1.7	743	PASS
69	198	0.00	100	36.9	43250	PASS
70	69	0.00	2	0.4	162	PASS
127	198	10	80	47.0	55130	PASS
197	198	0.00	2	0.2	207	PASS
198	198	100	100	100.0	117248	PASS
199	198	5	9	6.4	7548	PASS
275	198	10	60	28.0	32872	PASS
365	198	1	100	3.5	4129	PASS
441	198	0.01	100	14.6	17155	PASS
442	198	50	100	96.4	113024	PASS
443	442	15	24	18.8	21206	PASS