

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092521\
 Data File : BF125663.D
 Acq On : 25 Sep 2021 18:36
 Operator : JU/CG
 Sample : M3939-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TS-1

Quant Time: Sep 27 01:23:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.887	152	171507	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	701096	20.000	ng	# 0.00
39) Acenaphthene-d10	9.922	164	365954	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188	601796	20.000	ng	0.00
76) Chrysene-d12	14.039	240	393019	20.000	ng	0.00
86) Perylene-d12	15.515	264	393266	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	1045460	100.431	ng	0.00
7) Phenol-d6	6.504	99	1302269	93.052	ng	0.00
23) Nitrobenzene-d5	7.445	82	767295	76.336	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	375035	109.915	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	1477428	70.214	ng	0.00
79) Terphenyl-d14	12.992	244	1239515	54.617	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092521\
Data File : BF125663.D
Acq On : 25 Sep 2021 18:36
Operator : JU/CG
Sample : M3939-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TS-1

Quant Time: Sep 27 01:23:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration




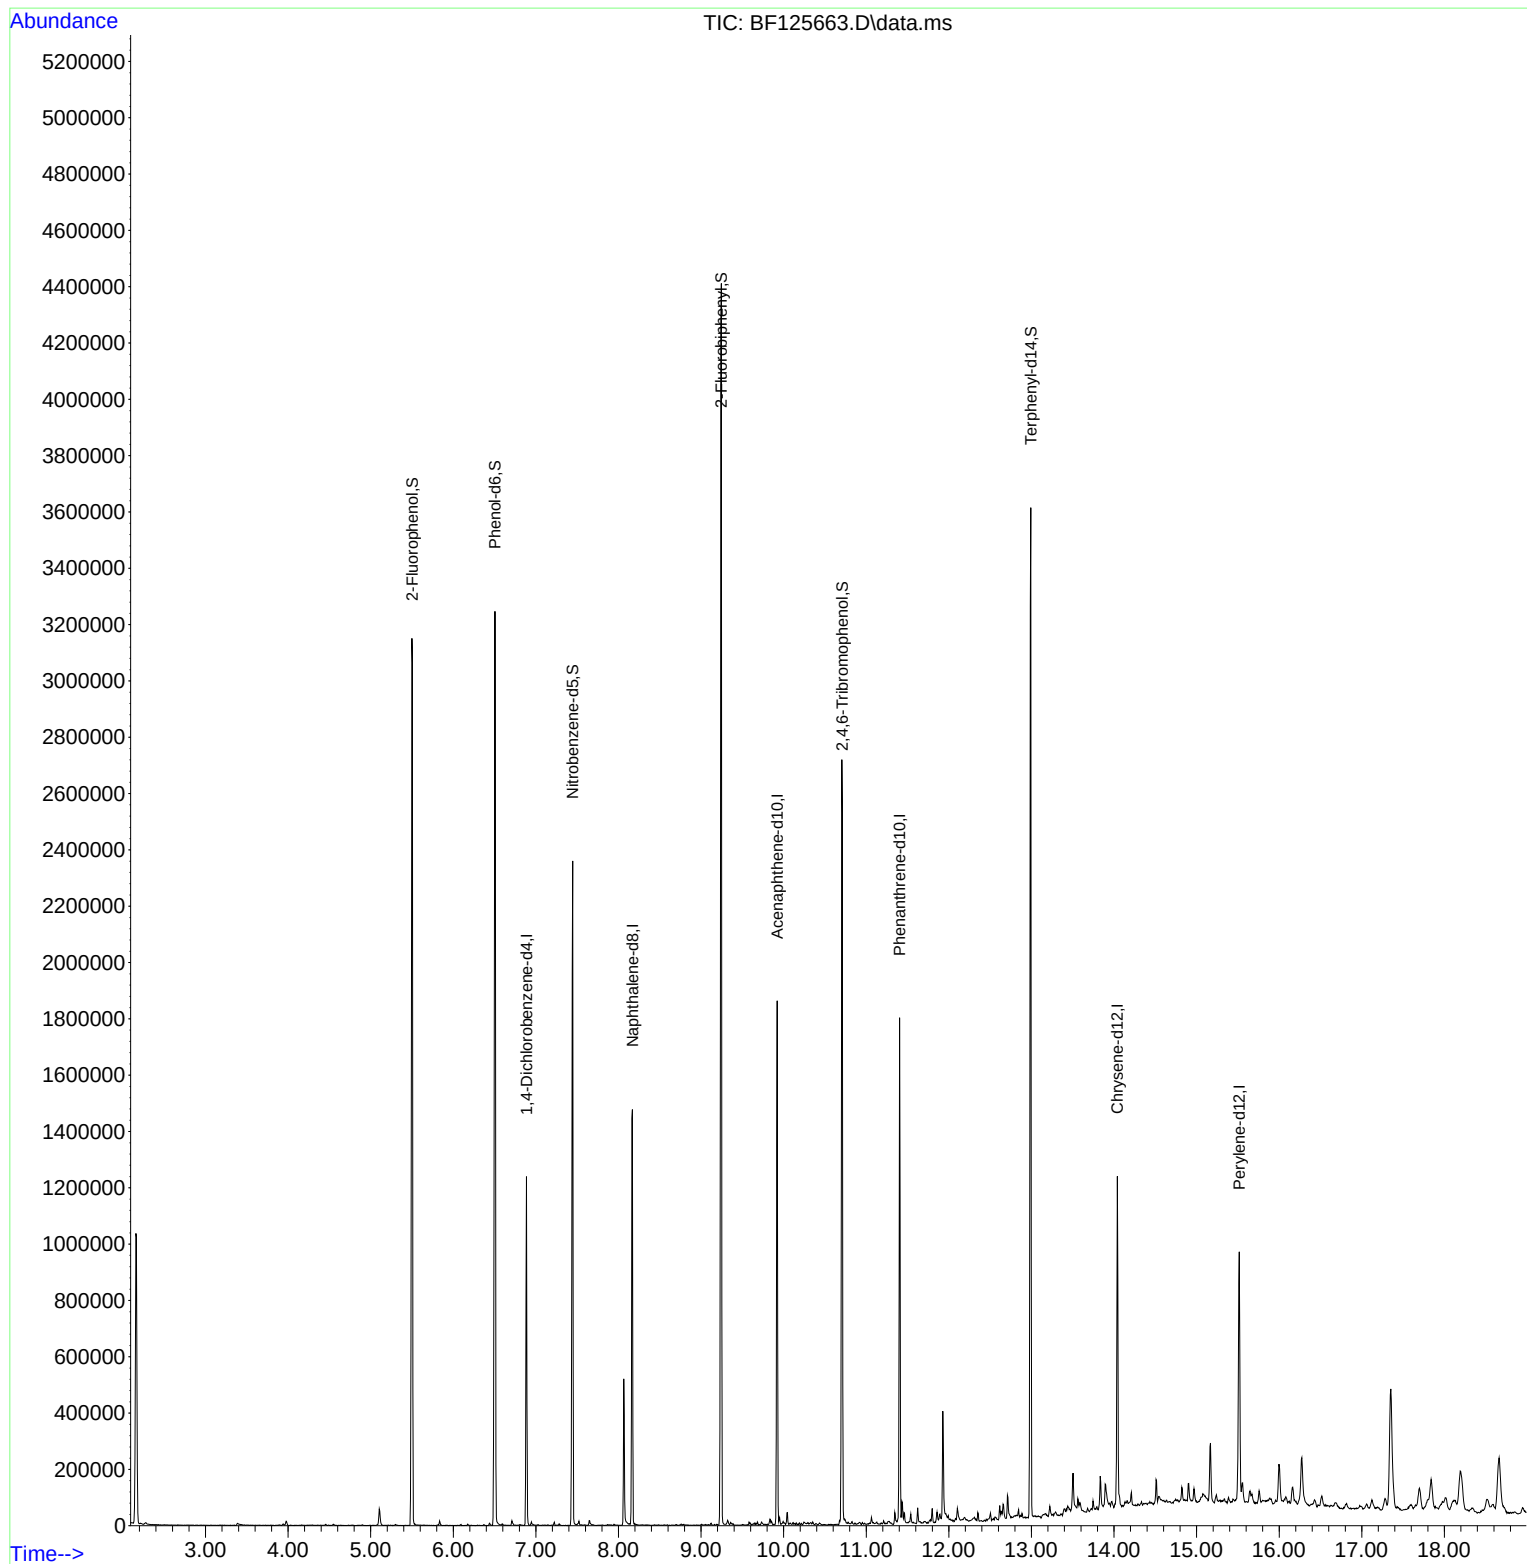




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.887 min Scan# 816
Delta R.T. -0.005 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36




Instrument :
BNA_F
ClientSampled :
TS-1


Tgt Ion:152 Resp: 171507
Ion Ratio Lower Upper
152 100
150 159.7 117.6 176.4
115 59.4 47.1 70.7

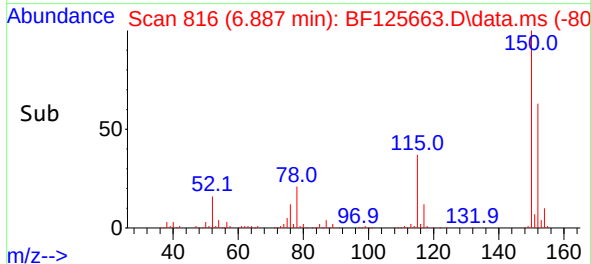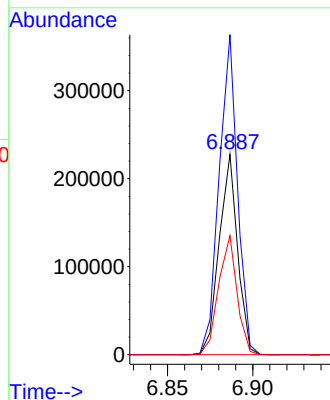

#5
2-Fluorophenol
Concen: 100.431 ng
RT: 5.504 min Scan# 581
Delta R.T. 0.000 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36

Tgt Ion:112 Resp: 1045460
Ion Ratio Lower Upper
112 100
64 50.2 44.2 66.2
63 25.2 26.2 39.2#


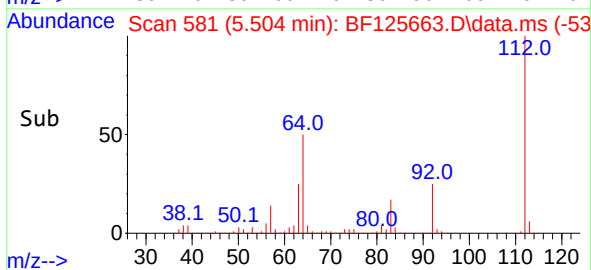
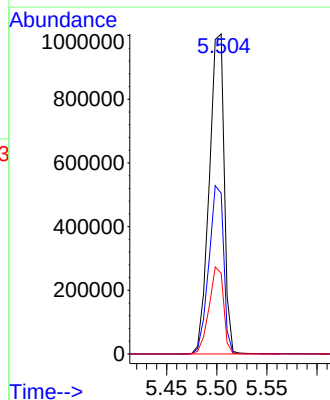
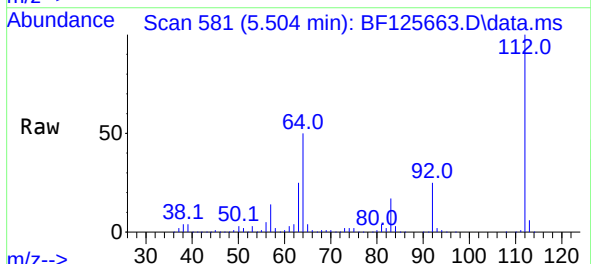




#7
Phenol-d6
Concen: 93.052 ng
RT: 6.504 min Scan# 751
Delta R.T. -0.006 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36




Instrument :
BNA_F
ClientSampleId :
TS-1


Tgt Ion: 99 Resp: 1302269
Ion Ratio Lower Upper
99 100
42 14.8 23.5 35.3#
71 30.6 25.6 38.4

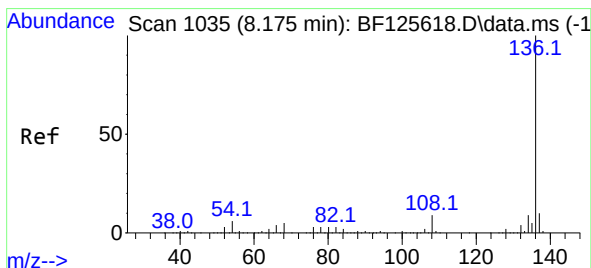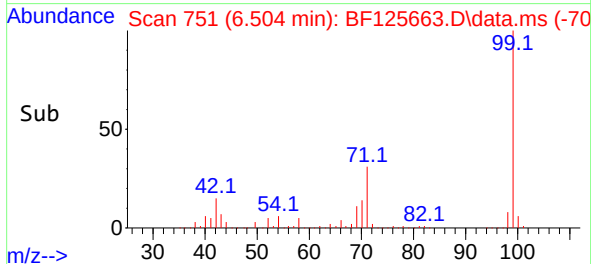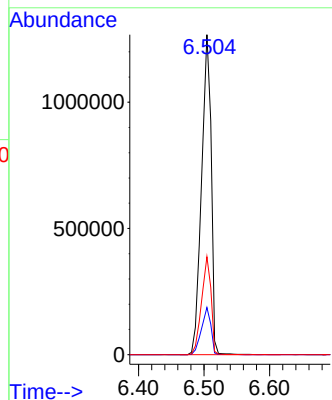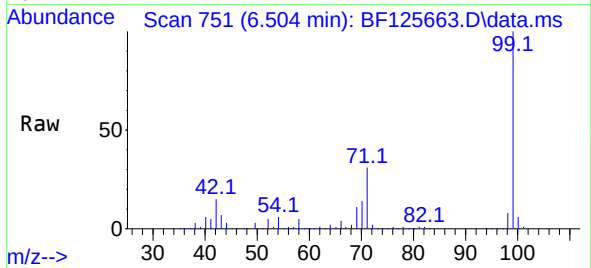

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1034
Delta R.T. -0.006 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36

Tgt Ion: 136 Resp: 701096
Ion Ratio Lower Upper
136 100
137 10.3 9.8 14.6
54 5.8 6.4 9.6#
68 4.8 3.3 4.9


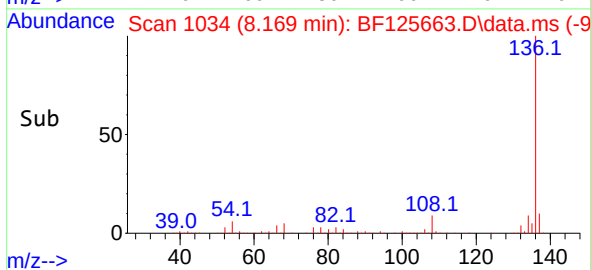
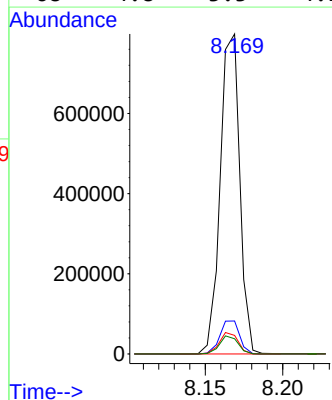
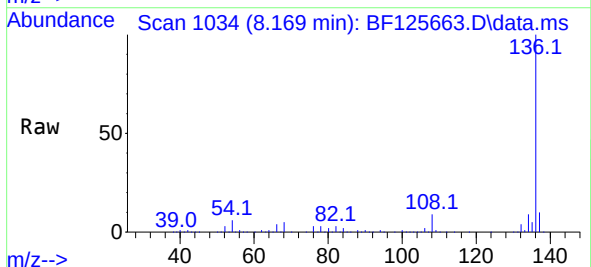




#23
Nitrobenzene-d5
Concen: 76.336 ng
RT: 7.445 min Scan# 911
Delta R.T. -0.006 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36




Instrument :
BNA_F
ClientSampleId :
TS-1


Tgt Ion: 82 Resp: 767295
Ion Ratio Lower Upper
82 100
128 49.1 40.6 60.8
54 43.2 49.6 74.4#

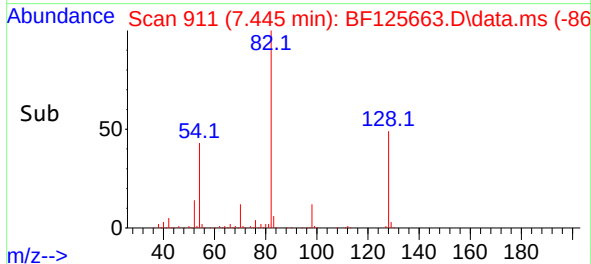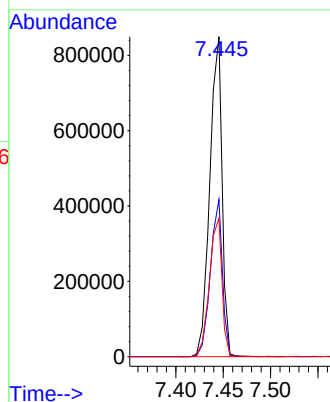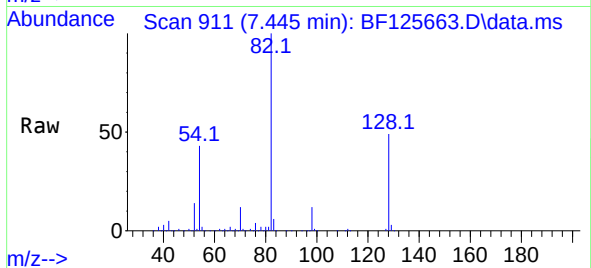

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.922 min Scan# 1332
Delta R.T. -0.006 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36

Tgt Ion:164 Resp: 365954
Ion Ratio Lower Upper
164 100
162 104.1 81.3 121.9
160 44.4 38.0 57.0


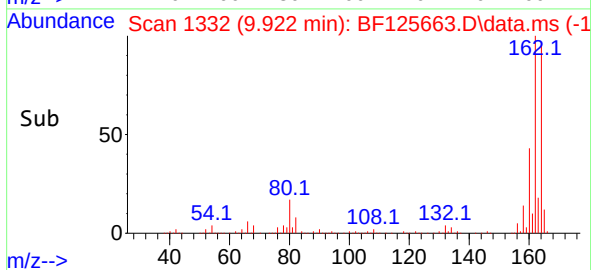
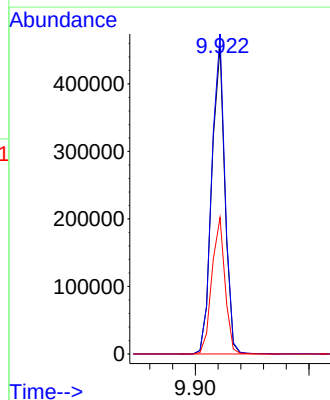
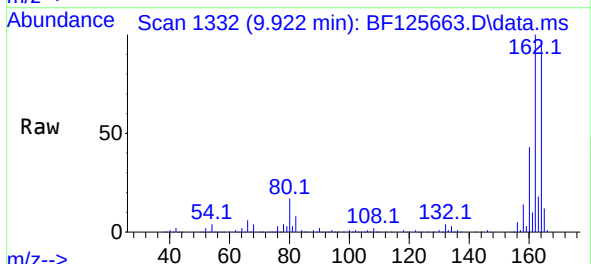




#42
2,4,6-Tribromophenol
Concen: 109.915 ng
RT: 10.710 min Scan# 1466
Delta R.T. -0.006 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36




Instrument :
BNA_F
ClientSampleId :
TS-1


Tgt Ion: 330 Resp: 375035
Ion Ratio Lower Upper
330 100
332 95.0 76.2 114.4
141 31.3 44.6 66.8#

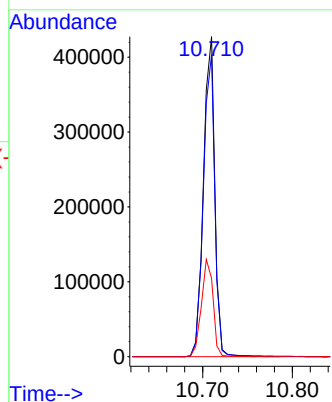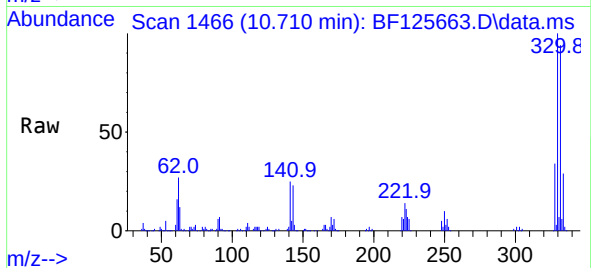

#45
2-Fluorobiphenyl
Concen: 70.214 ng
RT: 9.245 min Scan# 1217
Delta R.T. -0.006 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36

Tgt Ion: 172 Resp: 1477428
Ion Ratio Lower Upper
172 100
171 36.4 26.5 39.7
170 24.0 18.8 28.2

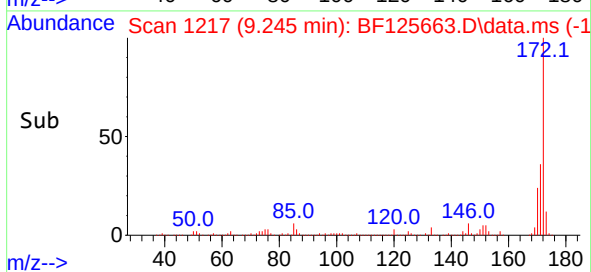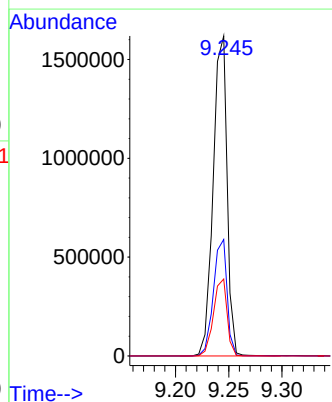







#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.404 min Scan# 1584
Delta R.T. -0.006 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36

Instrument :
BNA_F
ClientSampleId :
TS-1

Tgt Ion:188 Resp: 601796




Ion	Ratio	Lower	Upper
188	100		
94	9.7	6.7	10.1
80	10.2	7.5	11.3

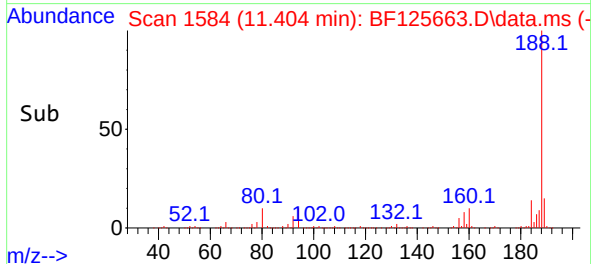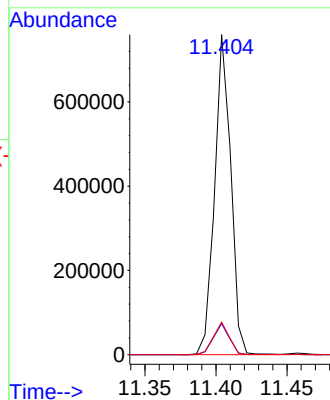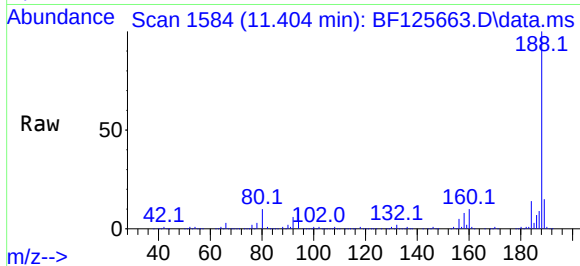


#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.039 min Scan# 2032
Delta R.T. -0.006 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36

Tgt Ion:240 Resp: 393019

Ion	Ratio	Lower	Upper
240	100		
120	12.6	10.8	16.2
236	24.7	21.6	32.4


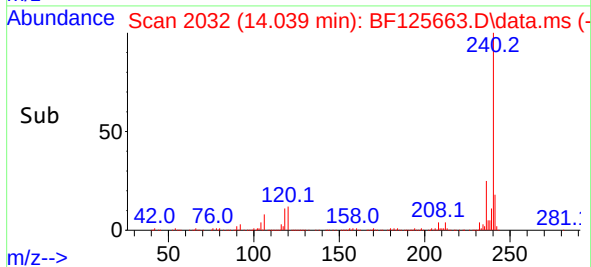
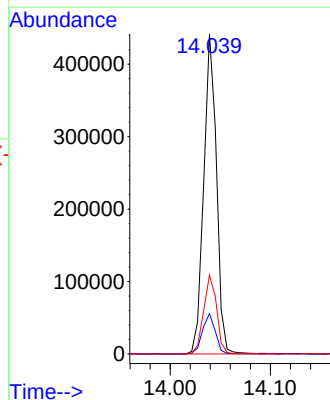
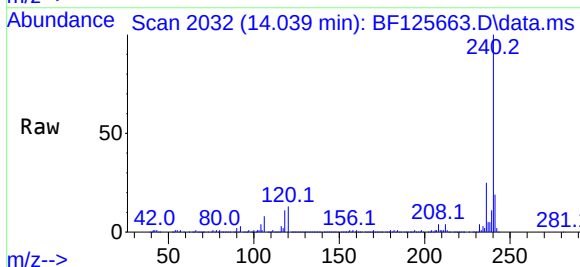


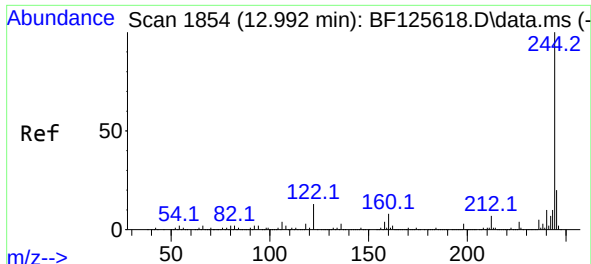

#79
Terphenyl-d14
Concen: 54.617 ng
RT: 12.992 min Scan# 1854
Delta R.T. 0.000 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36

Instrument :
BNA_F
ClientSampled :
TS-1

Tgt Ion:244 Resp: 1239515
Ion Ratio Lower Upper
244 100
212 6.5 5.9 8.9
122 10.3 9.0 13.4

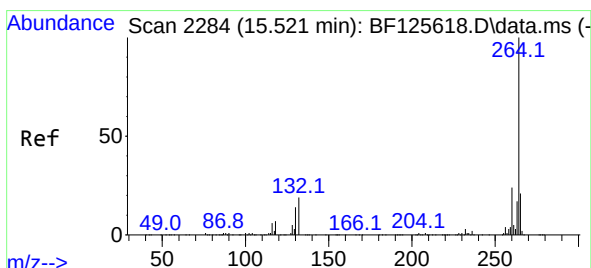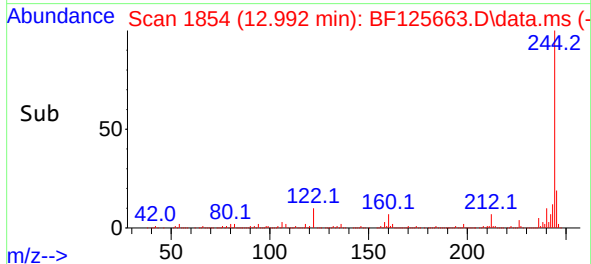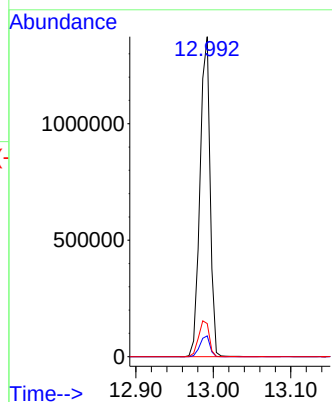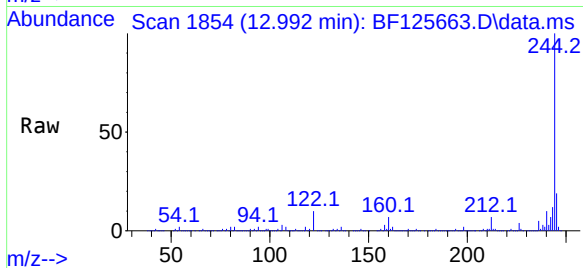

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.515 min Scan# 2283
Delta R.T. -0.006 min
Lab File: BF125663.D
Acq: 25 Sep 2021 18:36

Tgt Ion:264 Resp: 393266
Ion Ratio Lower Upper
264 100
260 23.0 19.6 29.4
265 20.7 17.2 25.8

