
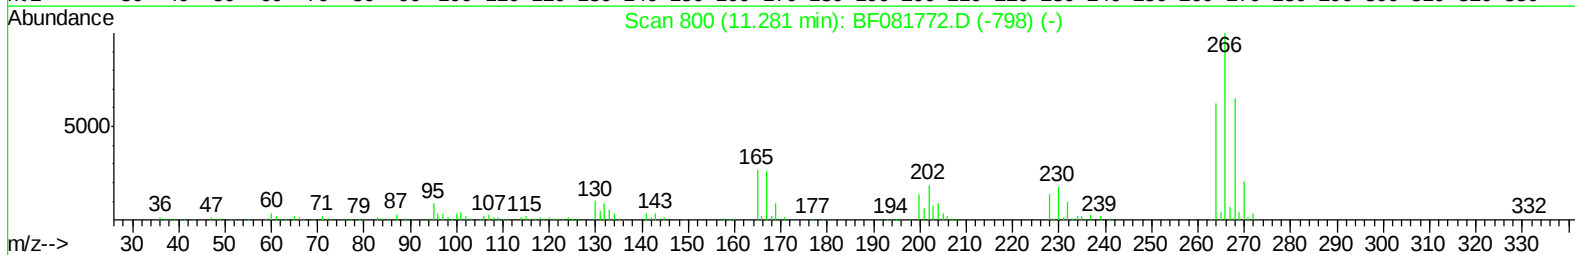
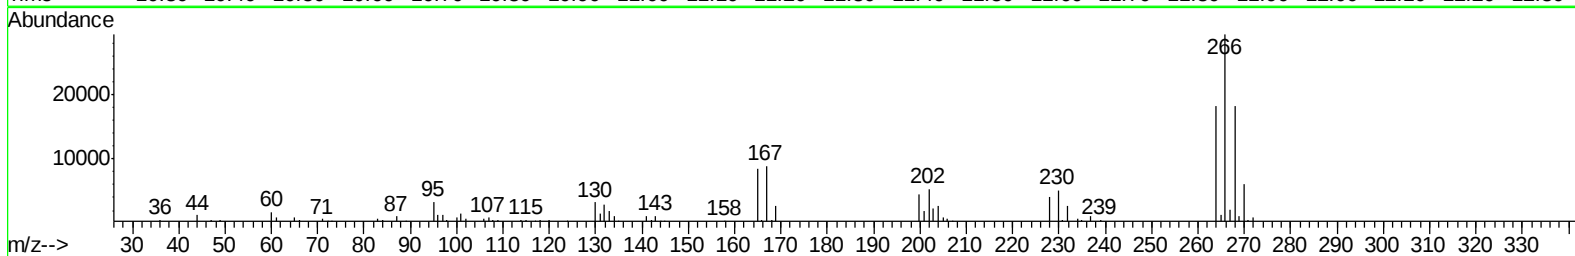


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092615\
Data File : BF081820.D
Acq On : 26 Sep 2015 9:32
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 08:48:33 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 06:02:49 2015
Response via : Initial Calibration

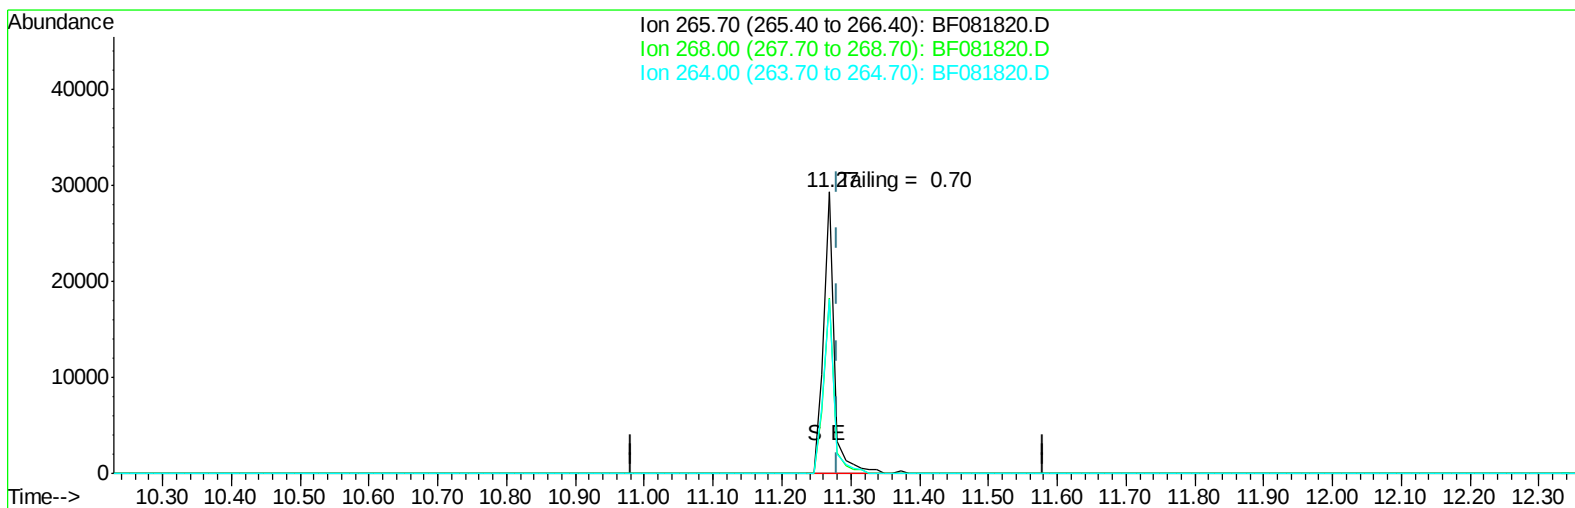

TIC: BF081820.D

(69) Pentachlorophenol (C)




11.269min (-0.011) 20979.79ng

response 31884

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	62.10
264.00	62.70	61.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092615\
Data File : BF081820.D
Acq On : 26 Sep 2015 9:32
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 08:48:33 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 25 06:02:49 2015
Response via : Initial Calibration

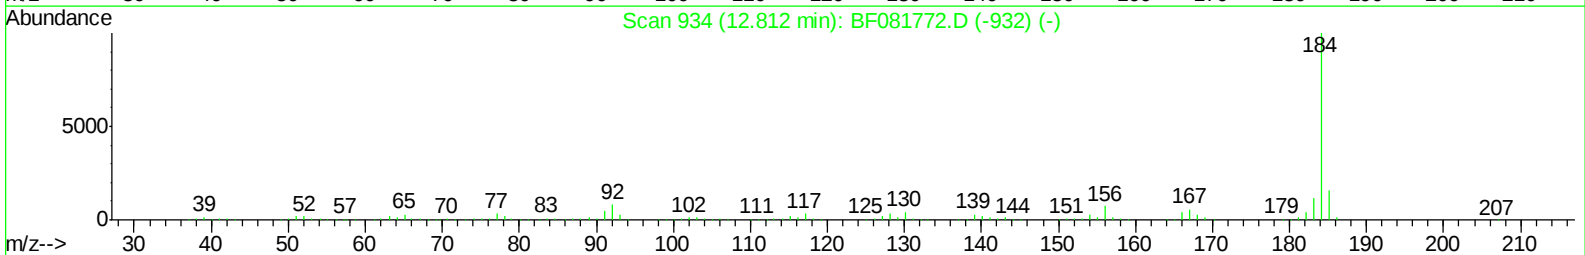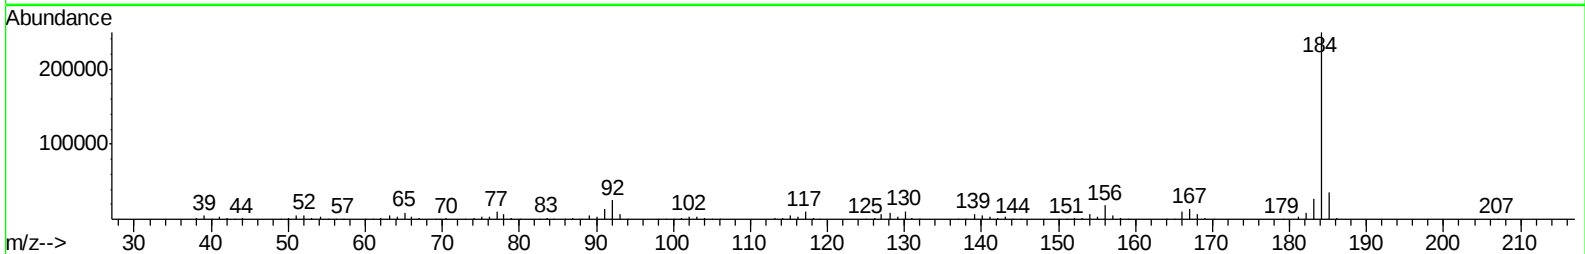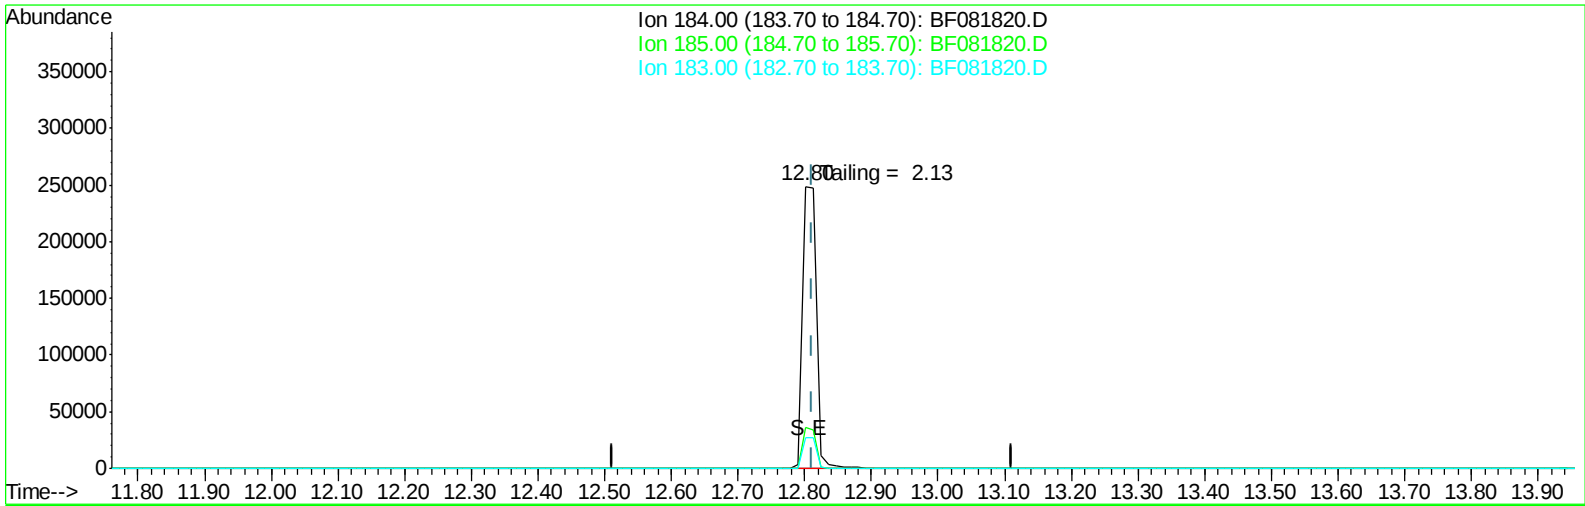

TIC: BF081820.D

(76) Benzidine

12.801min (-0.011) 0.00ng

response 357254

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.43
183.00	9.50	11.14
0.00	0.00	0.00