


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092615\
 Data File : BF081820.D
 Acq On : 26 Sep 2015 9:32
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 25 06:02:49 2015

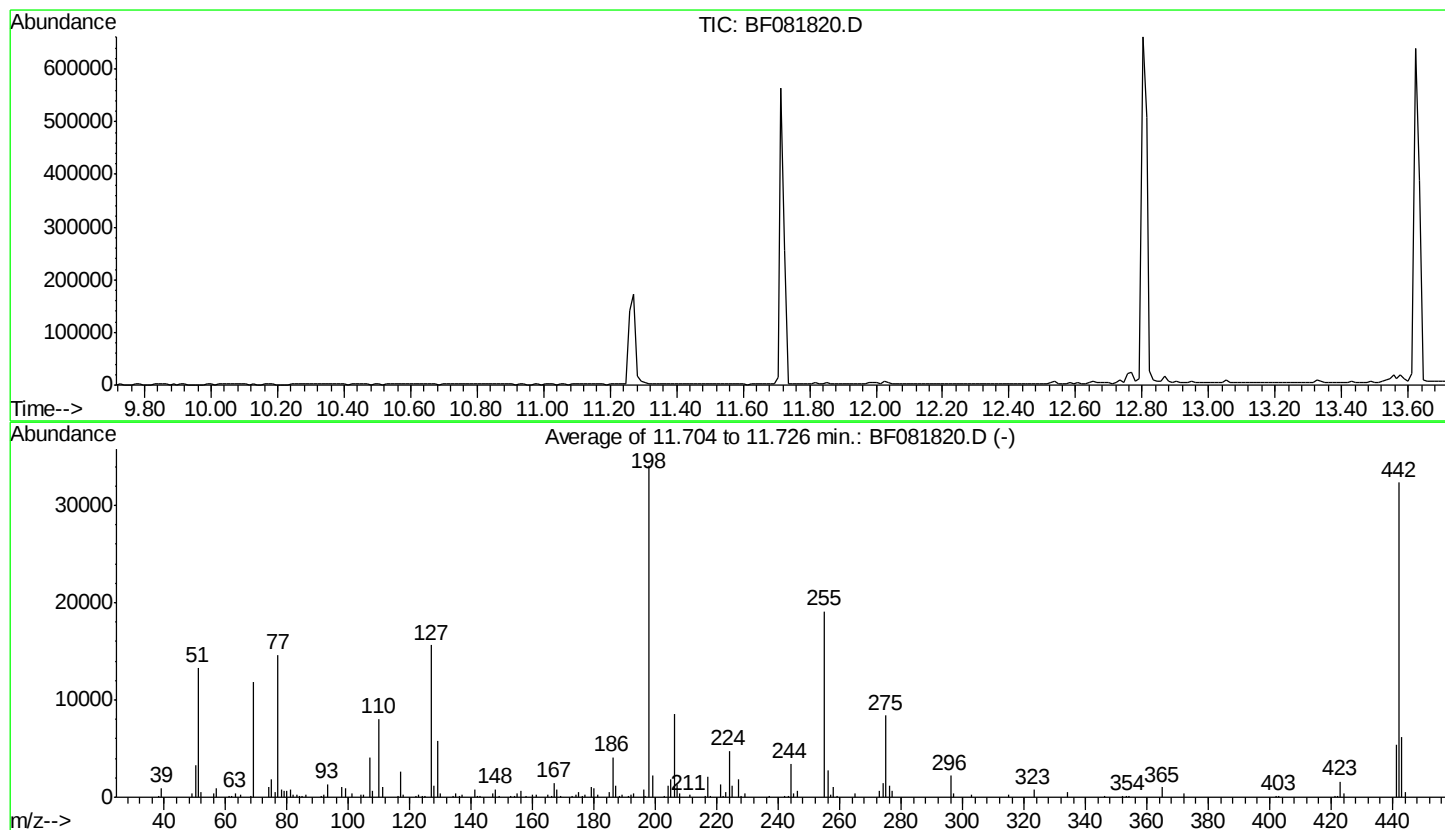

AutoFind: Scans 837, 838, 839; Background Corrected with Scan 834

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	13285	PASS
68	69	0.00	2	1.2	143	PASS
69	198	0.00	100	34.8	11842	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.8	15618	PASS
197	198	0.00	2	0.5	156	PASS
198	198	100	100	100.0	34070	PASS
199	198	5	9	6.7	2276	PASS
275	198	10	60	24.6	8395	PASS
365	198	1	100	3.0	1013	PASS
441	442	0.01	24	16.5	5338	PASS
442	198	50	100	94.9	32349	PASS
443	442	15	24	19.2	6216	PASS