

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092616\
 Data File : BF090247.D
 Acq On : 27 Sep 2016 4:52
 Operator : UM/SJ
 Sample : H4927-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TRACK-D-GRID-19B

Quant Time: Sep 27 05:17:40 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 26 15:58:38 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.48	152	141112	20.00	ng	0.00
21) Naphthalene-d8	7.77	136	539040	20.00	ng	0.00
38) Acenaphthene-d10	9.51	164	286410	20.00	ng	0.00
63) Phenanthrene-d10	10.97	188	386318	20.00	ng	-0.01
75) Chrysene-d12	13.59	240	284814	20.00	ng	-0.01
86) Perylene-d12	14.90	264	245916	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.05	112	958550	110.72	ng	0.02
7) Phenol-d6	6.14	99	1036125	96.91	ng	0.00
23) Nitrobenzene-d5	7.05	82	676358	72.74	ng	-0.01
41) 2,4,6-Tribromophenol	10.30	330	287335	116.94	ng	0.00
44) 2-Fluorobiphenyl	8.84	172	1197092	82.05	ng	-0.01
78) Terphenyl-d14	12.56	244	911195	81.22	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.05	70	77337	12.31	ng	Qvalue # 81
31) Naphthalene	7.78	128	162902	6.35	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092616\
Data File : BF090247.D
Acq On : 27 Sep 2016 4:52
Operator : UM/SJ
Sample : H4927-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TRACK-D-GRID-19B

Quant Time: Sep 27 05:17:40 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 26 15:58:38 2016
Response via : Initial Calibration

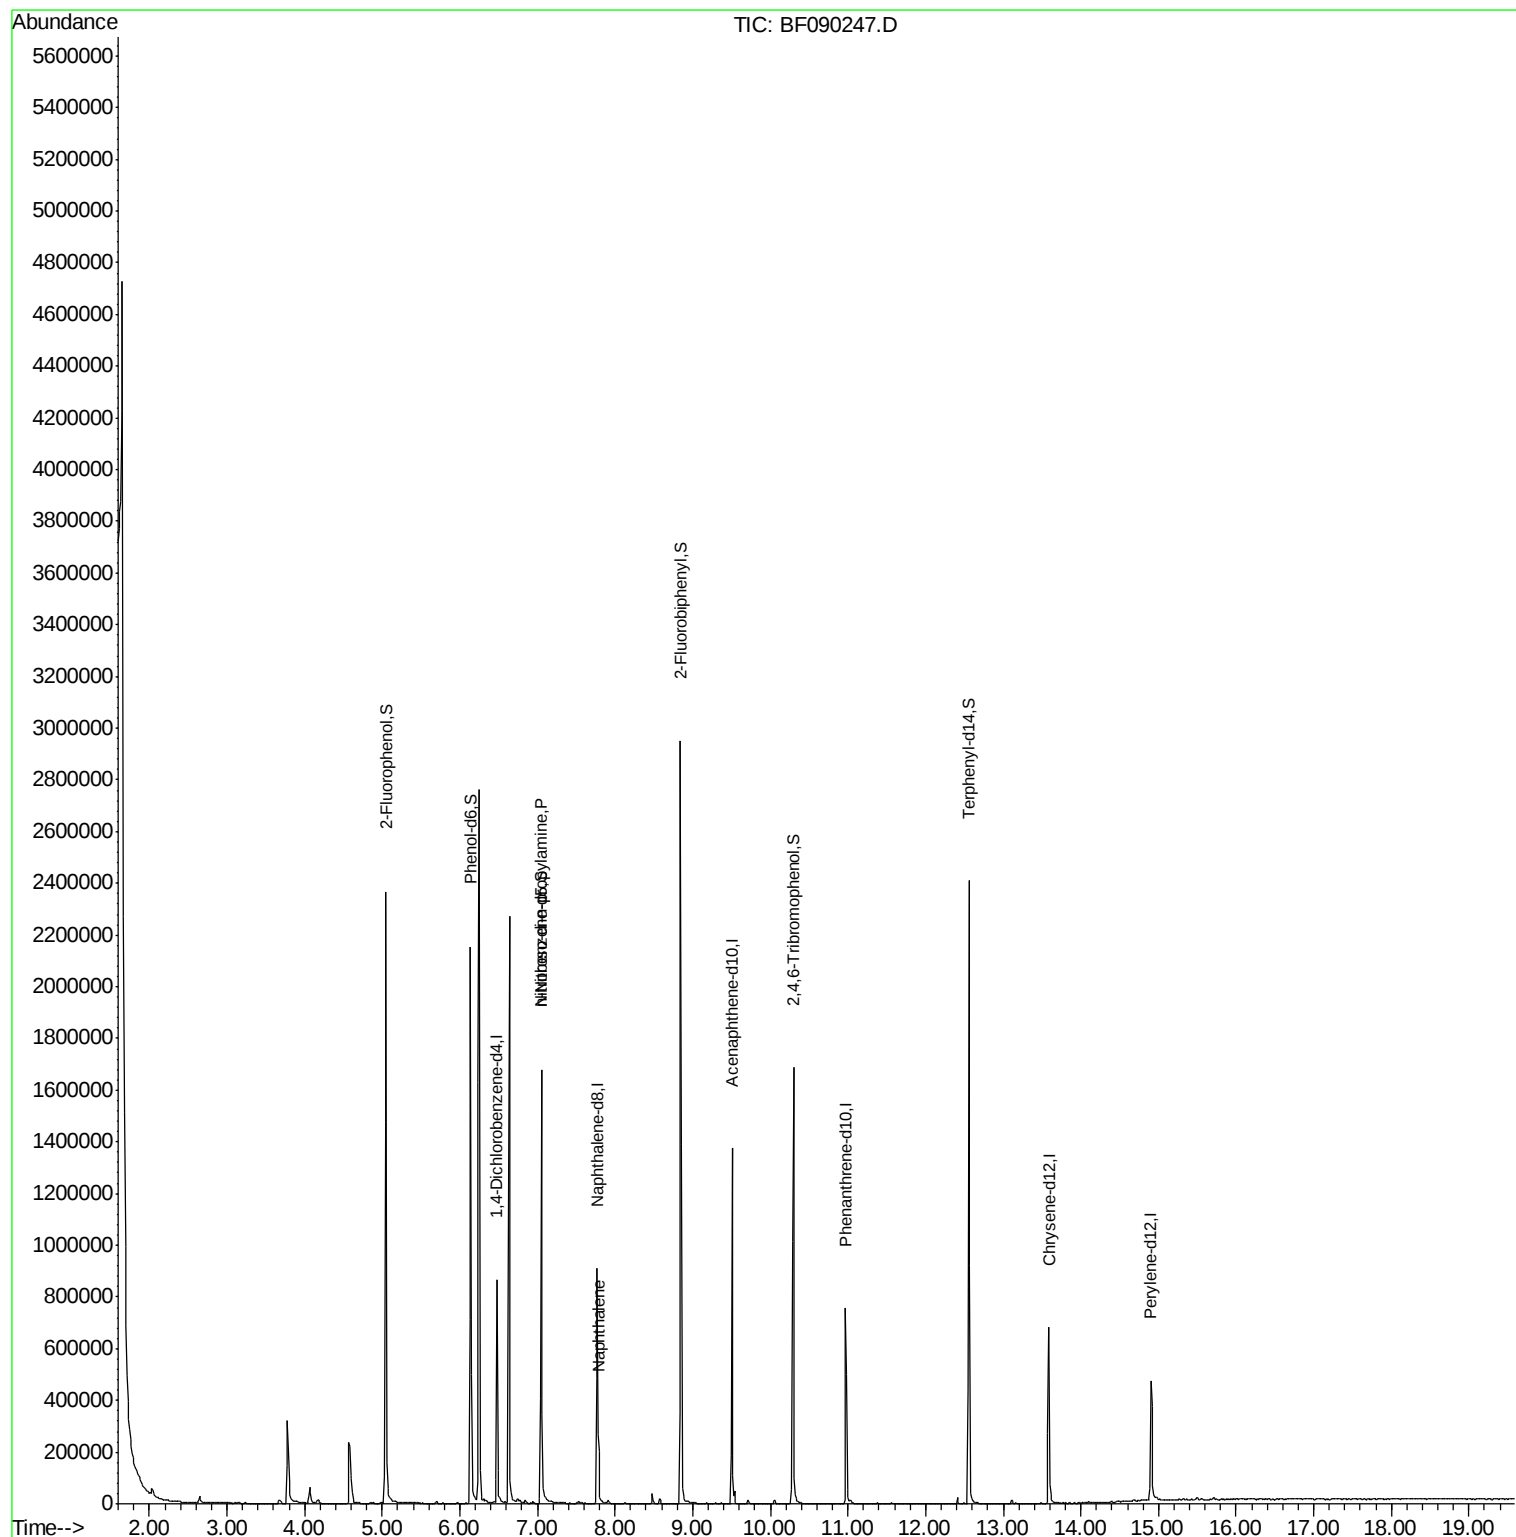

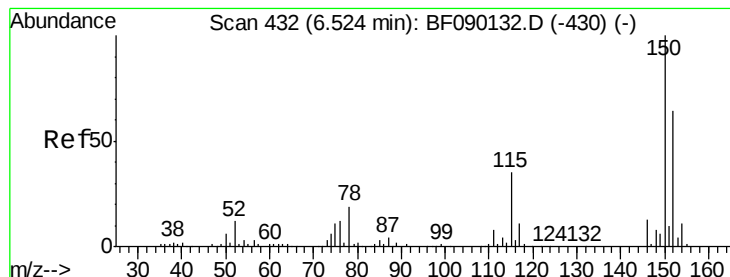

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.48 min Scan# 428

Delta R.T. -0.00 min

Lab File: BF090247.D

Acq: 27 Sep 2016 4:52

Instrument :

BNA_F

ClientSampleId :

TRACK-D-GRID-19B


Tgt Ion:152 Resp: 141112

Ion Ratio Lower Upper

152 100

150 153.5 128.9 193.3




115 61.6 55.5 83.3



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

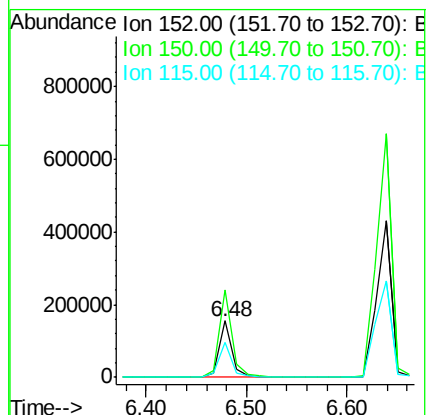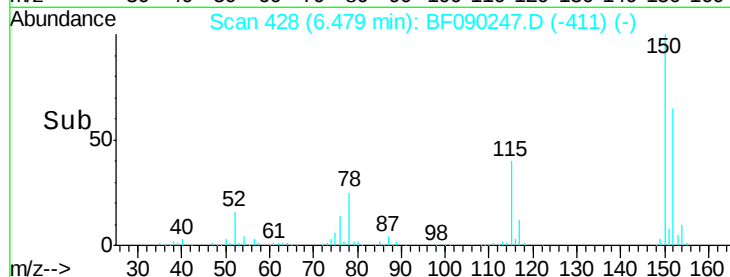

#5

2-Fluorophenol

Concen: 110.72 ng

RT: 5.05 min Scan# 303

Delta R.T. 0.02 min

Lab File: BF090247.D

Acq: 27 Sep 2016 4:52


Tgt Ion:112 Resp: 958550

Ion Ratio Lower Upper

112 100

64 49.5 39.8 59.6



63 24.0 18.9 28.3





Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

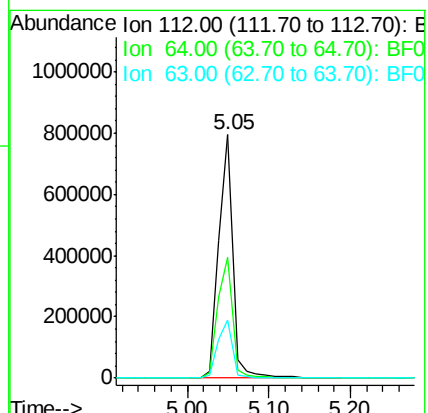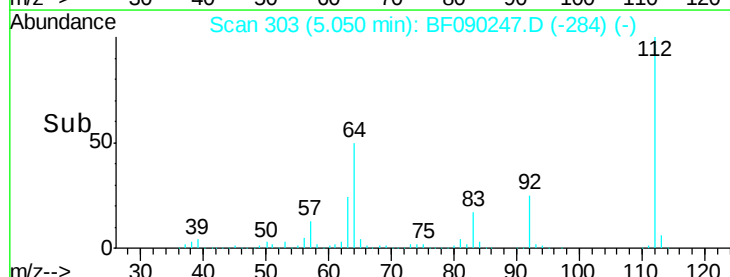

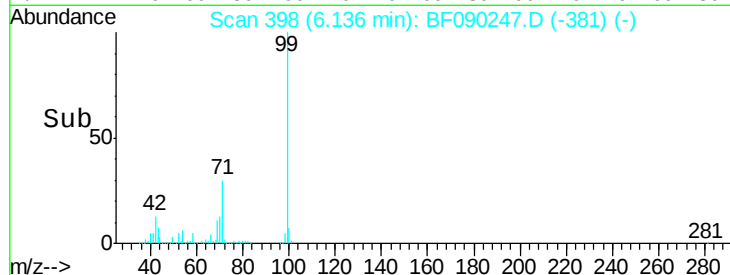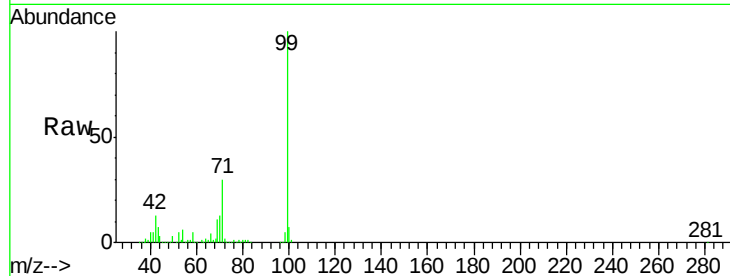

#7

Phenol-d6

Concen: 96.91 ng

RT: 6.14 min Scan# 398

Delta R.T. -0.00 min

Lab File: BF090247.D

Acq: 27 Sep 2016 4:52

Instrument :

BNA_F

ClientSampleId :

TRACK-D-GRID-19B





Tgt Ion: 99 Resp: 1036125

Ion Ratio Lower Upper

99 100

42 13.3 10.6 15.8

71 30.0 23.0 34.6

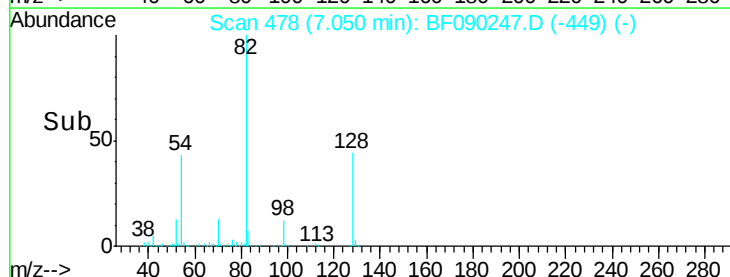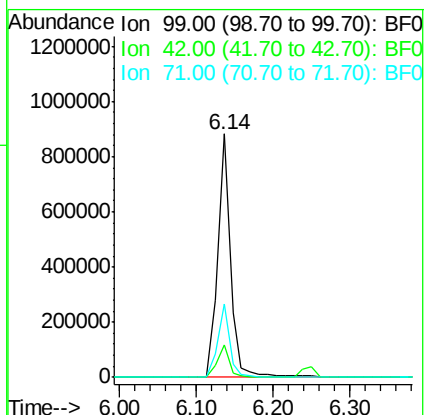

#19

n-Nitroso-di-n-propylamine

Concen: 12.31 ng

RT: 7.05 min Scan# 478

Delta R.T. 0.14 min

Lab File: BF090247.D

Acq: 27 Sep 2016 4:52

Tgt Ion: 70 Resp: 77337


Ion Ratio Lower Upper


70 100

42 38.7 35.1 52.7

101 0.0 7.5 11.3#

130 2.2 16.6 25.0#

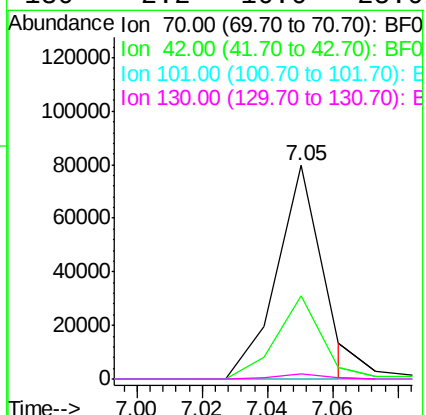


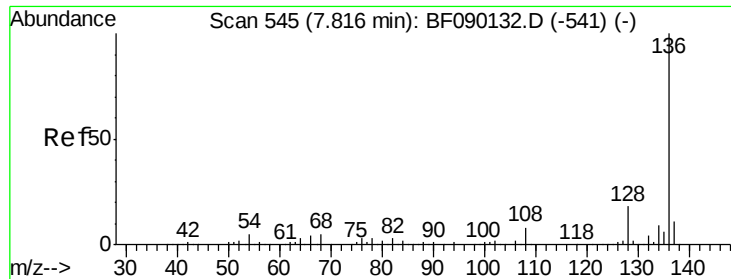




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.77 min Scan# 541
Delta R.T. -0.00 min
Lab File: BF090247.D
Acq: 27 Sep 2016 4:52

Instrument :
BNA_F
ClientSampleId :
TRACK-D-GRID-19B

Tgt Ion:	136	Resp:	539040
Ion	Ratio	Lower	Upper
136	100		
137	10.6	9.0	13.4
54	5.3	6.4	9.6#
68	5.3	6.3	9.5#

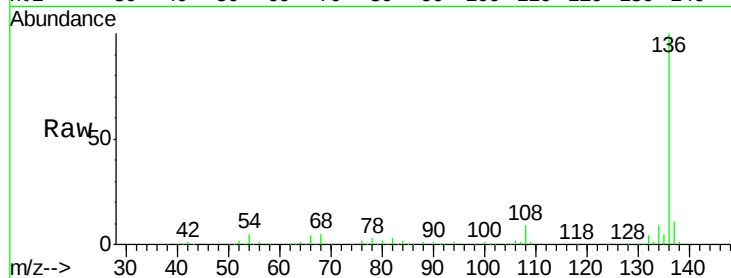


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

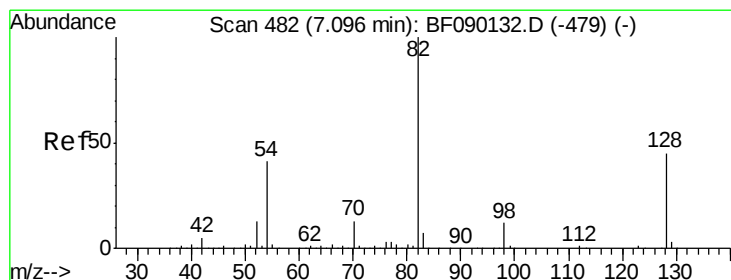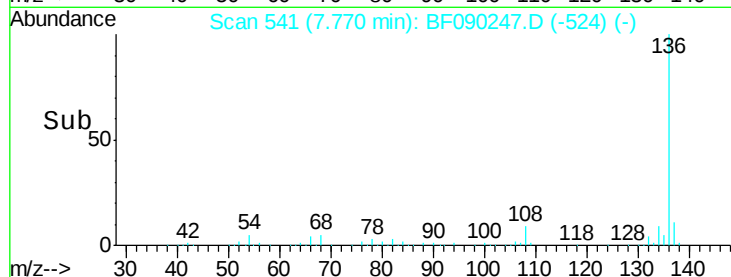
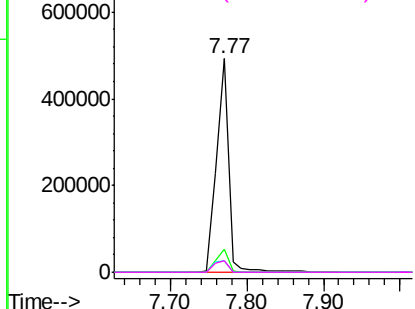



#23
Nitrobenzene-d5
Concen: 72.74 ng
RT: 7.05 min Scan# 478
Delta R.T. -0.01 min
Lab File: BF090247.D
Acq: 27 Sep 2016 4:52

Tgt Ion:	82	Resp:	676358
Ion	Ratio	Lower	Upper
82	100		
128	43.5	37.5	56.3
54	42.6	31.9	47.9

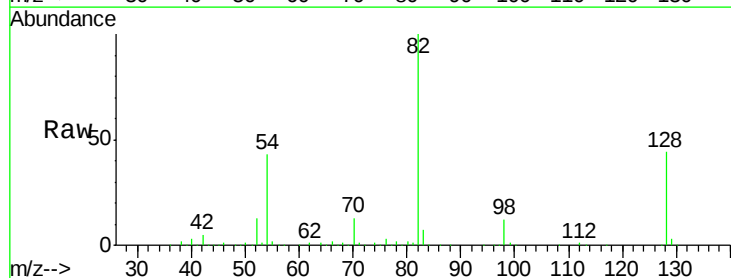

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

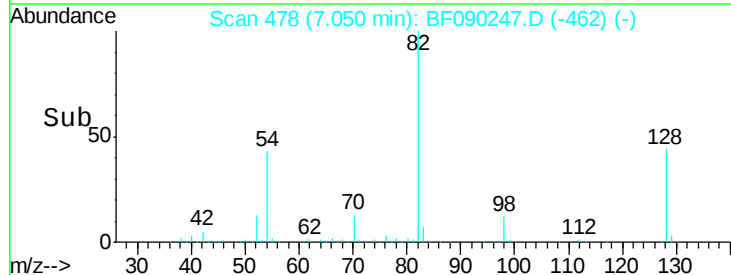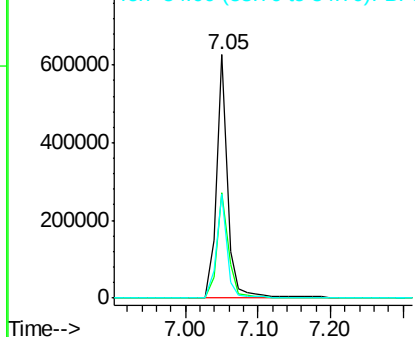

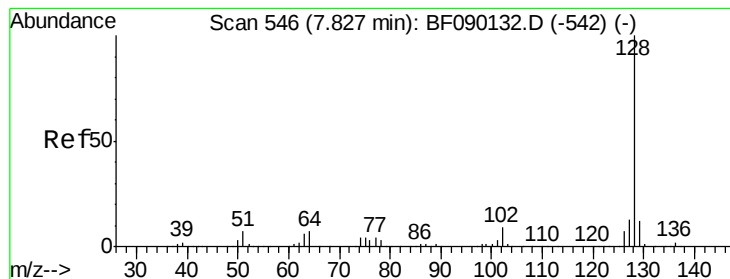

#31

Naphthalene

Concen: 6.35 ng

RT: 7.78 min Scan# 542

Delta R.T. -0.01 min

Lab File: BF090247.D

Acq: 27 Sep 2016 4:52

Instrument :

BNA_F

ClientSampleId :

TRACK-D-GRID-19B


Tgt Ion:128 Resp: 162902

Ion Ratio Lower Upper

128 100

129 11.8 9.3 13.9




127 12.7 10.8 16.2



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

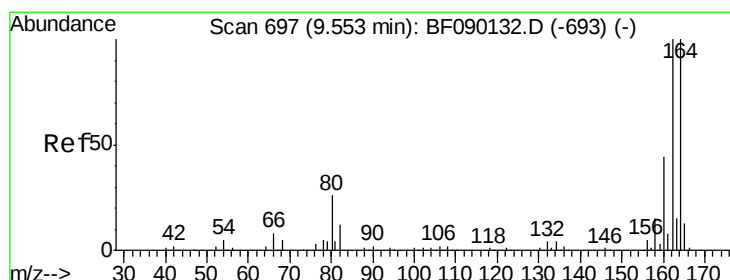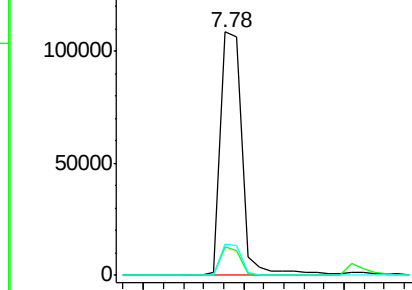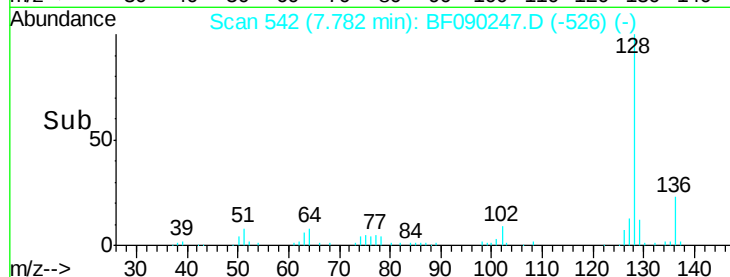

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.51 min Scan# 693

Delta R.T. -0.00 min

Lab File: BF090247.D

Acq: 27 Sep 2016 4:52


Tgt Ion:164 Resp: 286410

Ion Ratio Lower Upper

164 100

162 100.6 81.4 122.2



160 44.0 36.6 54.8




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

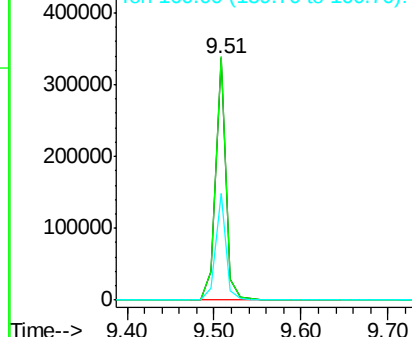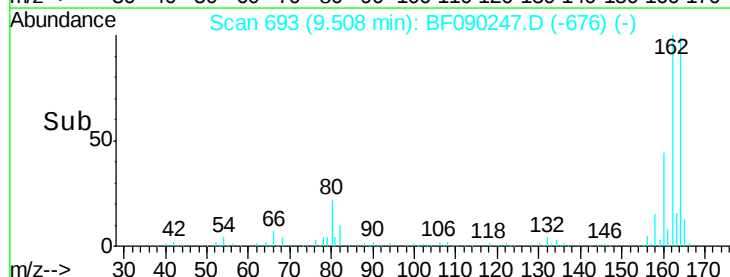


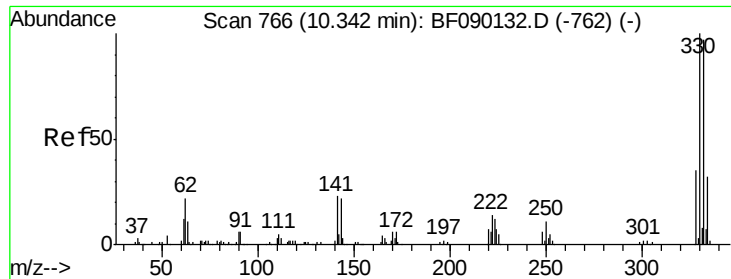




#41
 2,4,6-Tribromophenol
 Concen: 116.94 ng
 RT: 10.30 min Scan# 762
 Delta R.T. -0.00 min
 Lab File: BF090247.D
 Acq: 27 Sep 2016 4:52

Instrument :
 BNA_F
 ClientSampleId :
 TRACK-D-GRID-19B

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.4	78.1	117.1
141	32.3	23.9	35.9

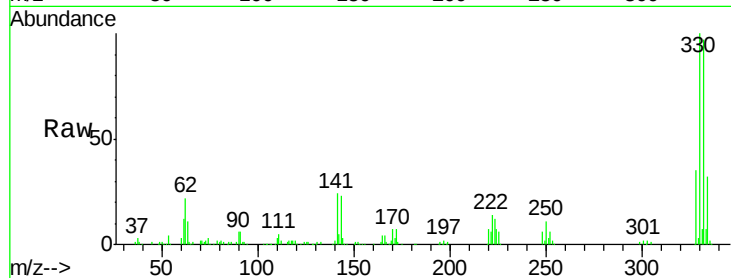


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

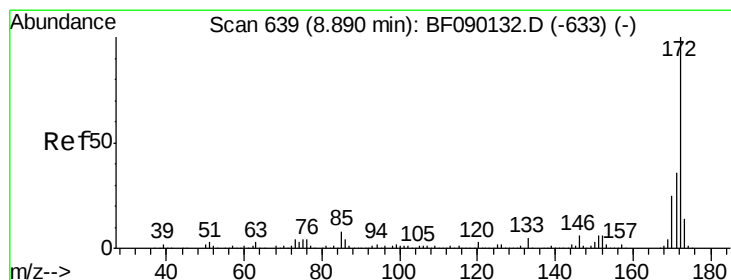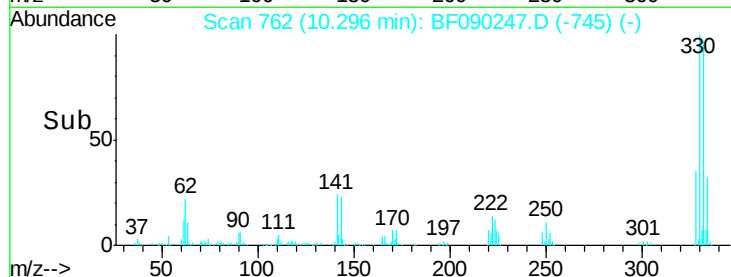
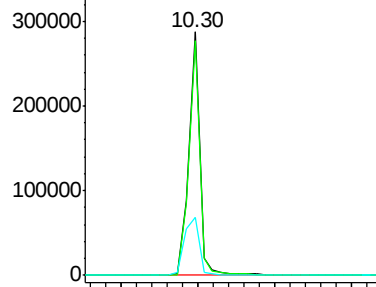



#44
 2-Fluorobiphenyl
 Concen: 82.05 ng
 RT: 8.84 min Scan# 635
 Delta R.T. -0.01 min
 Lab File: BF090247.D
 Acq: 27 Sep 2016 4:52

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.2	43.8
170	24.6	19.8	29.8

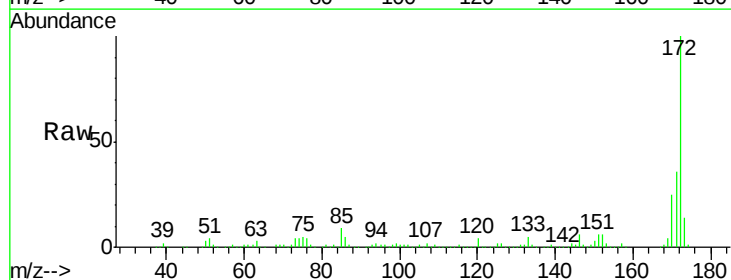

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

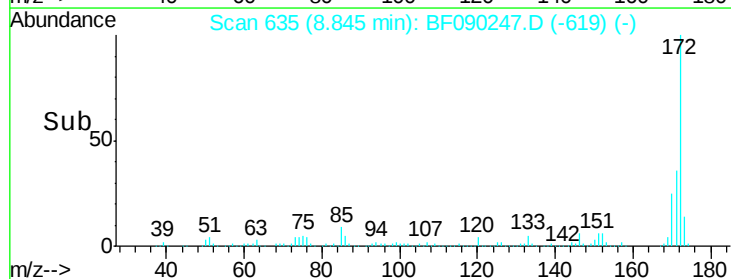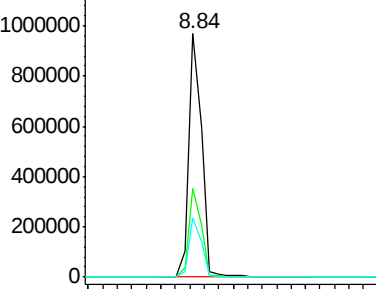


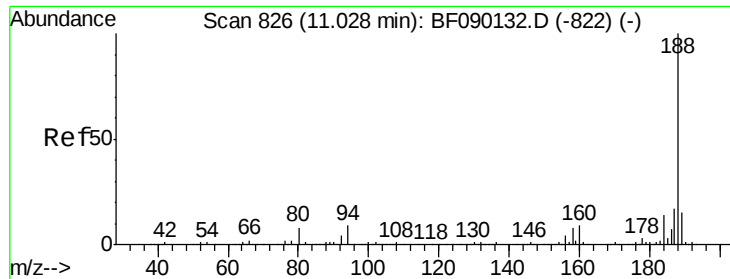




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 10.97 min Scan# 821
 Delta R.T. -0.01 min
 Lab File: BF090247.D
 Acq: 27 Sep 2016 4:52

Instrument :
 BNA_F
 ClientSampleId :
 TRACK-D-GRID-19B

Tgt Ion:188 Resp: 386318
 Ion Ratio Lower Upper
 188 100
 94 15.6 10.5 15.7
 80 16.8 11.2 16.8#




Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

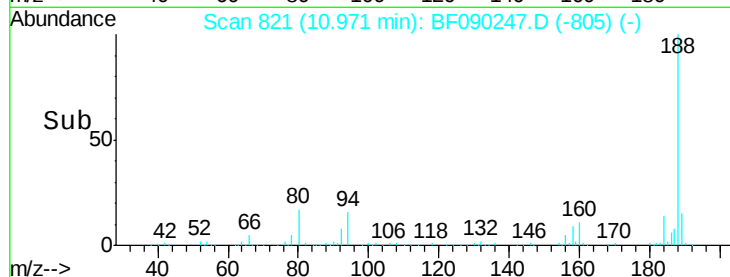
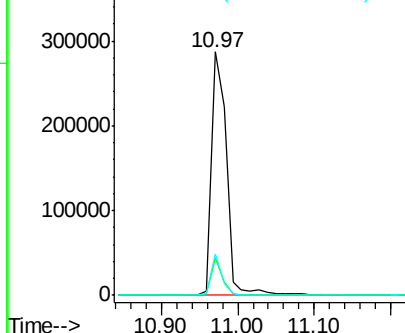



#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 13.59 min Scan# 1050
 Delta R.T. -0.01 min
 Lab File: BF090247.D
 Acq: 27 Sep 2016 4:52

Tgt Ion:240 Resp: 284814
 Ion Ratio Lower Upper
 240 100
 120 11.0 10.6 16.0
 236 25.9 21.6 32.4



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

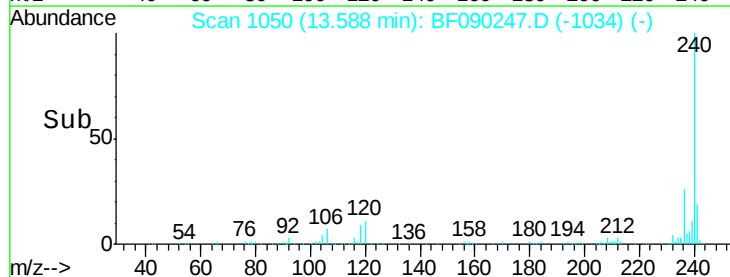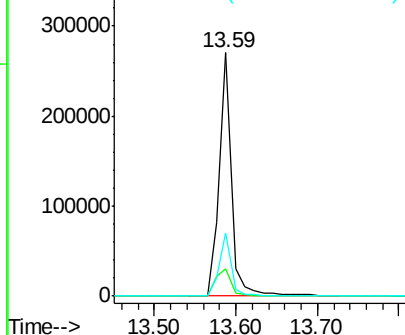

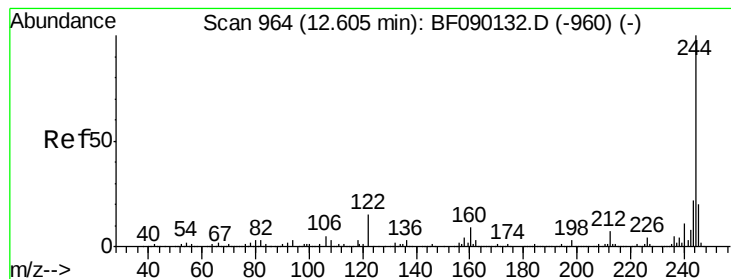

#78

Terphenyl-d14

Concen: 81.22 ng

RT: 12.56 min Scan# 960

Delta R.T. -0.00 min

Lab File: BF090247.D

Acq: 27 Sep 2016 4:52

Instrument :

BNA_F

ClientSampleId :

TRACK-D-GRID-19B


Tgt Ion:244 Resp: 911195

Ion Ratio Lower Upper

244 100

212 7.3 5.8 8.8




122 16.2 9.4 14.0#

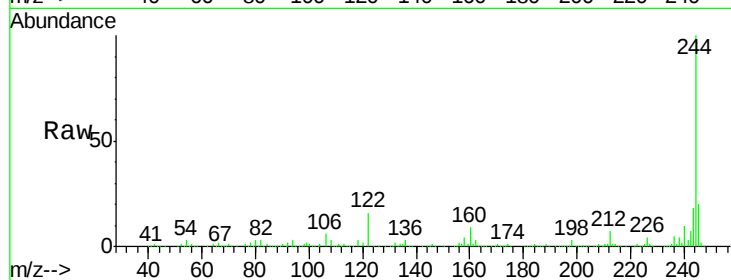

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

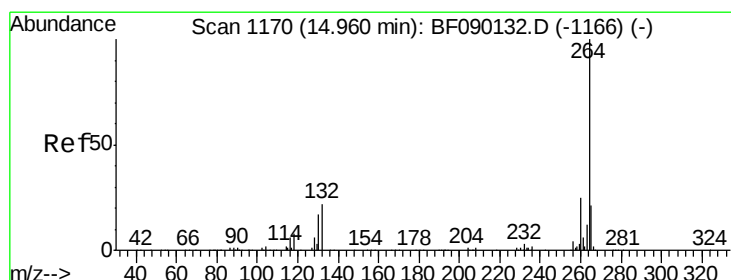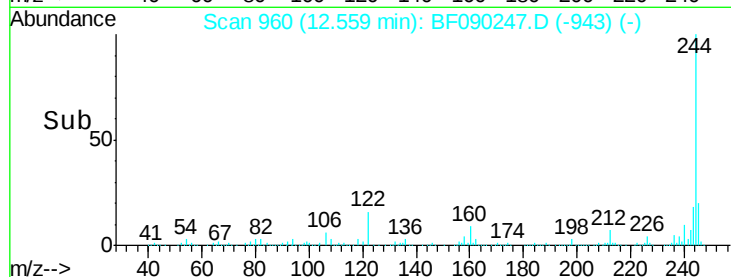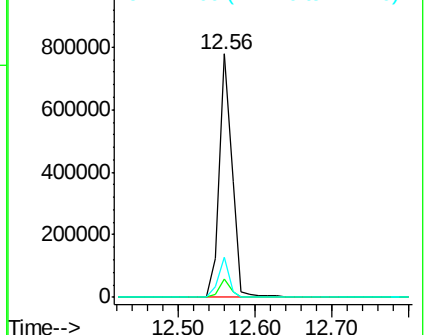

#86

Perylene-d12

Concen: 20.00 ng

RT: 14.90 min Scan# 1165

Delta R.T. -0.01 min

Lab File: BF090247.D

Acq: 27 Sep 2016 4:52


Tgt Ion:264 Resp: 245916

Ion Ratio Lower Upper

264 100

260 24.1 19.5 29.3

265 21.5 17.0 25.4

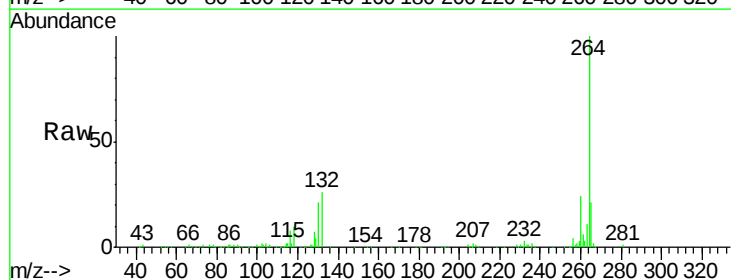

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

