
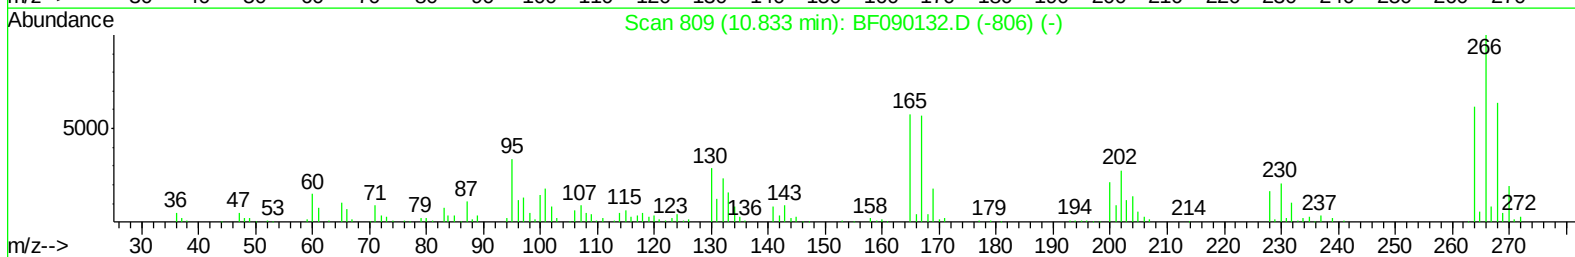
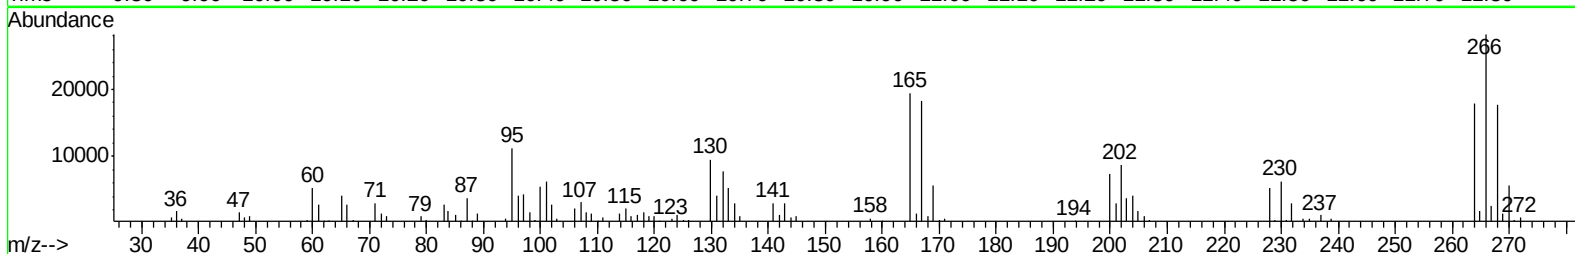


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092616\
Data File : BF090238.D
Acq On : 27 Sep 2016 00:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 04:08:02 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 26 15:58:38 2016
Response via : Initial Calibration

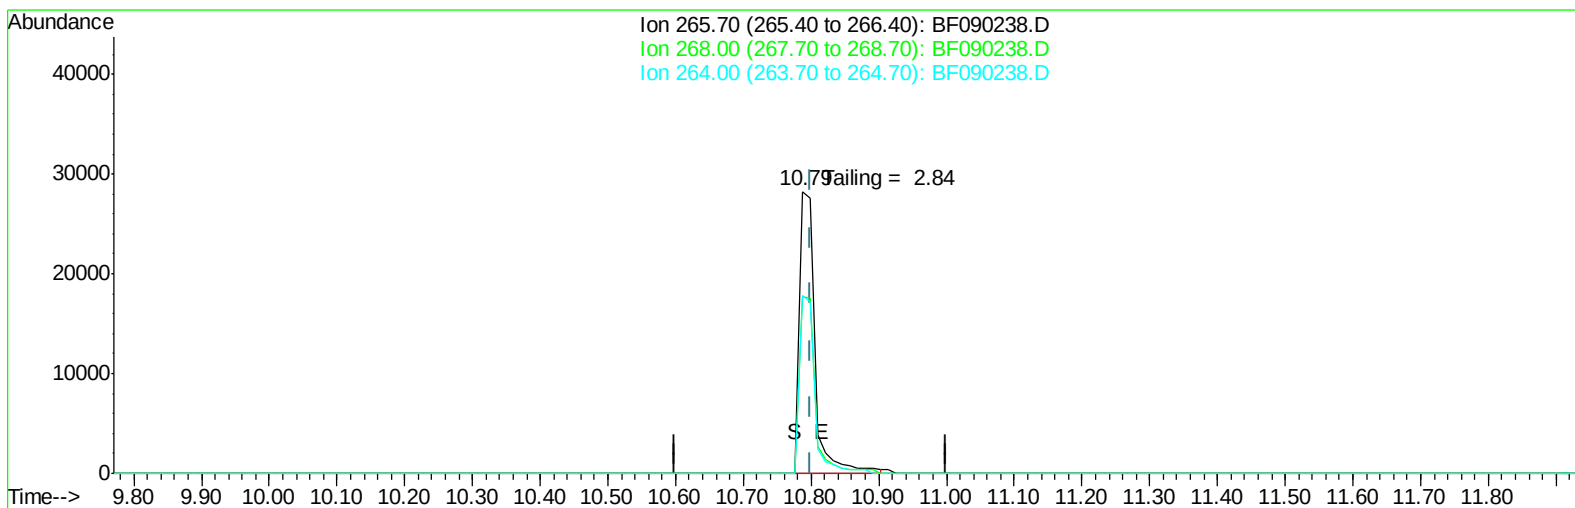

TIC: BF090238.D

(69) Pentachlorophenol (C)




10.788min (-0.011) 0.00ng

response 45789

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	62.57
264.00	62.90	63.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092616\
Data File : BF090238.D
Acq On : 27 Sep 2016 00:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 04:08:02 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 26 15:58:38 2016
Response via : Initial Calibration

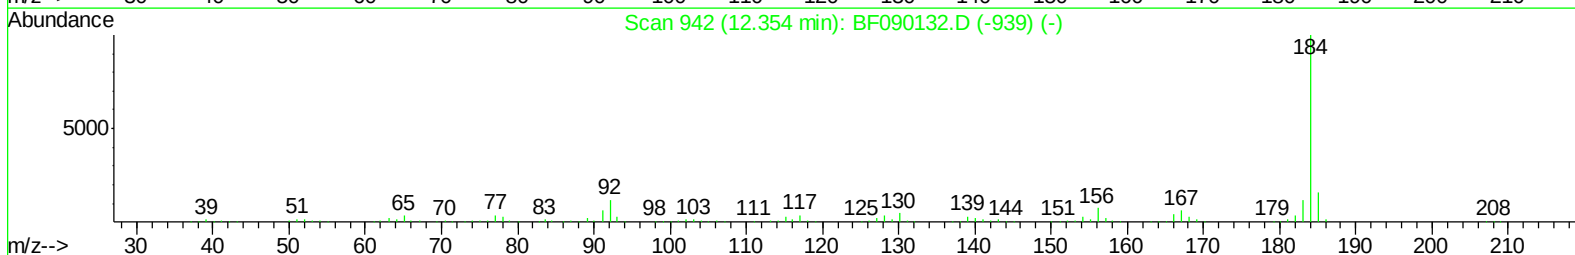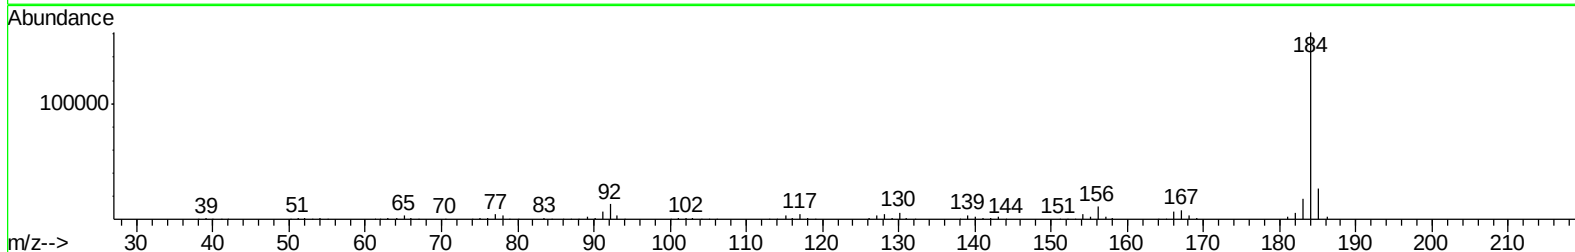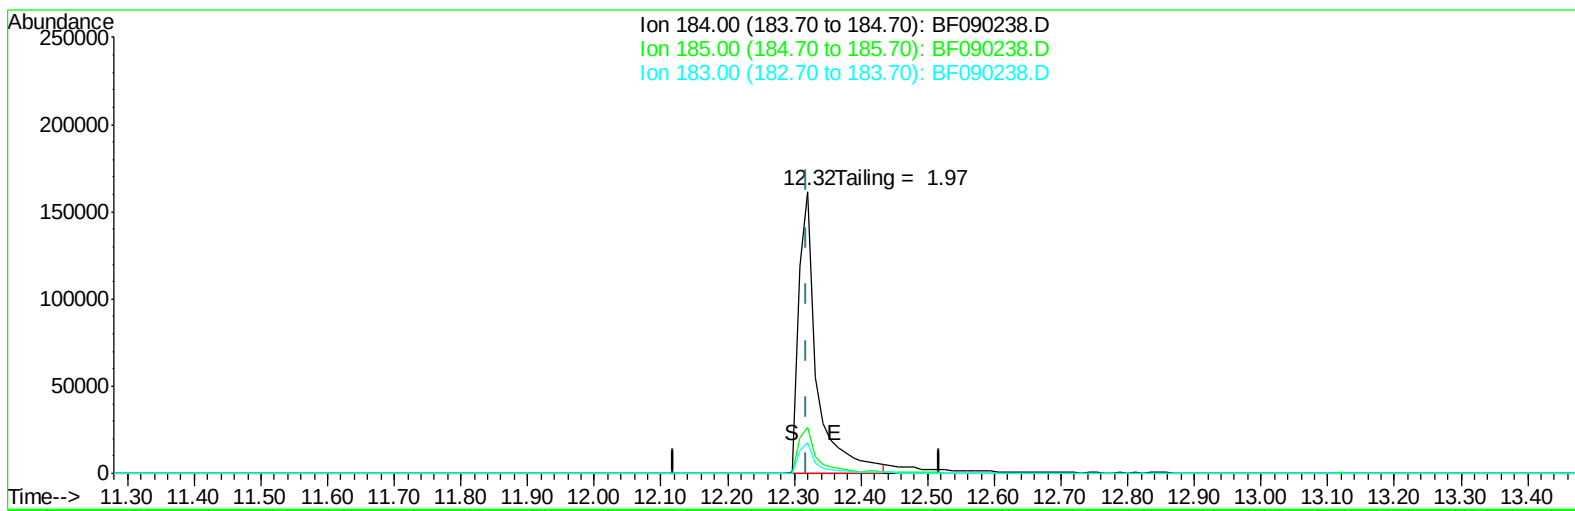

TIC: BF090238.D

(76) Benzidine

12.319min (-0.000) 0.00ng

response 314651

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	16.28
183.00	11.50	10.96
0.00	0.00	0.00