

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092616\
 Data File : BF090235.D
 Acq On : 26 Sep 2016 21:34
 Operator : UM/SJ
 Sample : H4946-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-05S-092216

Quant Time: Sep 27 01:35:20 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 26 15:58:38 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.48	152	135475	20.00	ng	0.00
21) Naphthalene-d8	7.77	136	538487	20.00	ng	0.00
38) Acenaphthene-d10	9.51	164	327499	20.00	ng	0.00
63) Phenanthrene-d10	10.97	188	490521	20.00	ng	-0.01
75) Chrysene-d12	13.59	240	443757	20.00	ng	-0.01
86) Perylene-d12	14.90	264	332902	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.03	112	339475	40.84	ng	0.00
7) Phenol-d6	6.12	99	291715	28.42	ng	-0.01
23) Nitrobenzene-d5	7.05	82	689695	74.25	ng	-0.01
41) 2,4,6-Tribromophenol	10.30	330	292936	104.26	ng	0.00
44) 2-Fluorobiphenyl	8.84	172	1115596	66.87	ng	-0.01
78) Terphenyl-d14	12.56	244	978351	55.97	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.24	163	53306	2.56	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092616\
Data File : BF090235.D
Acq On : 26 Sep 2016 21:34
Operator : UM/SJ
Sample : H4946-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-05S-092216

Quant Time: Sep 27 01:35:20 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 26 15:58:38 2016
Response via : Initial Calibration

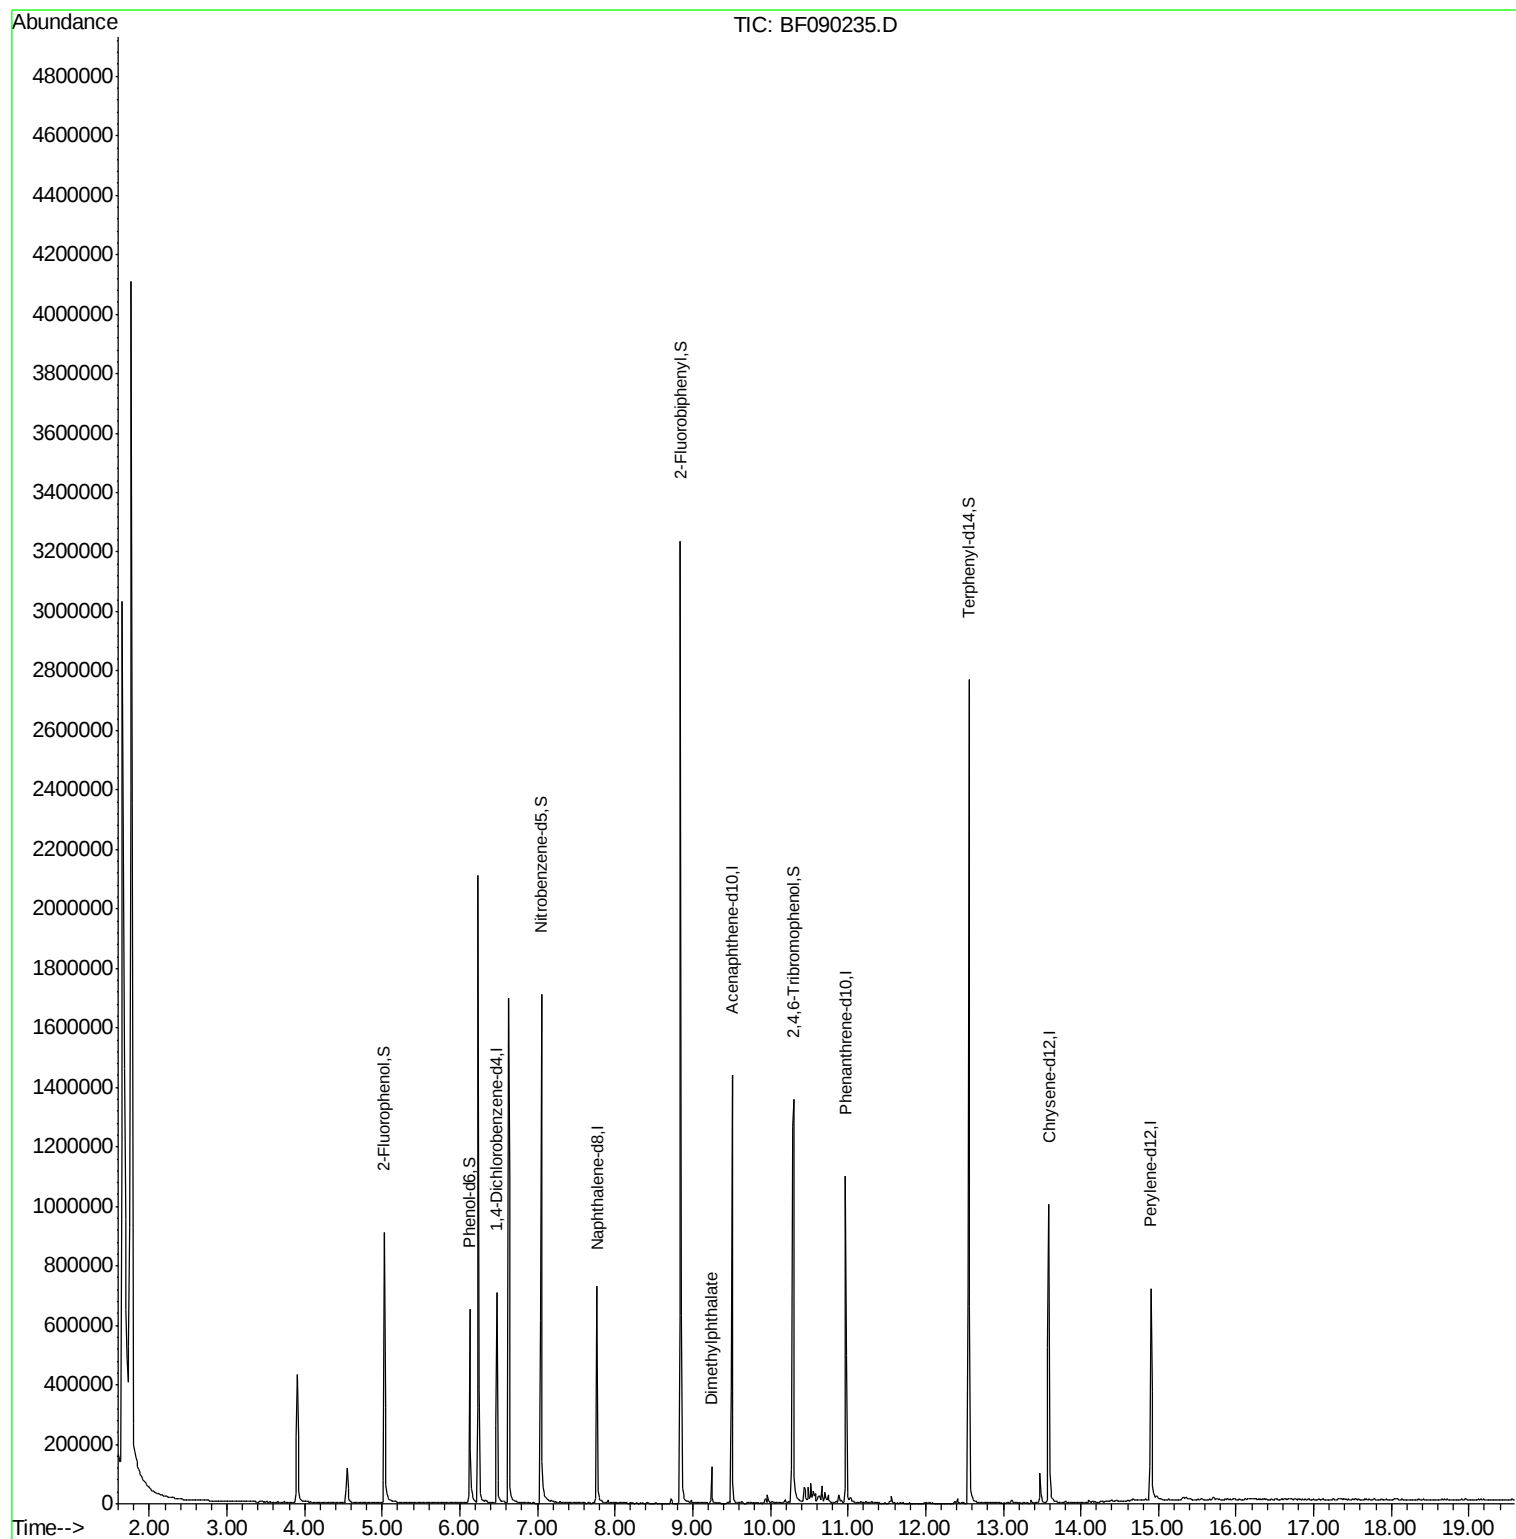

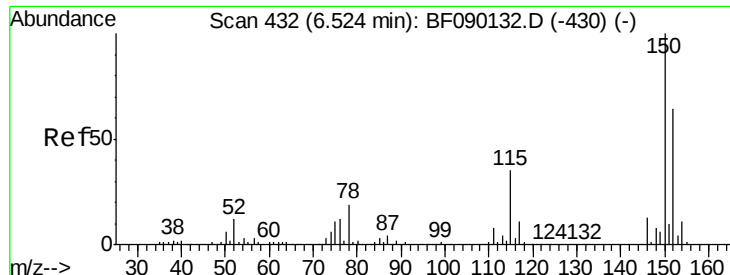

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.48 min Scan# 428

Delta R.T. -0.00 min

Lab File: BF090235.D

Acq: 26 Sep 2016 21:34

Instrument :

BNA_F

ClientSampleId :

MW-05S-092216


Tot Ion:152 Resp: 135475

Ion Ratio Lower Upper

152 100

150 153.9 128.9 193.3




115 56.0 55.5 83.3

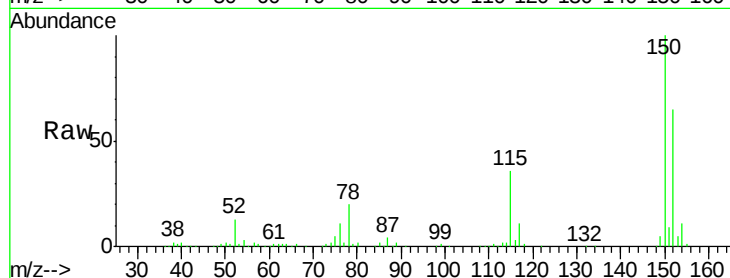

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

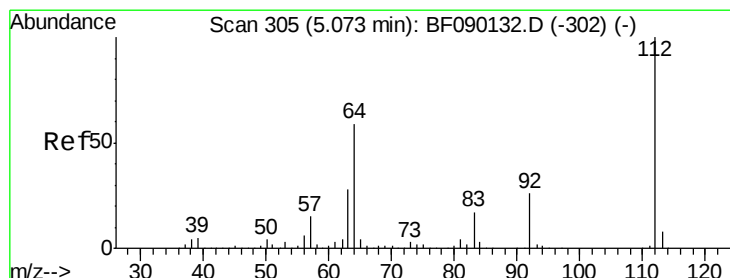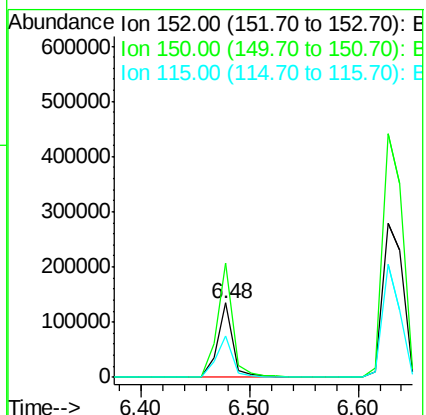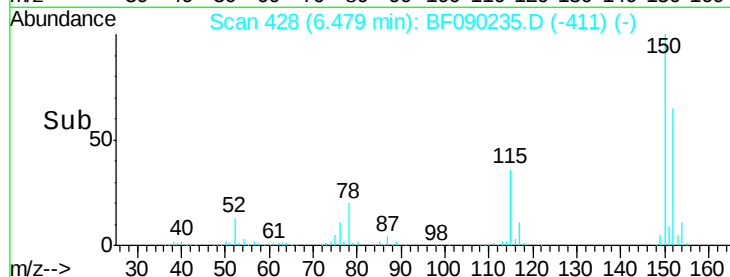

#5

2-Fluorophenol

Concen: 40.84 ng

RT: 5.03 min Scan# 301

Delta R.T. -0.00 min

Lab File: BF090235.D

Acq: 26 Sep 2016 21:34


Tgt Ion:112 Resp: 339475

Ion Ratio Lower Upper

112 100

64 54.5 39.8 59.6



63 26.0 18.9 28.3

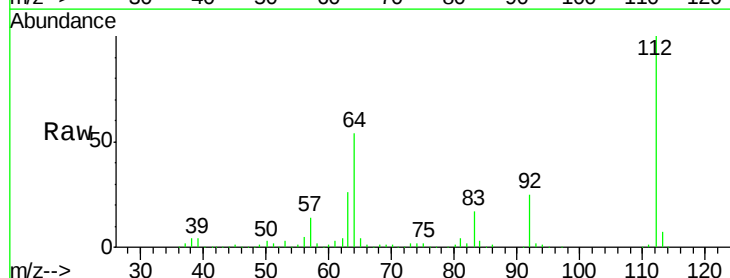


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

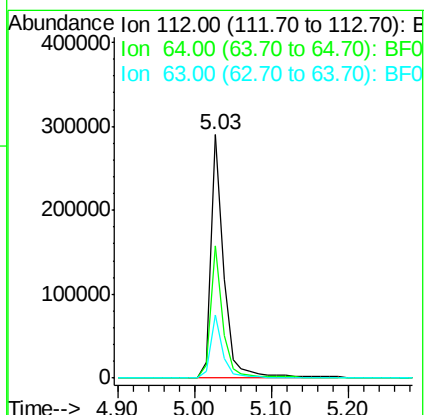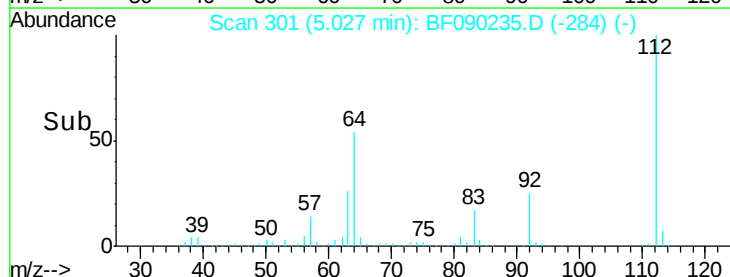

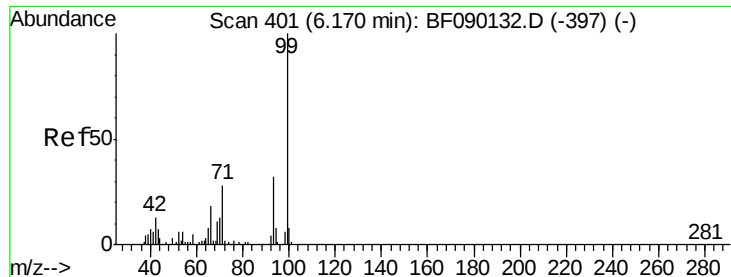

#7

Phenol-d6

Concen: 28.42 ng

RT: 6.12 min Scan# 397

Delta R.T. -0.01 min

Lab File: BF090235.D

Acq: 26 Sep 2016 21:34

Instrument :

BNA_F

ClientSampled :

MW-05S-092216


Tot Ion: 99 Resp: 291715

Ion Ratio Lower Upper

99 100

42 13.2 10.6 15.8




71 28.7 23.0 34.6

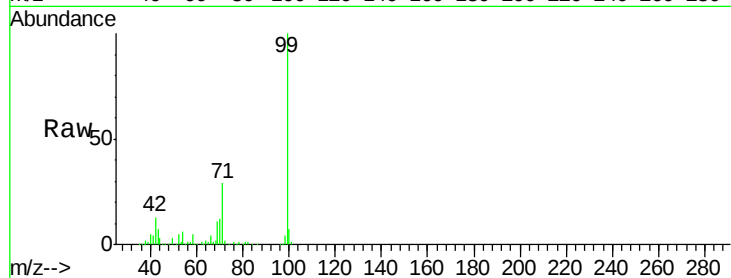

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

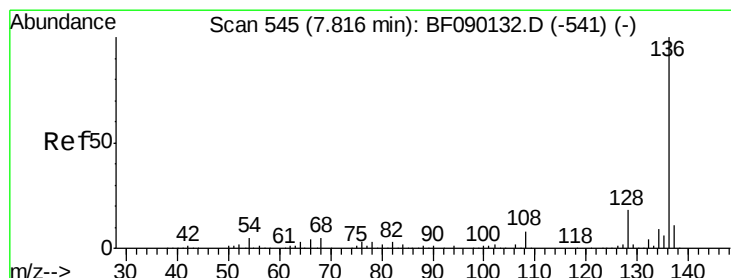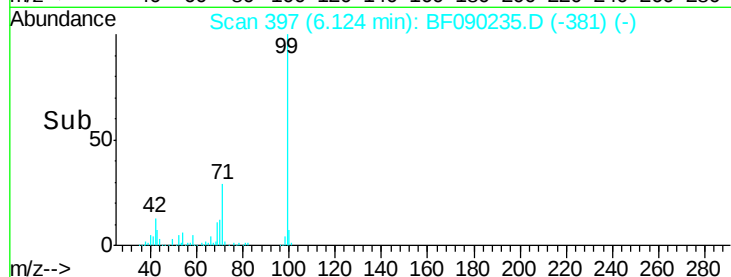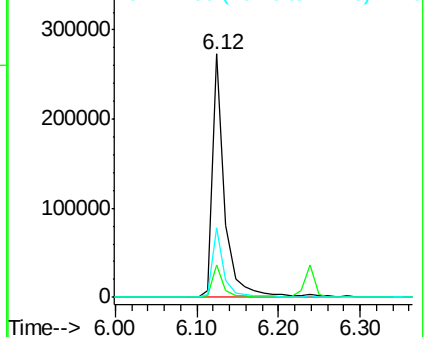

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.77 min Scan# 541

Delta R.T. -0.00 min

Lab File: BF090235.D

Acq: 26 Sep 2016 21:34

Tgt Ion: 136 Resp: 538487


Ion Ratio Lower Upper

136 100

137 10.7 9.0 13.4

54 4.8 6.4 9.6#

68 4.6 6.3 9.5#


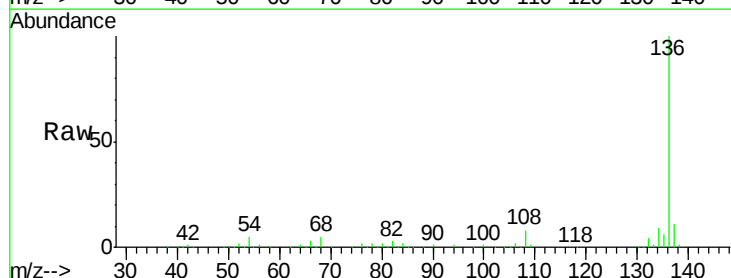



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



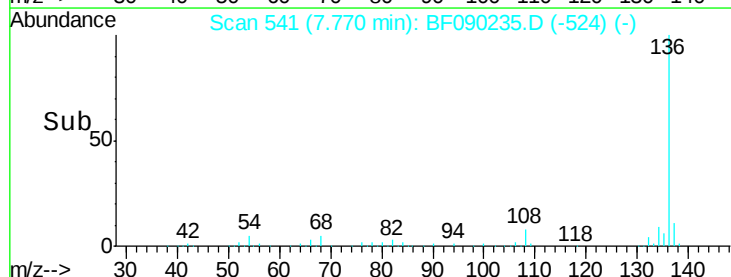
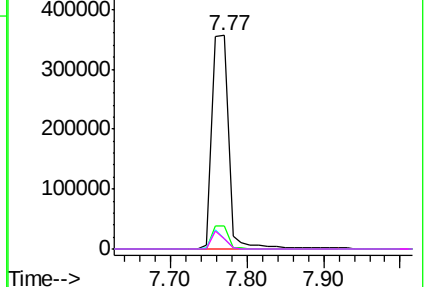


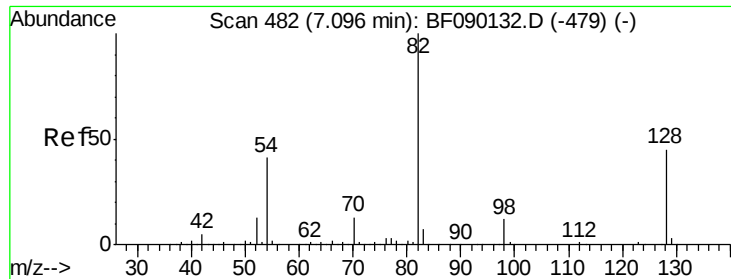

#23
 Nitrobenzene-d5
 Concen: 74.25 ng
 RT: 7.05 min Scan# 478
 Delta R.T. -0.01 min
 Lab File: BF090235.D
 Acq: 26 Sep 2016 21:34




Instrument :
 BNA_F
 ClientSampleId :
 MW-05S-092216


Tot Ion	82	Resp	689695
Ion Ratio	100	Lower	Upper
128	45.7	37.5	56.3
54	41.2	31.9	47.9

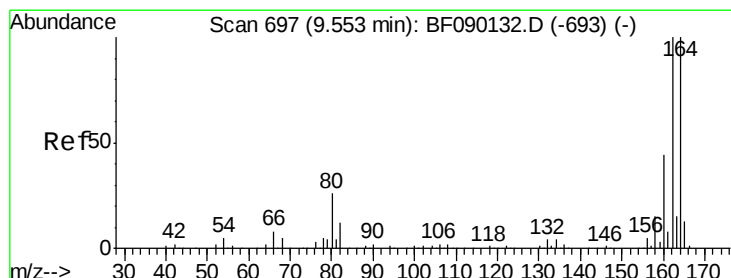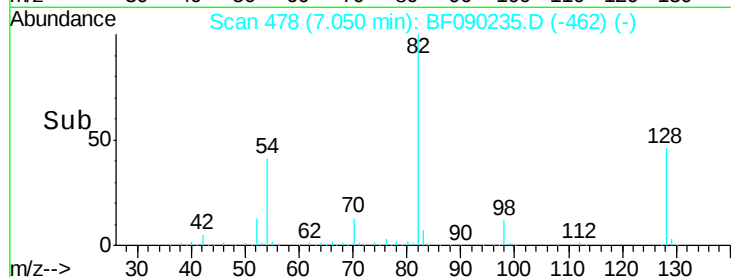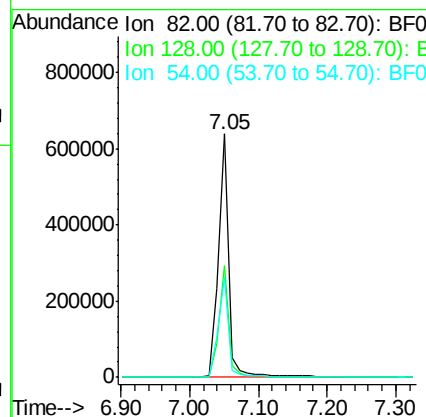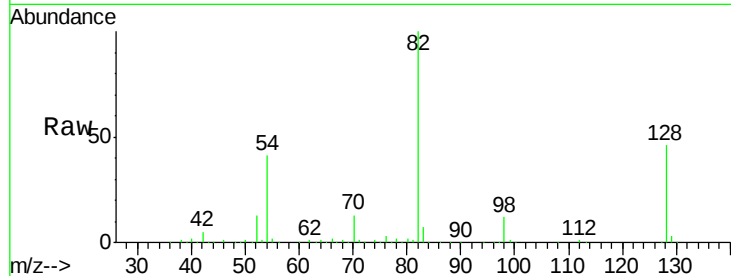

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.51 min Scan# 693
 Delta R.T. -0.00 min
 Lab File: BF090235.D
 Acq: 26 Sep 2016 21:34

Tgt Ion	164	Resp	327499
Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td>	100	Lower	Upper
162	98.1	81.4	122.2
160	42.9	36.6	54.8


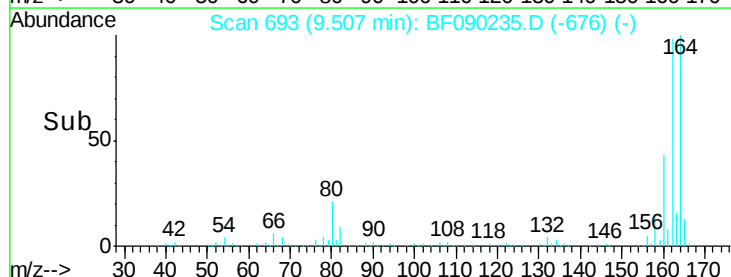
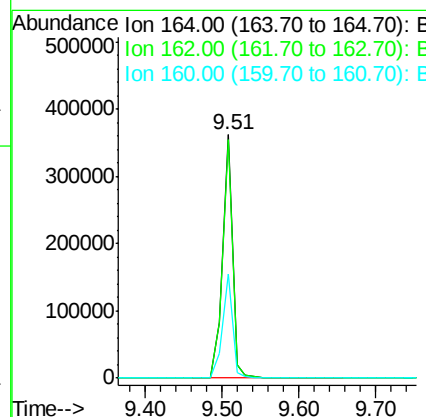
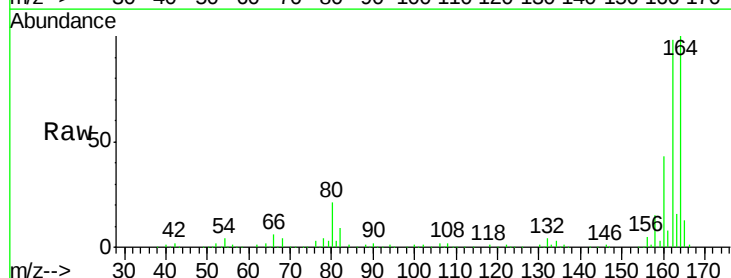


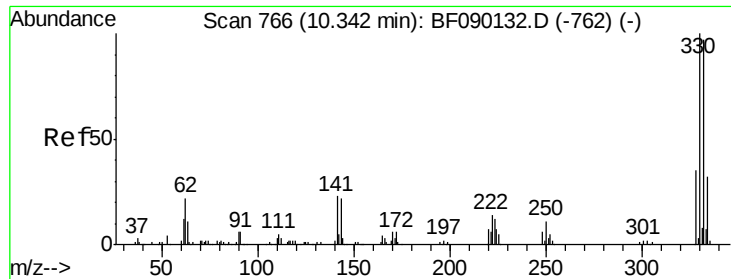

#41
 2,4,6-Tribromophenol
 Concen: 104.26 ng
 RT: 10.30 min Scan# 762
 Delta R.T. -0.00 min
 Lab File: BF090235.D
 Acq: 26 Sep 2016 21:34




Instrument :
 BNA_F
 ClientSampleId :
 MW-05S-092216


Tot Ion:330 Resp: 292936
 Ion Ratio Lower Upper
 330 100
 332 96.2 78.1 117.1
 141 30.1 23.9 35.9

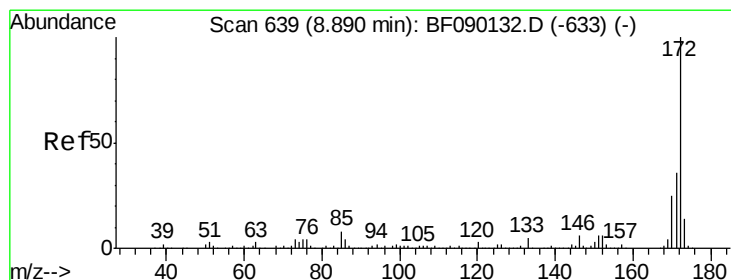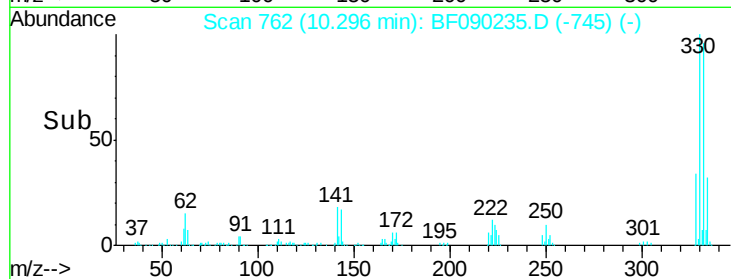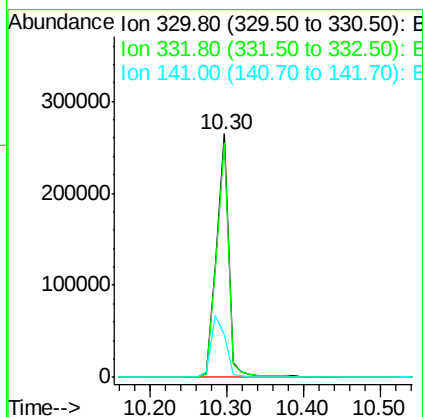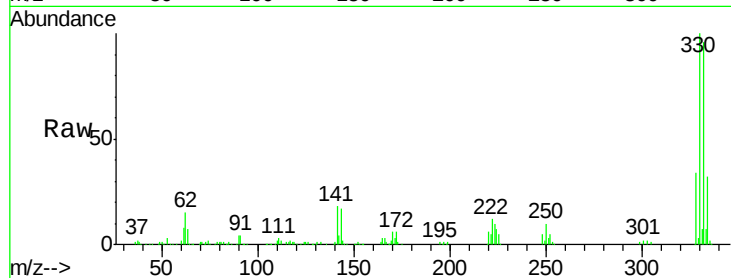

#44
 2-Fluorobiphenyl
 Concen: 66.87 ng
 RT: 8.84 min Scan# 635
 Delta R.T. -0.01 min
 Lab File: BF090235.D
 Acq: 26 Sep 2016 21:34

Tgt Ion:172 Resp: 1115596
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.2 43.8
 170 24.6 19.8 29.8

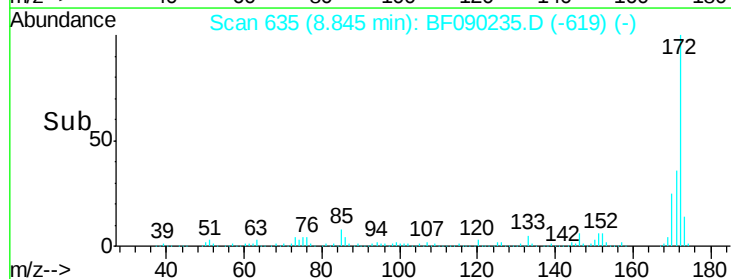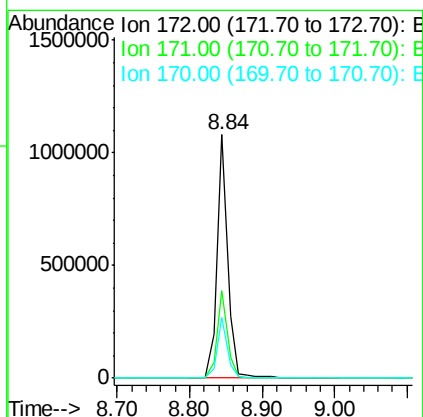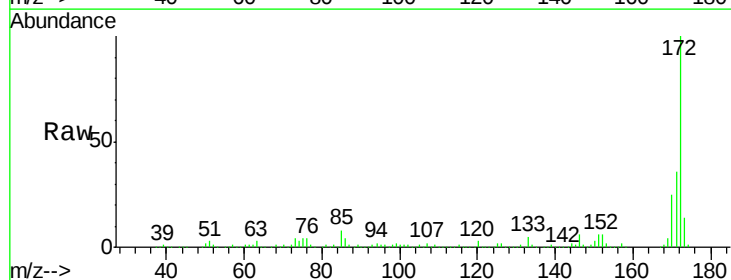


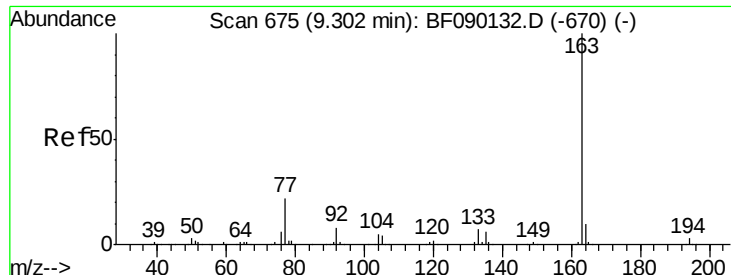




#49
Dimethylphthalate
Concen: 2.56 ng
RT: 9.24 min Scan# 670
Delta R.T. -0.02 min
Lab File: BF090235.D
Acq: 26 Sep 2016 21:34

Instrument :
BNA_F
ClientSampleId :
MW-05S-092216

Tot Ion:163 Resp: 53306
Ion Ratio Lower Upper
163 100
194 3.2 2.8 4.2
164 10.5 8.1 12.1

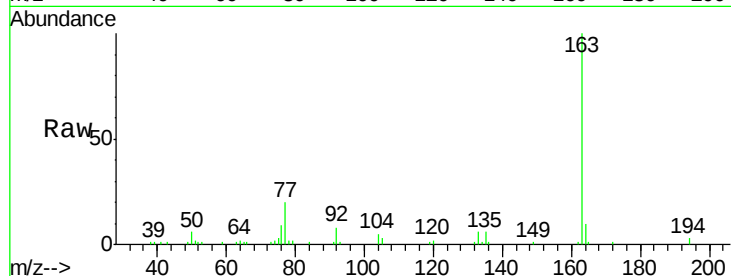


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

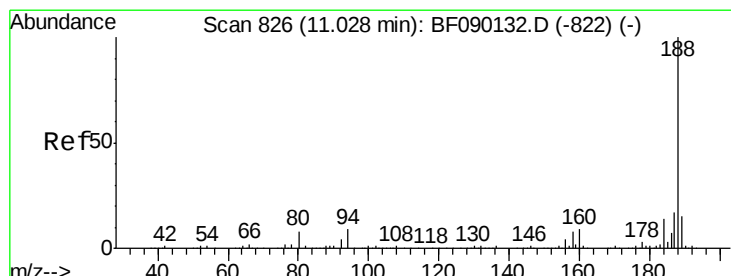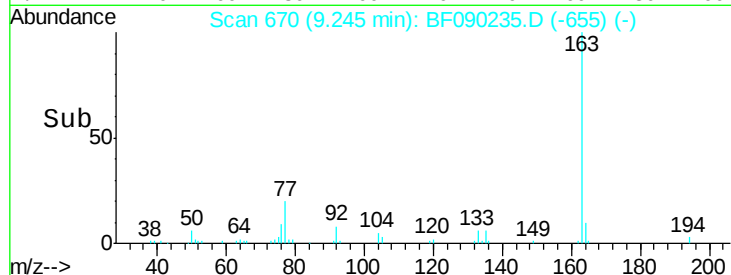
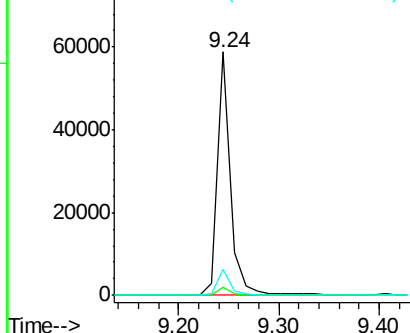



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 10.97 min Scan# 821
Delta R.T. -0.01 min
Lab File: BF090235.D
Acq: 26 Sep 2016 21:34

Tgt Ion:188 Resp: 490521
Ion Ratio Lower Upper
188 100
94 14.0 10.5 15.7
80 15.0 11.2 16.8

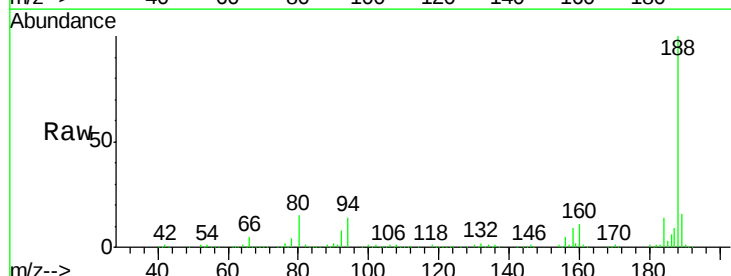

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

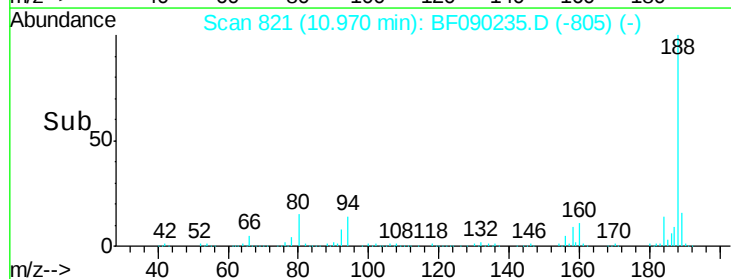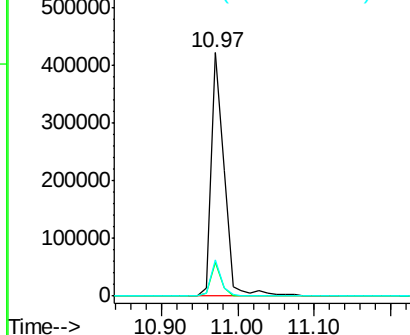

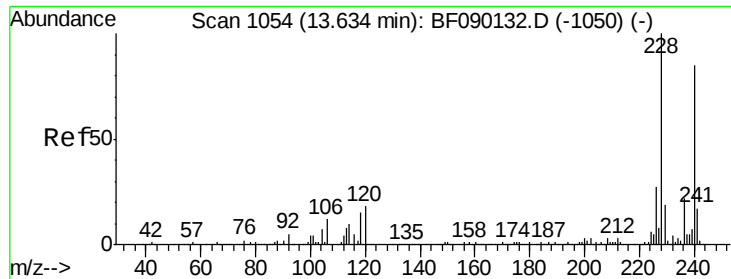

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.59 min Scan# 1050

Delta R.T. -0.01 min

Lab File: BF090235.D

Acq: 26 Sep 2016 21:34

Instrument :

BNA_F

ClientSampleId :

MW-05S-092216


Tot Ion:240 Resp: 443757

Ion Ratio Lower Upper

240 100

120 10.6 10.6 16.0#




236 26.3 21.6 32.4

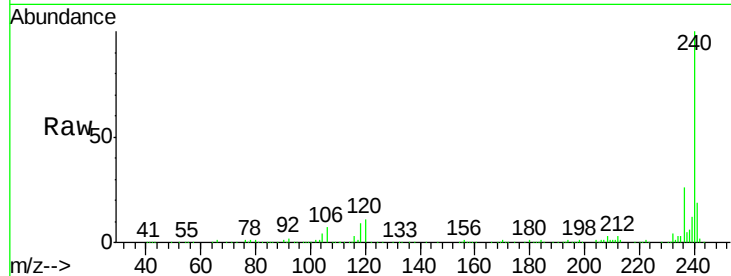

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

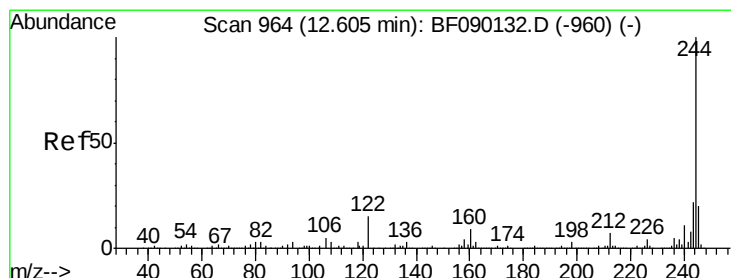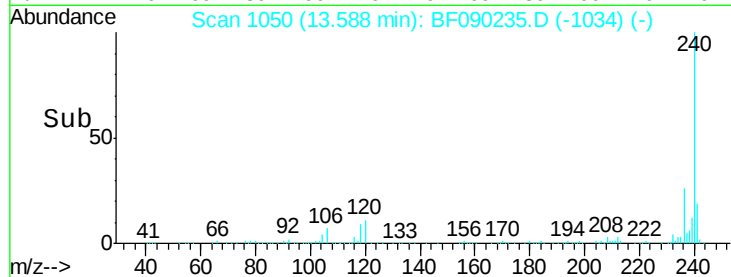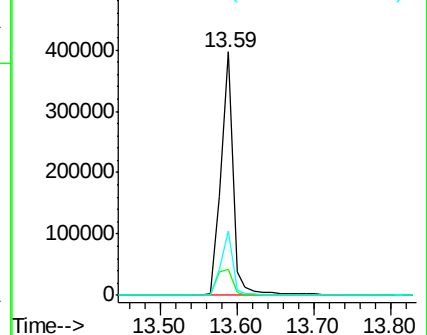

#78

Terphenyl-d14

Concen: 55.97 ng

RT: 12.56 min Scan# 960

Delta R.T. -0.00 min

Lab File: BF090235.D

Acq: 26 Sep 2016 21:34


Tgt Ion:244 Resp: 978351

Ion Ratio Lower Upper

244 100

212 7.5 5.8 8.8



122 15.5 9.4 14.0#



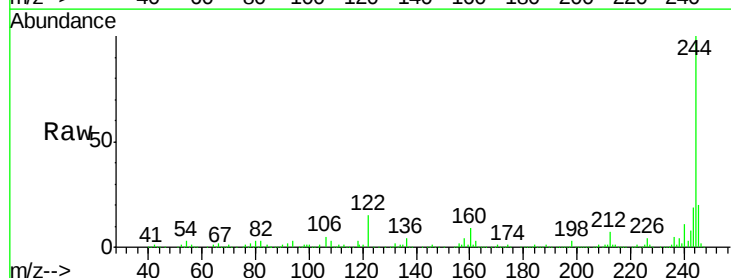


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

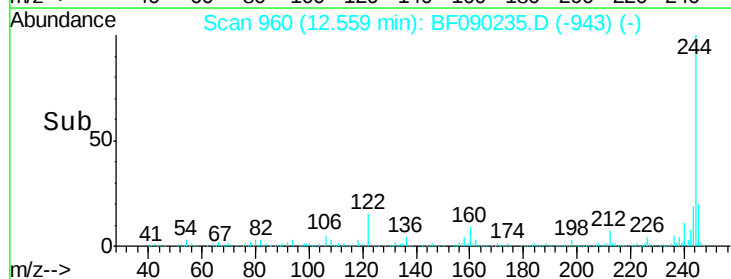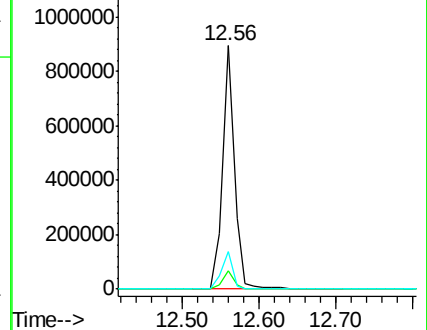

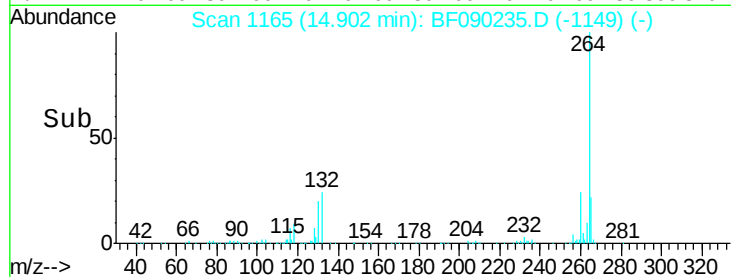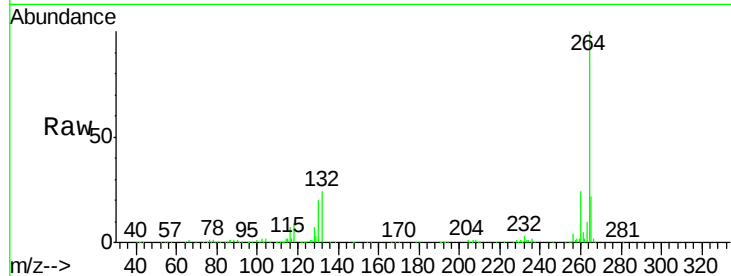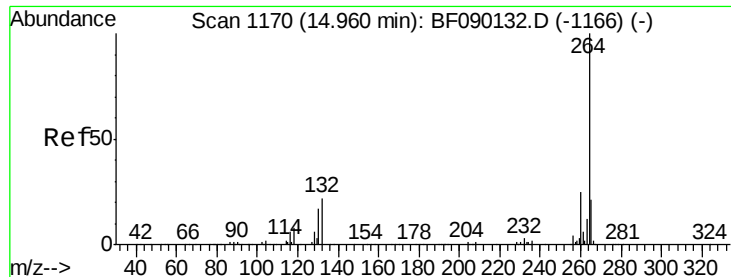

#86
Pervlene-d12
Concen: 20.00 ng
RT: 14.90 min Scan# 1165
Delta R.T. -0.01 min
Lab File: BF090235.D
Acq: 26 Sep 2016 21:34

Instrument :
BNA_F
ClientSampleId :
MW-05S-092216

Tot Ion:	264	Resp:	332902
Ion	Ratio	Lower	Upper
264	100		
260	24.1	19.5	29.3
265	22.1	17.0	25.4

