


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092616\
 Data File : BF090238.D
 Acq On : 27 Sep 2016 00:45
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 26 15:58:38 2016

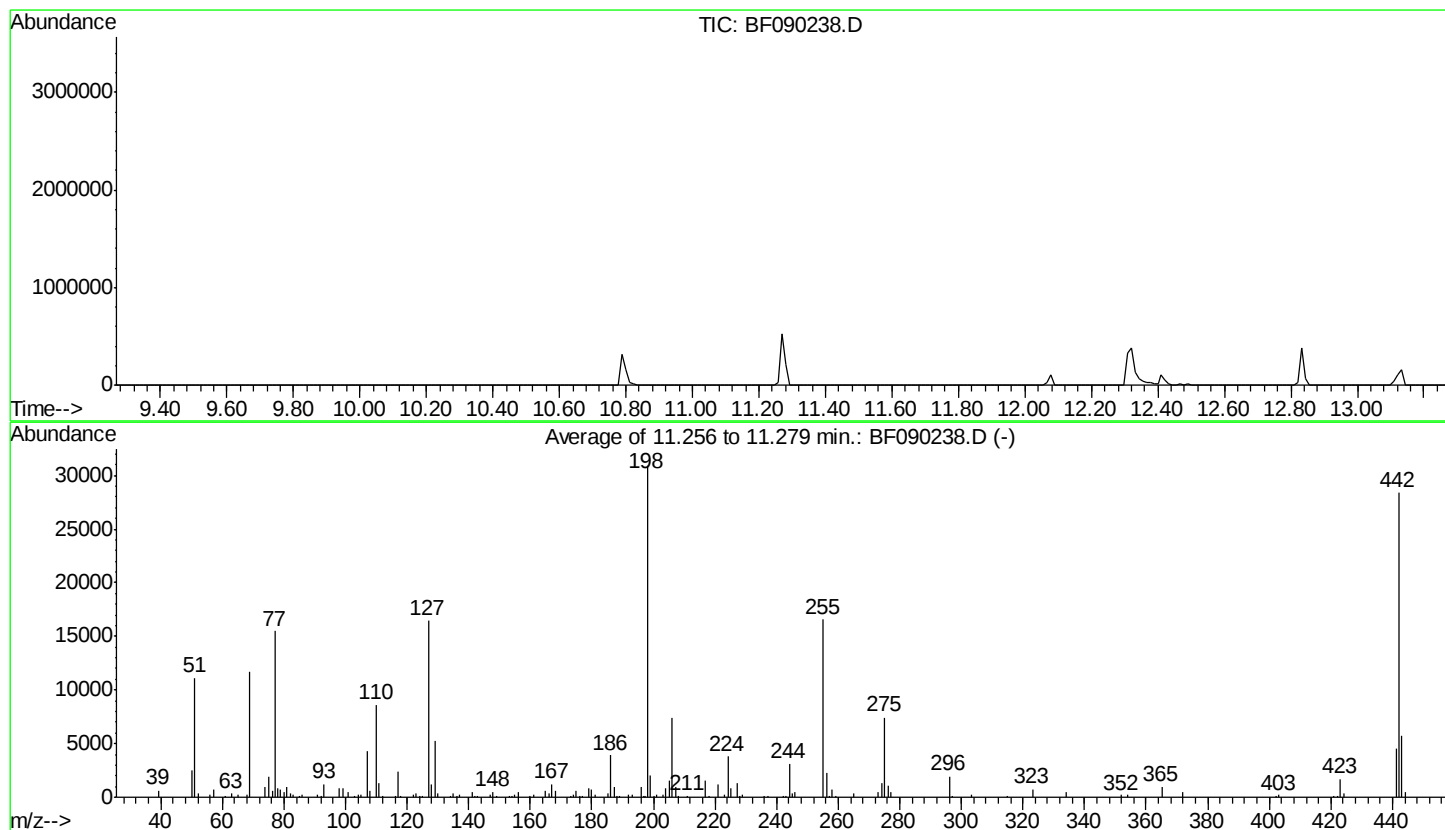

AutoFind: Scans 846, 847, 848; Background Corrected with Scan 843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	11145	PASS
68	69	0.00	2	1.7	203	PASS
69	198	0.00	100	38.0	11750	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.1	16431	PASS
197	198	0.00	2	0.5	147	PASS
198	198	100	100	100.0	30917	PASS
199	198	5	9	6.6	2050	PASS
275	198	10	60	24.1	7460	PASS
365	198	1	100	3.2	977	PASS
441	442	0.01	24	16.0	4528	PASS
442	198	50	100	91.7	28352	PASS
443	442	15	24	20.2	5713	PASS