
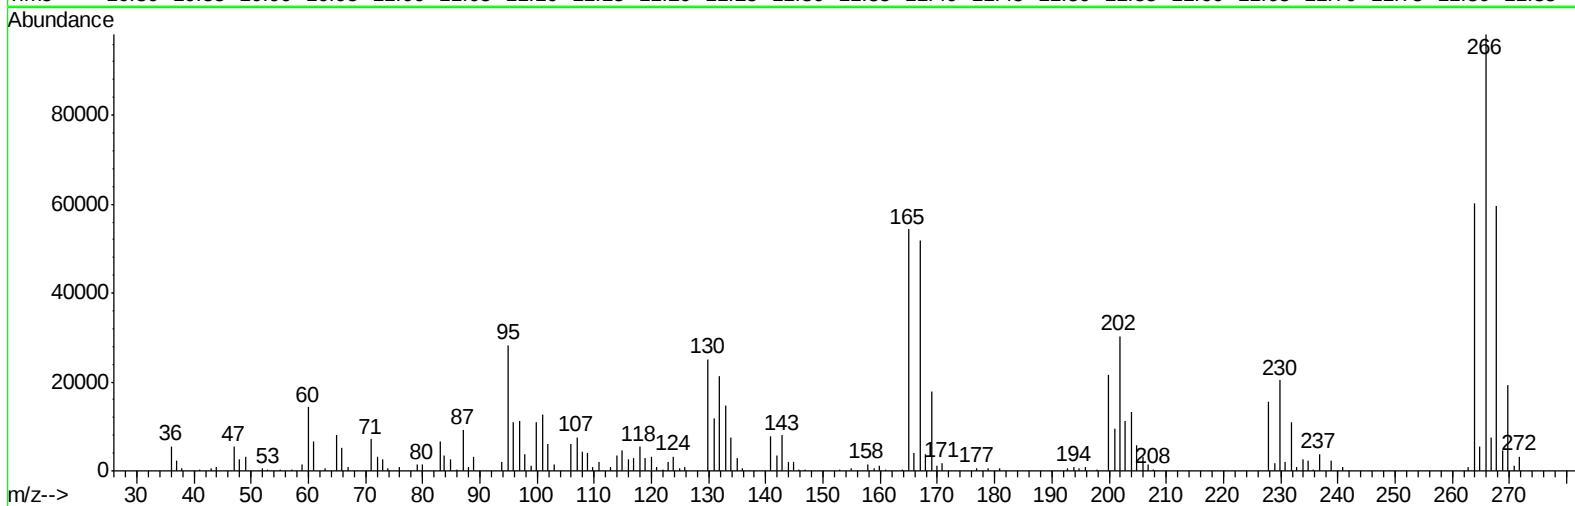


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092617\
Data File : BF098826.D
Acq On : 26 Sep 2017 12:19
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 03:57:06 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

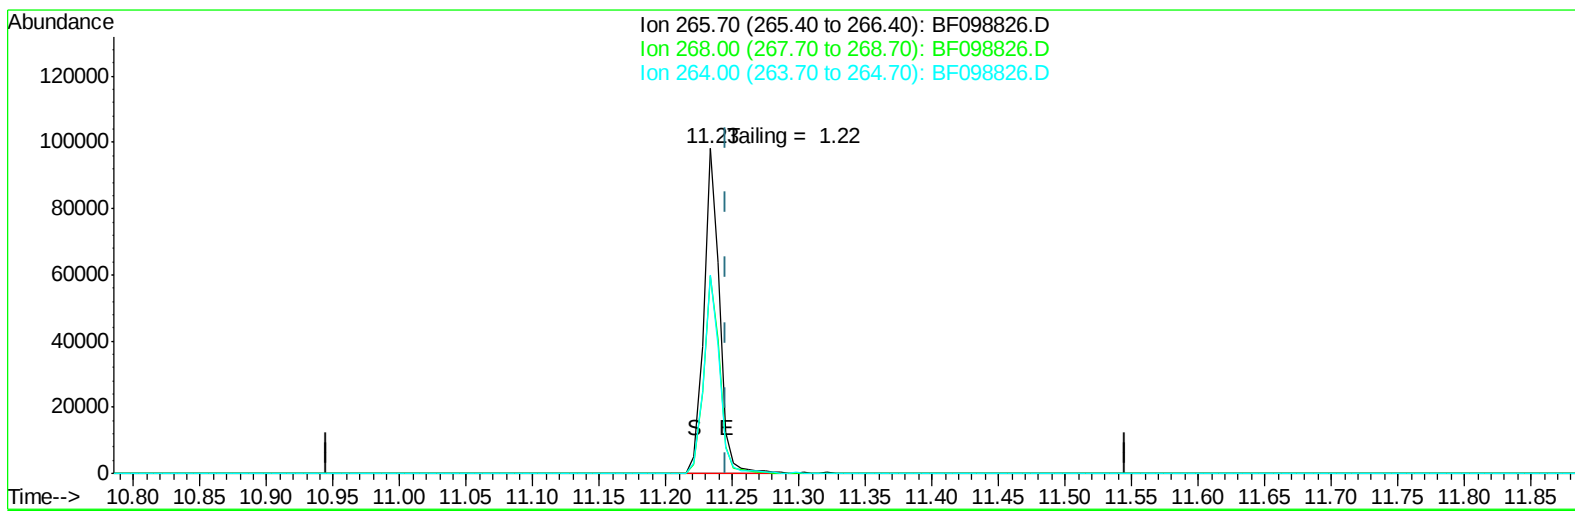

TIC: BF098826.D

(69) Pentachlorophenol (C)



11.233min (-0.012) 24876.75ng

response 79634

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.86
264.00	61.90	61.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092617\
 Data File : BF098826.D
 Acq On : 26 Sep 2017 12:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 03:57:06 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 23 13:50:58 2017
 Response via : Initial Calibration

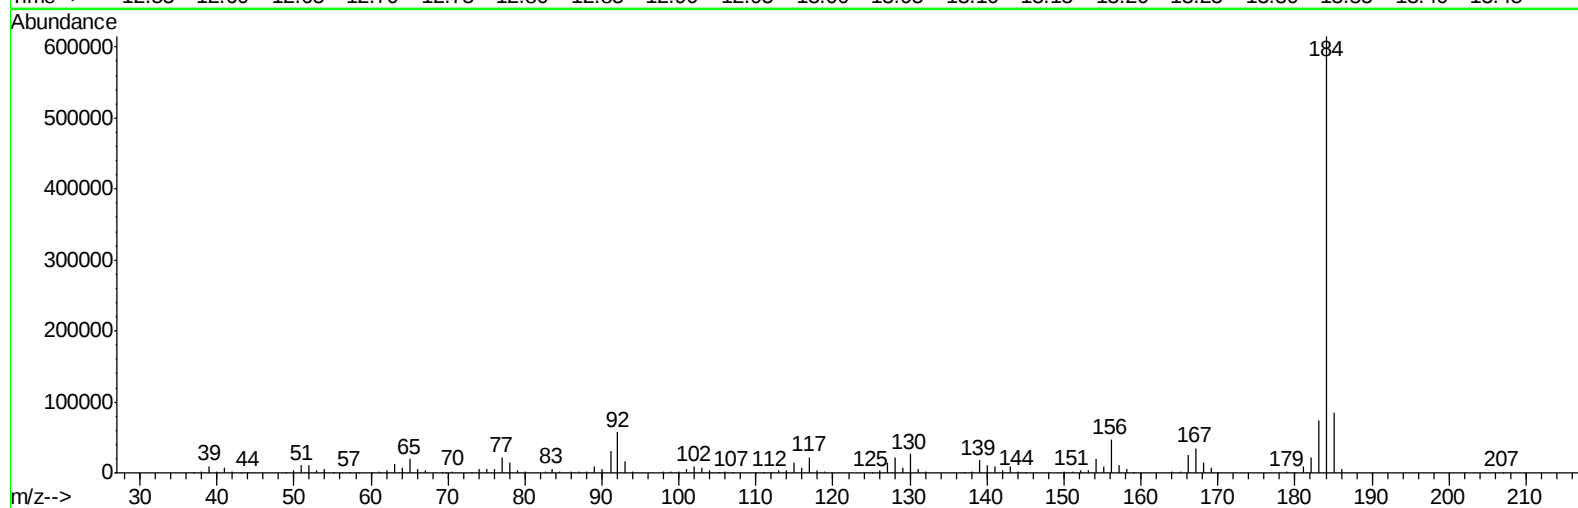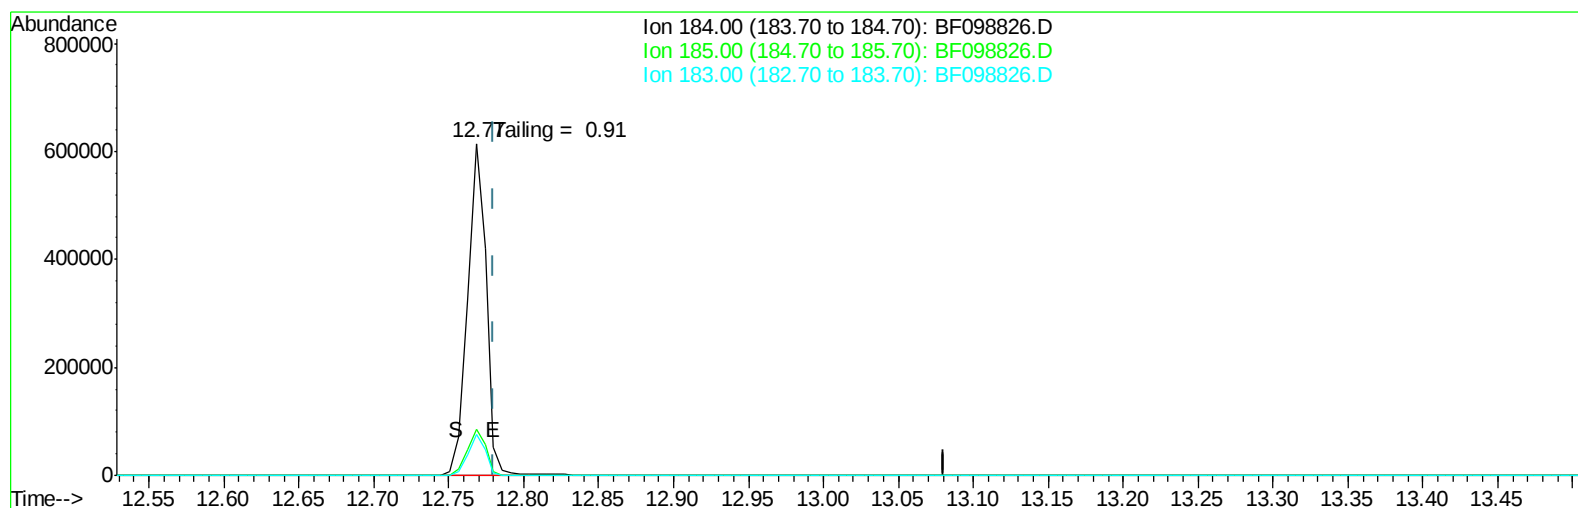

TIC: BF098826.D

(76) Benzidine

12.768min (-0.012) 0.00ng

response 536926

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.83
183.00	11.60	12.16
0.00	0.00	0.00